
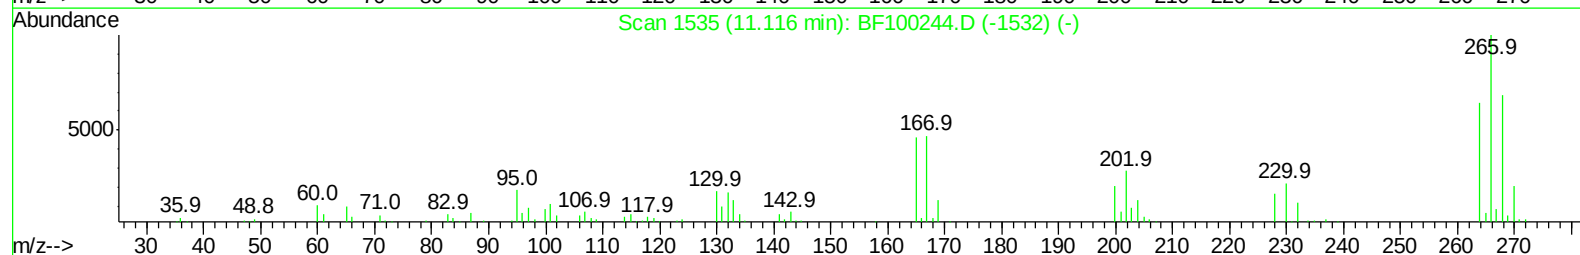
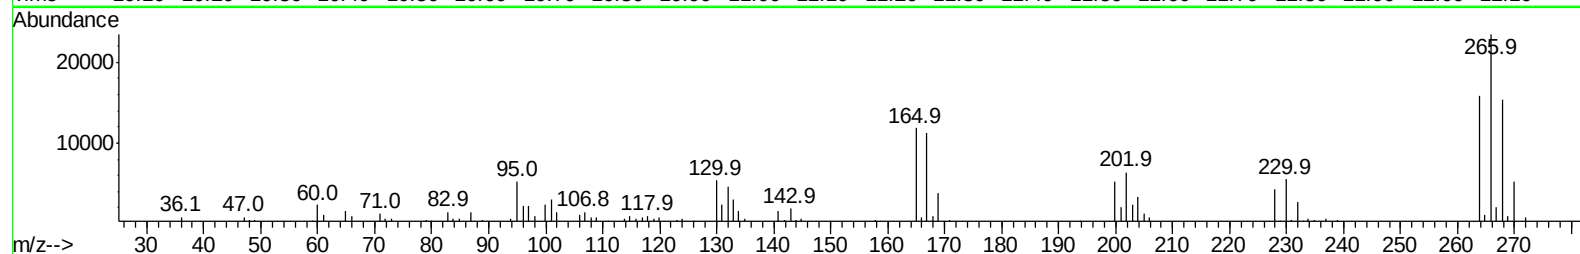


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF110617\
Data File : BF100253.D
Acq On : 6 Nov 2017 16:10
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 07 07:51:44 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF102317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 07 02:59:38 2017
Response via : Initial Calibration

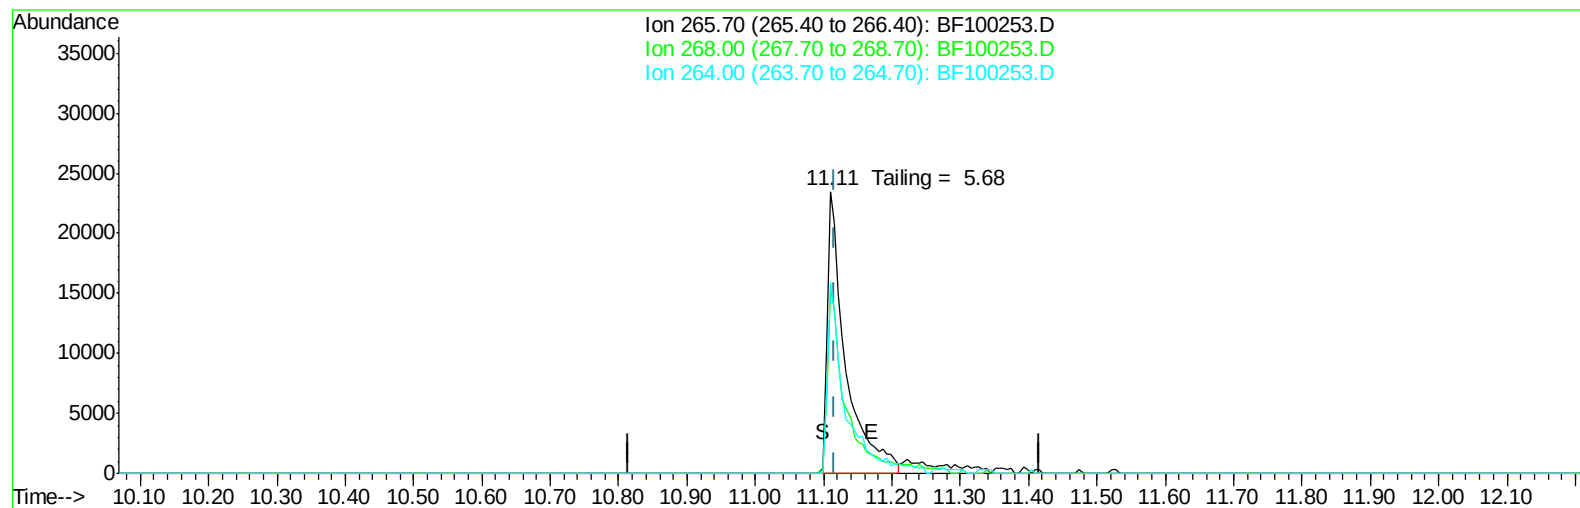

TIC: BF100253.D

(69) Pentachlorophenol (C)




11.110min (-0.006) 40607.63ng

response 44478

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	65.51
264.00	61.90	67.80
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF110617\
 Data File : BF100253.D
 Acq On : 6 Nov 2017 16:10
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 07 07:51:44 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF102317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 07 02:59:38 2017
 Response via : Initial Calibration

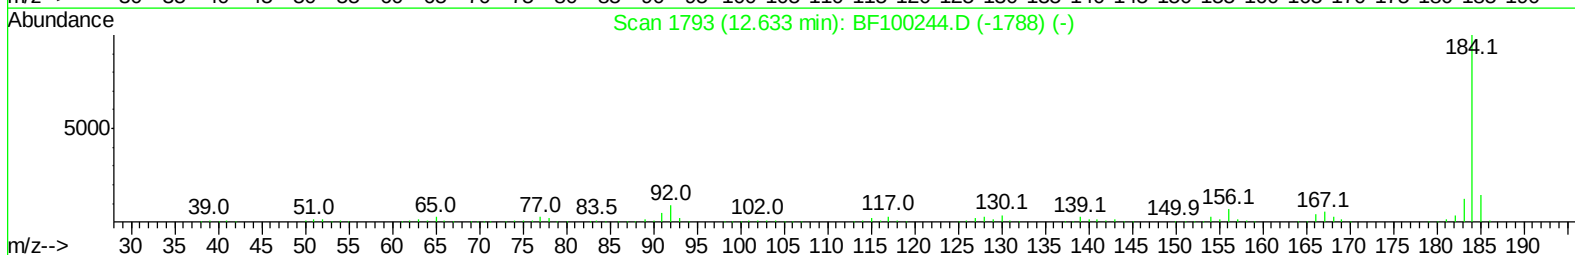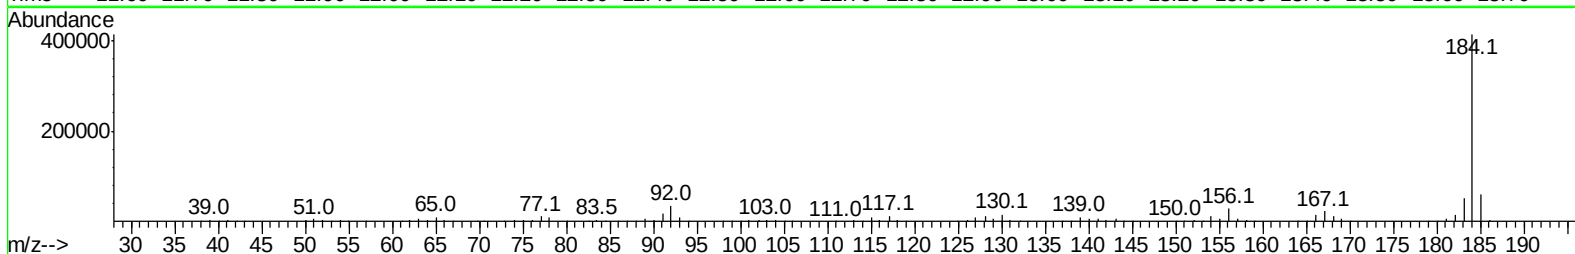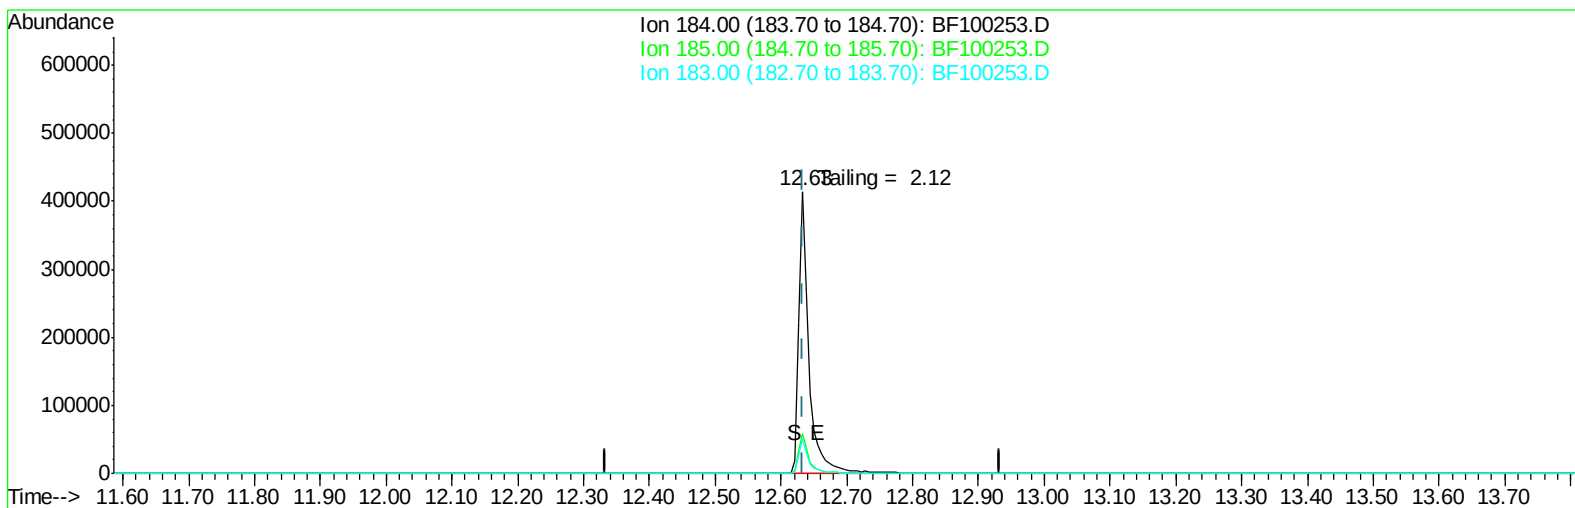

TIC: BF100253.D

(76) Benzidine

12.633min (-0.000) 0.00ng

response 449451

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.33
183.00	11.60	12.19
0.00	0.00	0.00