

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF110617\
 Data File : BF100262.D
 Acq On : 6 Nov 2017 20:27
 Operator : SJ/JU
 Sample : PB104022BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB104022BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.992	492	494	517	rBV	80860	179485	9.68%	1.289%
2	5.392	560	562	592	rBV	738658	1353938	73.04%	9.726%
3	6.410	732	735	753	rBV	923885	1319906	71.21%	9.481%
4	6.534	753	756	777	rVB	1408496	1553977	83.83%	11.163%
5	6.763	792	795	805	rBV	356907	420376	22.68%	3.020%
6	6.910	817	820	843	rBV	1153980	1206991	65.11%	8.670%
7	7.333	889	892	920	rBV	651473	854561	46.10%	6.139%
8	8.039	1010	1012	1033	rBV	466687	600935	32.42%	4.317%
9	9.110	1191	1194	1209	rBV	2043918	1853635	100.00%	13.315%
10	9.792	1307	1310	1324	rBV2	701924	695584	37.53%	4.997%
11	10.592	1443	1446	1466	rBV	785430	904120	48.78%	6.495%
12	11.286	1561	1564	1577	rBV	653315	678136	36.58%	4.871%
13	12.868	1829	1833	1842	rBV	1605234	1556579	83.97%	11.181%
14	13.945	2013	2016	2028	rBV	354168	379347	20.47%	2.725%
15	15.409	2261	2265	2278	rBV	233785	363714	19.62%	2.613%


Sum of corrected areas: 13921284

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF110617\
Data File : BF100262.D
Acq On : 6 Nov 2017 20:27
Operator : SJ/JU
Sample : PB104022BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB104022BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

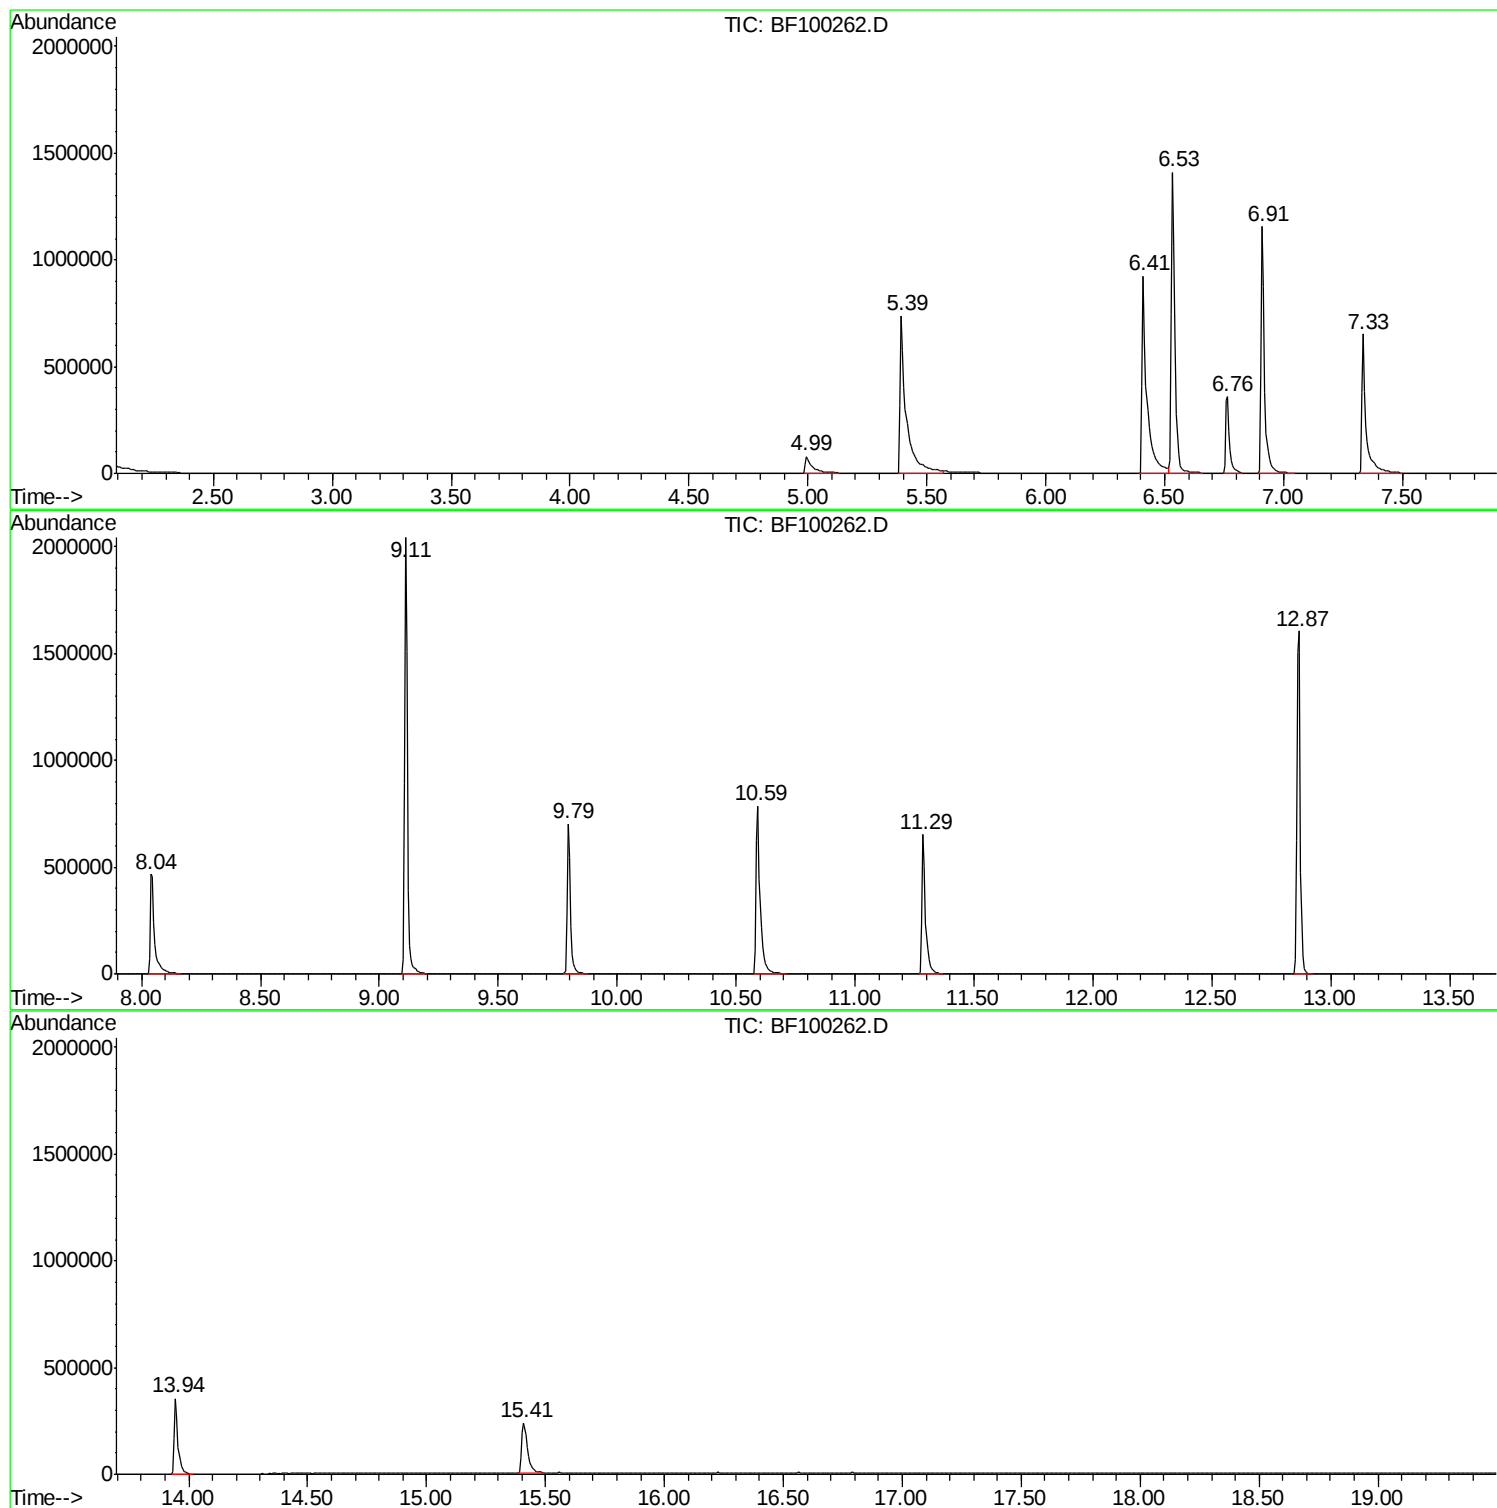

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF110617\
Data File : BF100262.D
Acq On : 6 Nov 2017 20:27
Operator : SJ/JU
Sample : PB104022BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB104022BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.99	8.54 ng	179485	1,4-Dichlorobenzene-d4	6.76

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56
2		3-Hexanol	102	C6H14O	000623-37-0	28
3		Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9
4		Guanidine	59	CH5N3	000113-00-8	9
5		Butane, 1-ethoxy-	102	C6H14O	000628-81-9	9

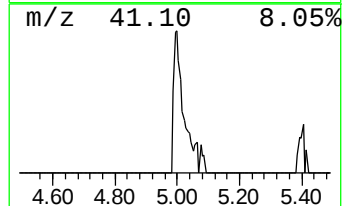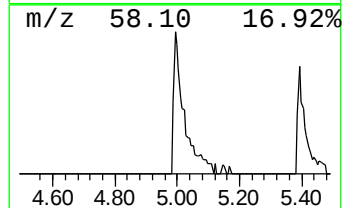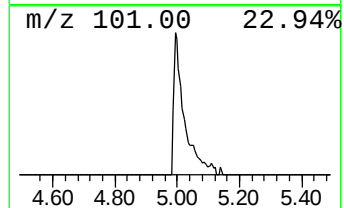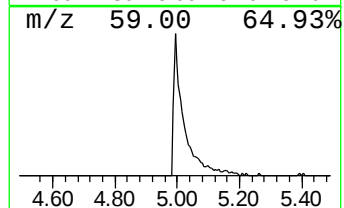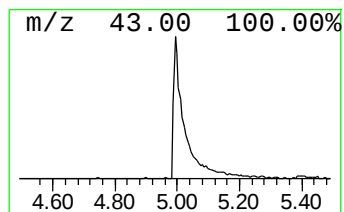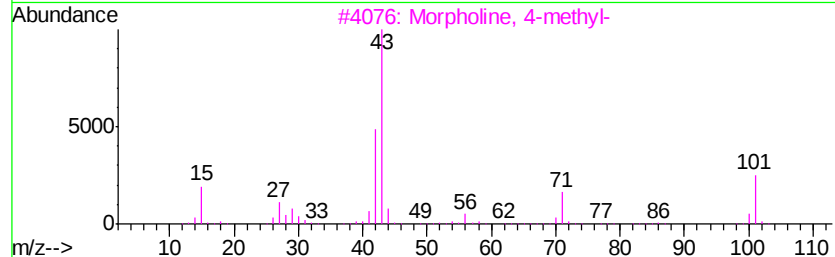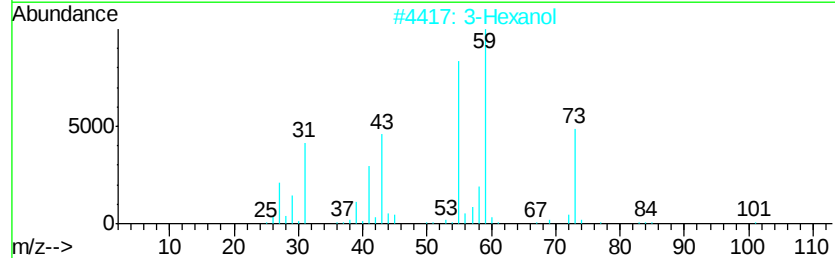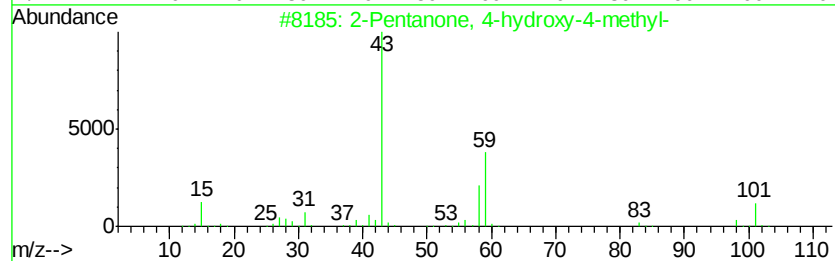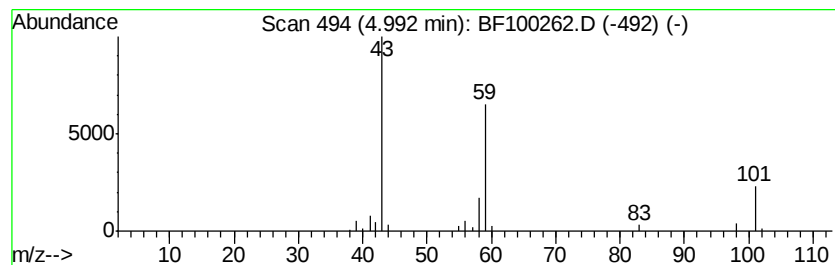

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF110617\
Data File : BF100262.D
Acq On : 6 Nov 2017 20:27
Operator : SJ/JU
Sample : PB104022BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB104022BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.53 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.53	73.93 ng	1553980	1,4-Dichlorobenzene-d4	6.76

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	38
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	25
3		1H-Indazole, 7-methyl-	132	C8H8N2	1000316-00-7	10
4		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	9
5		Xenon	132	Xe	007440-63-3	9

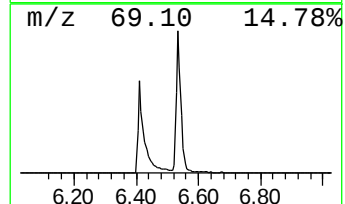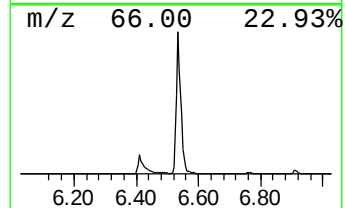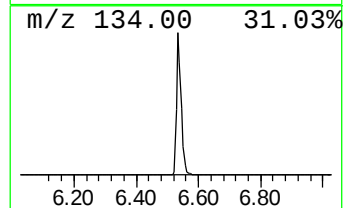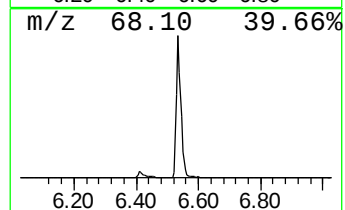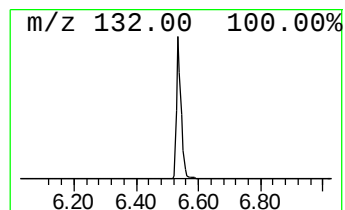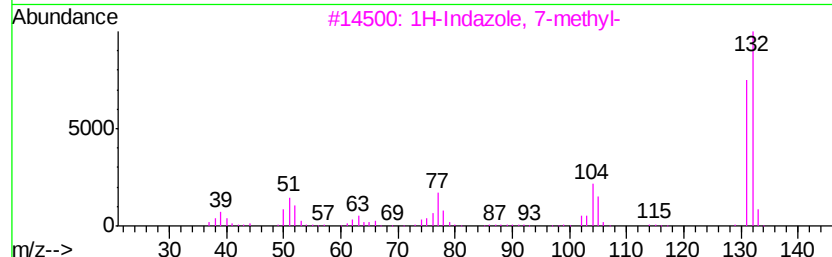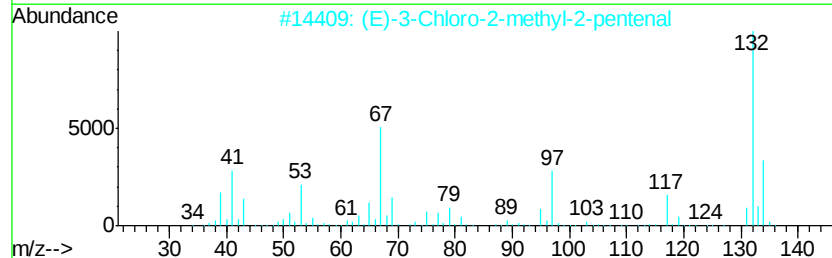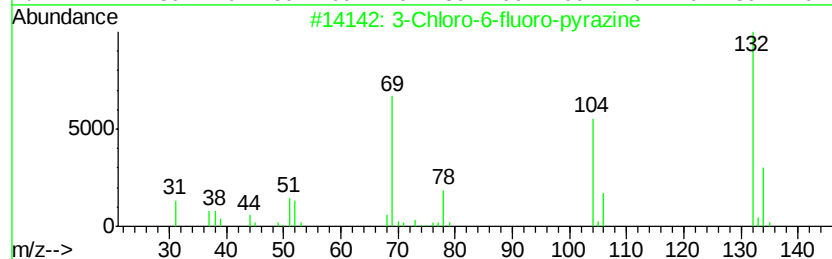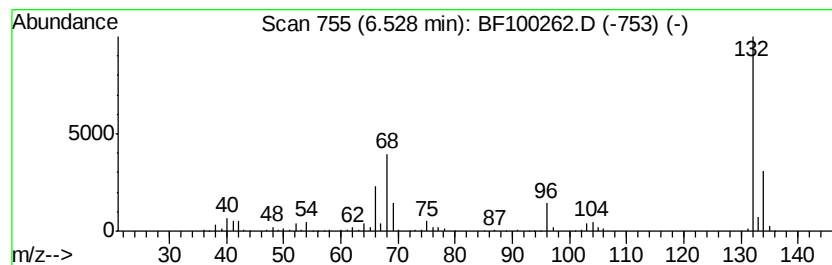

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF110617\
Data File : BF100262.D
Acq On : 6 Nov 2017 20:27
Operator : SJ/JU
Sample : PB104022BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB104022BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	4.99	8.5	ng	179485	1	6.76	420376	20.0
unknown6.53	6.53	73.9	ng	1553980	1	6.76	420376	20.0