


Data Path : Z:\HPCHEM1\BNA_F\Data\BF110617\
 Data File : BF100243.D
 Acq On : 6 Nov 2017 10:10
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 07 14:09:40 2017

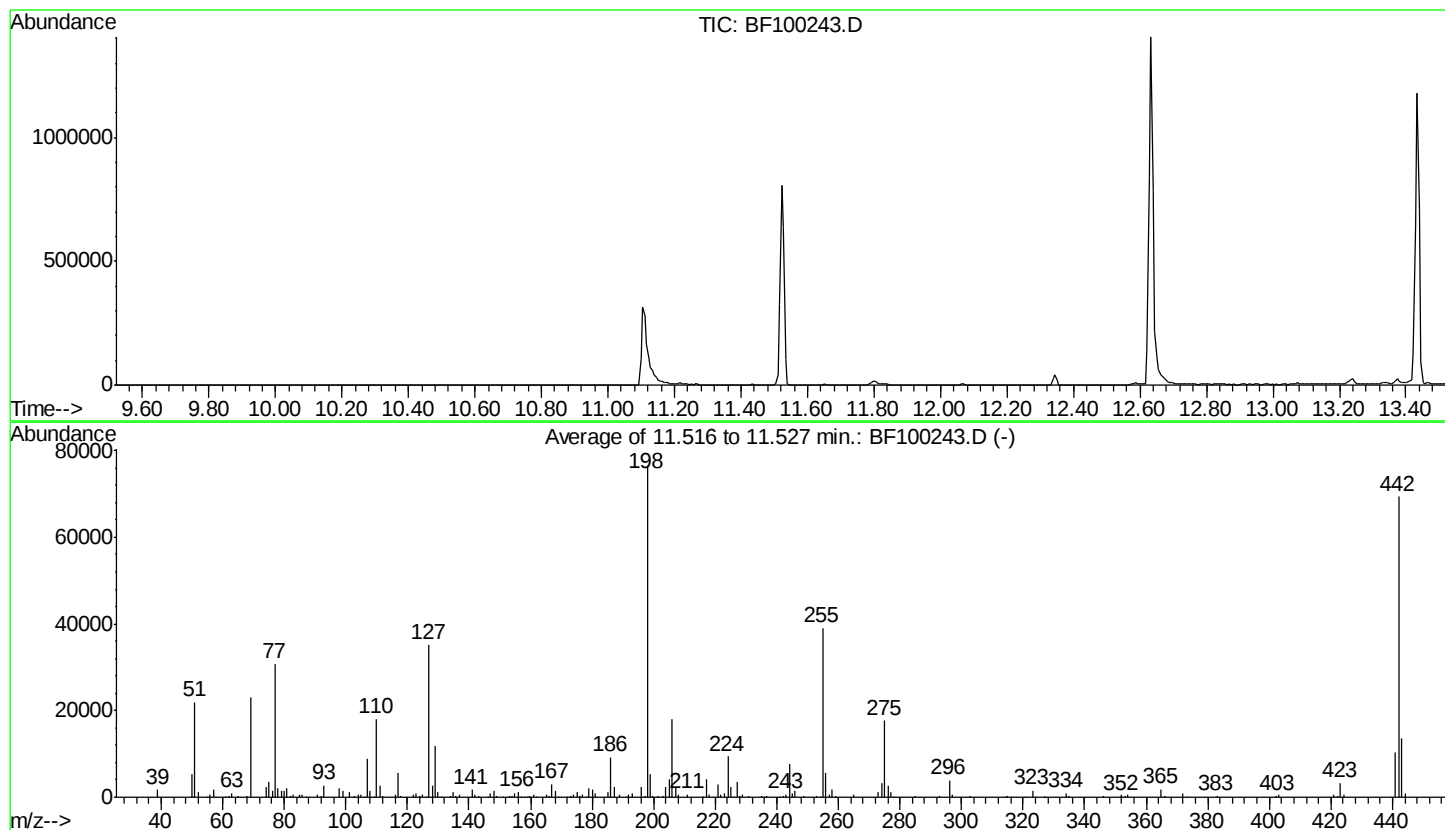

AutoFind: Scans 1603, 1604, 1605; Background Corrected with Scan 1598

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.7	21936	PASS
68	69	0.00	2	1.7	385	PASS
69	198	0.00	100	30.3	23168	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.0	35242	PASS
197	198	0.00	2	0.5	392	PASS
198	198	100	100	100.0	76538	PASS
199	198	5	9	7.1	5401	PASS
275	198	10	60	23.0	17622	PASS
365	198	1	100	2.4	1827	PASS
441	443	0.01	100	76.6	10431	PASS
442	198	50	100	90.6	69344	PASS
443	442	15	24	19.6	13626	PASS