


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110624\
Data File : BF140252.D
Acq On : 06 Nov 2024 12:15
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110524.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Nov 05 16:47:56 2024

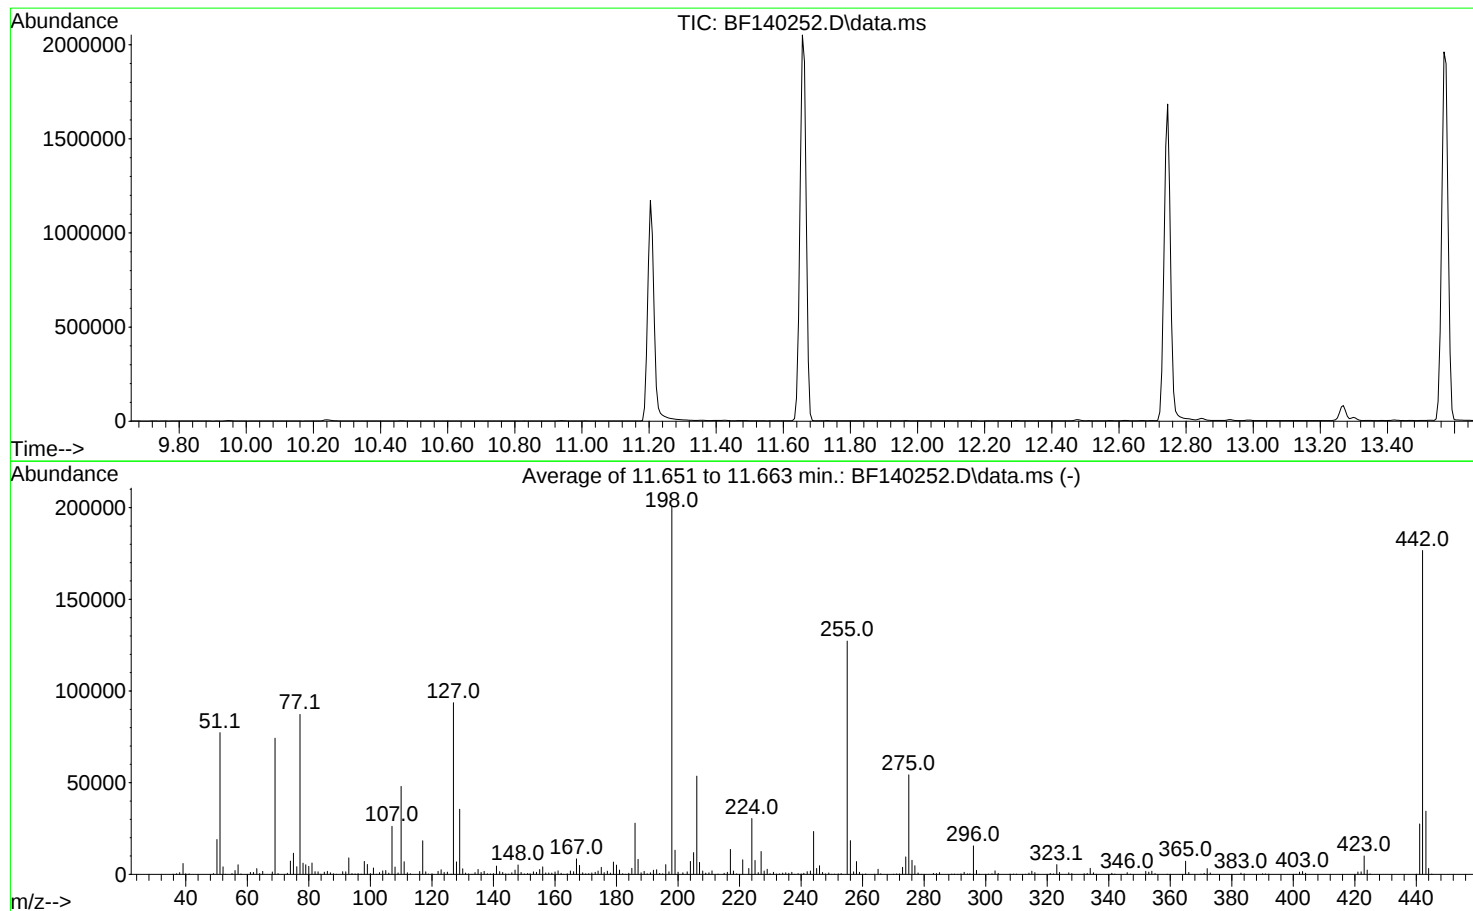




AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.6	77352	PASS
68	69	0.00	2	1.7	1286	PASS
69	198	0.00	100	37.0	74275	PASS
70	69	0.00	2	0.6	481	PASS
127	198	10	80	46.7	93603	PASS
197	198	0.00	2	0.7	1398	PASS
198	198	100	100	100.0	200619	PASS
199	198	5	9	6.6	13208	PASS
275	198	10	60	27.1	54301	PASS
365	198	1	100	3.6	7184	PASS
441	198	0.01	100	13.7	27466	PASS
442	442	50	100	100.0	176595	PASS
443	442	15	24	19.5	34512	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110624\
Data File : BF140252.D
Acq On : 06 Nov 2024 12:15
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 07 01:55:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 05 16:47:56 2024
Response via : Initial Calibration

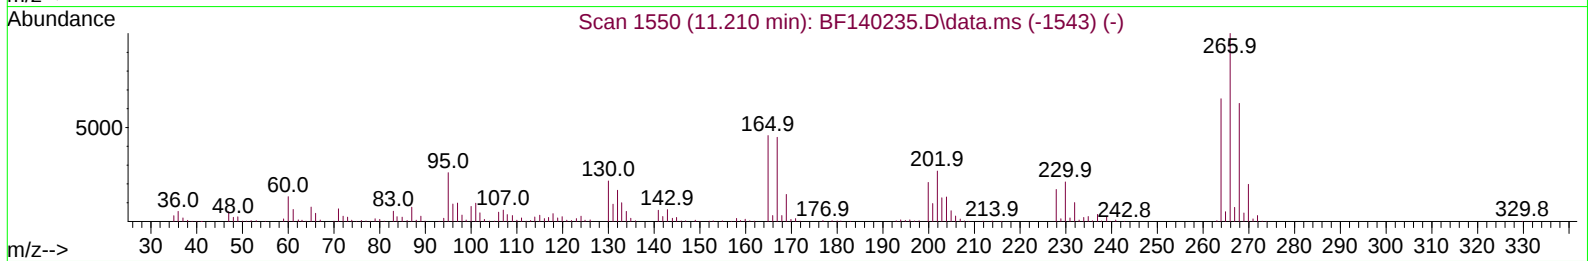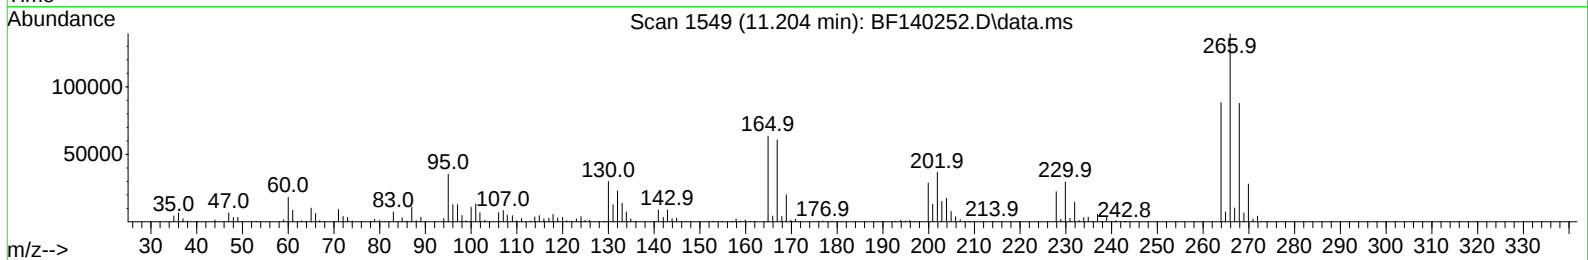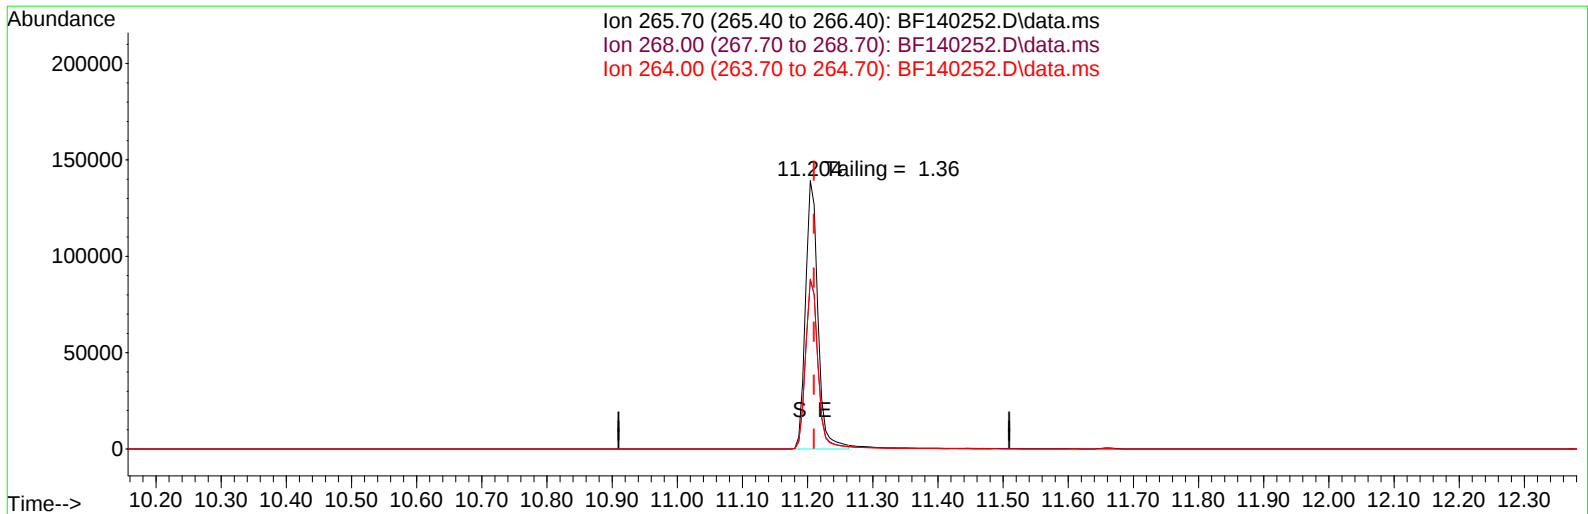

TIC: BF140252.D\data.ms

(70) Pentachlorophenol (C)

11.204min (-0.006) 35384.38 ng




response 191474

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.80	62.99
264.00	65.30	63.40
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110624\
Data File : BF140252.D
Acq On : 06 Nov 2024 12:15
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 07 01:55:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 05 16:47:56 2024
Response via : Initial Calibration

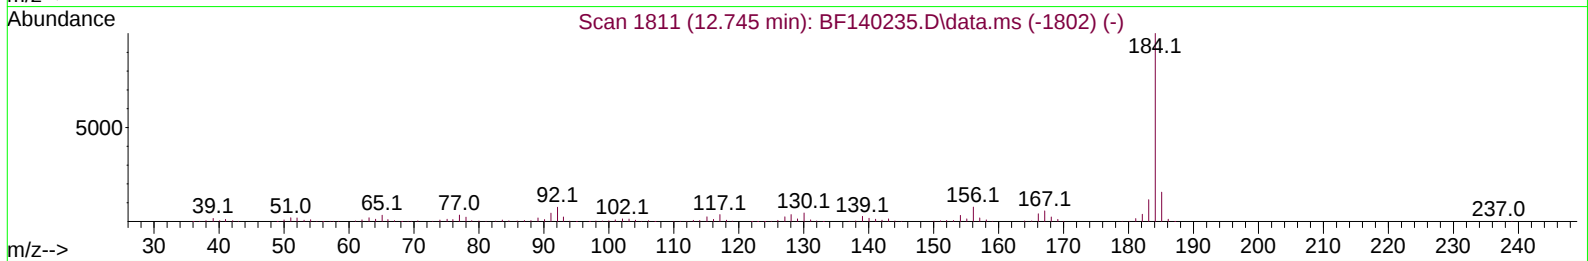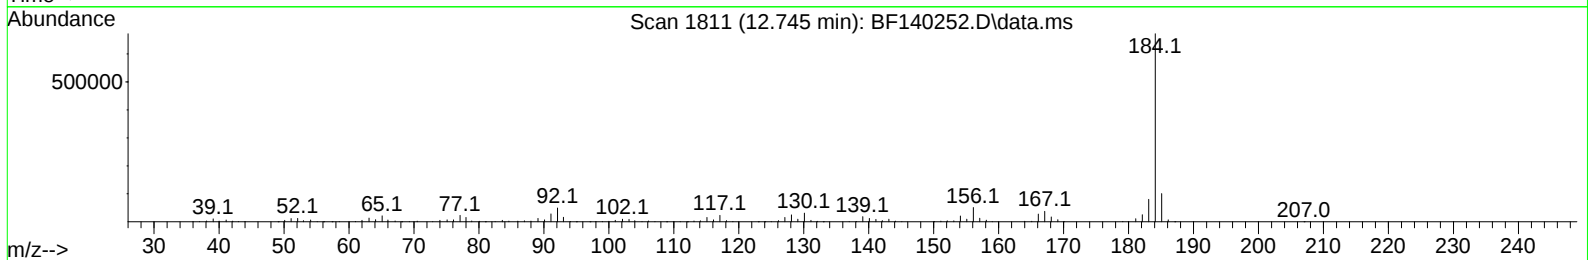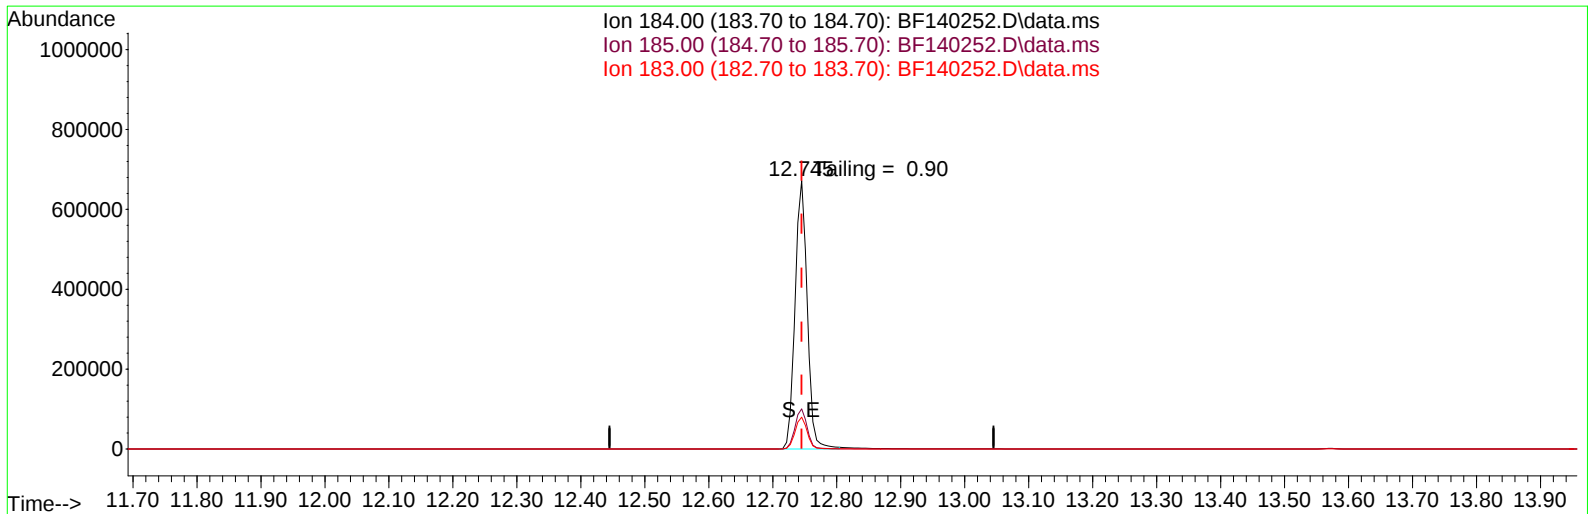

TIC: BF140252.D\data.ms

(77) Benzidine

12.745min (+ 0.000) 79884.52 ng

response 902769

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.60	14.96
183.00	11.60	11.90
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/6/2024	BNA_F	<u>BF140252.D</u>
Compound Name	Response	Retention Time
DDT	500910	13.574
DDD	24423	13.269
DDE	1323	12.933
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
25746	526656	4.89

Instrument :
BNA_F
ClientSampleId :
DFTPP