
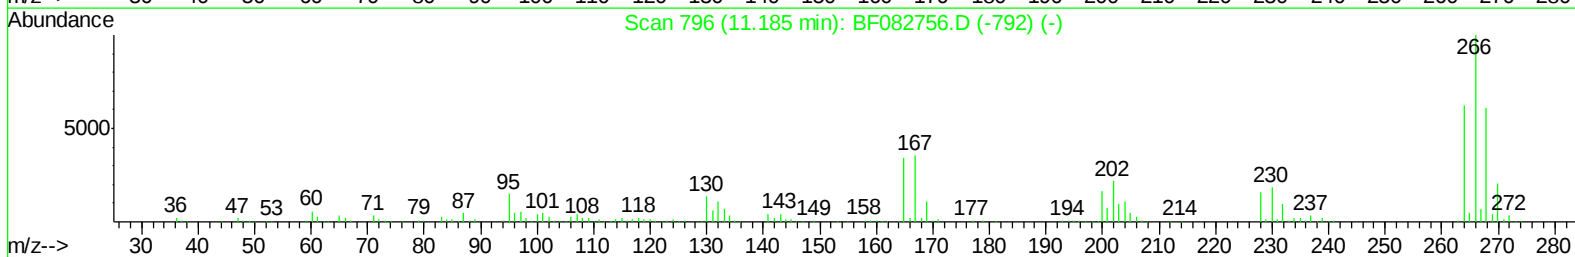
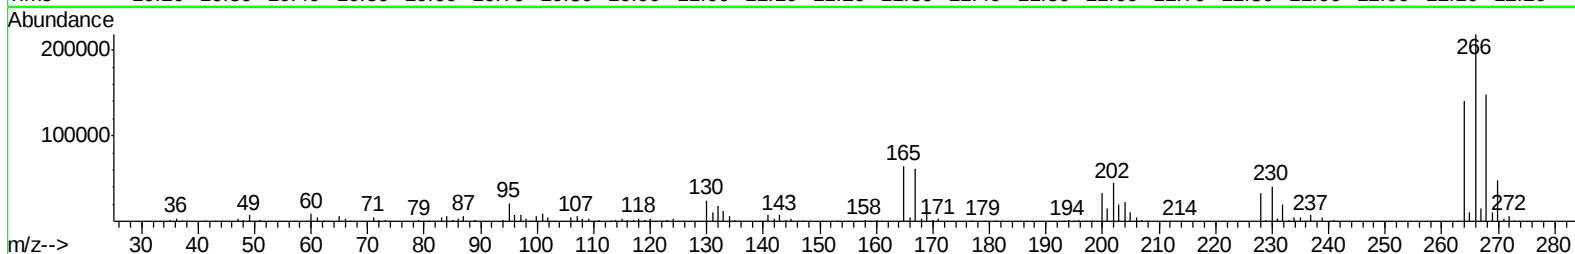


Data Path : Z:\HPCHEM1\BNA F\Data\BF110715\
Data File : BF082751.D
Acq On : 6 Nov 2015 9:51
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 06 17:53:38 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 06 14:39:58 2015
Response via : Initial Calibration

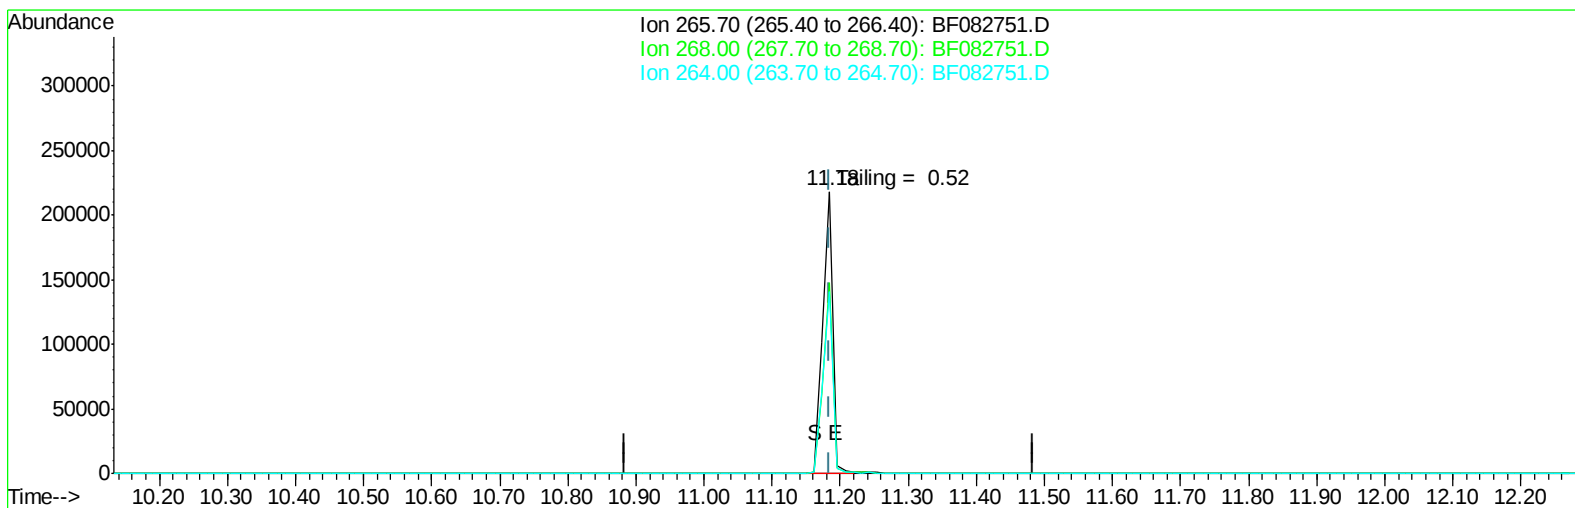

TIC: BF082751.D

(69) Pentachlorophenol (C)




11.185min (+0.000) 0.00ng

response 227843

Ion	Exp%	Act%
265.70	100	100
268.00	63.80	67.69
264.00	63.20	64.64
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF110715\
Data File : BF082751.D
Acq On : 6 Nov 2015 9:51
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 06 17:53:38 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 06 14:39:58 2015
Response via : Initial Calibration

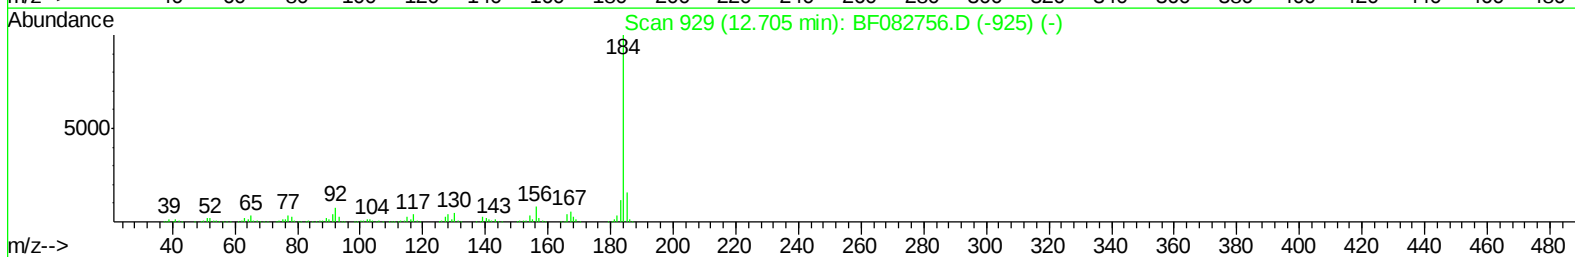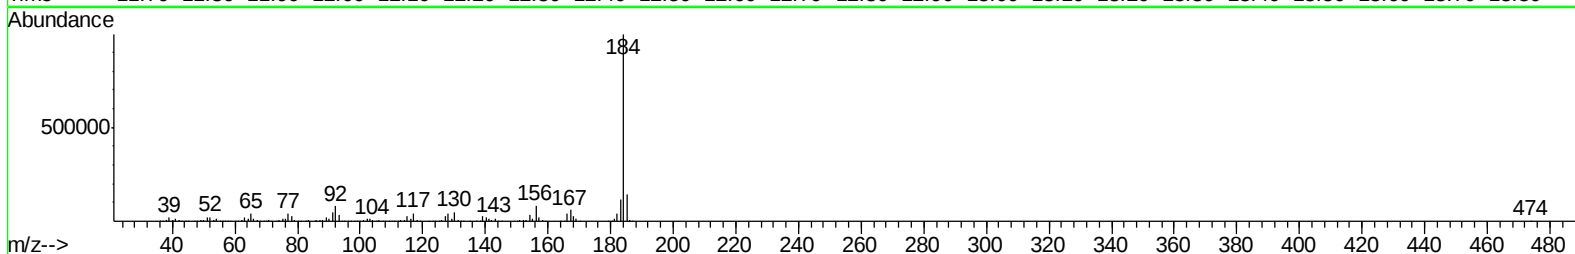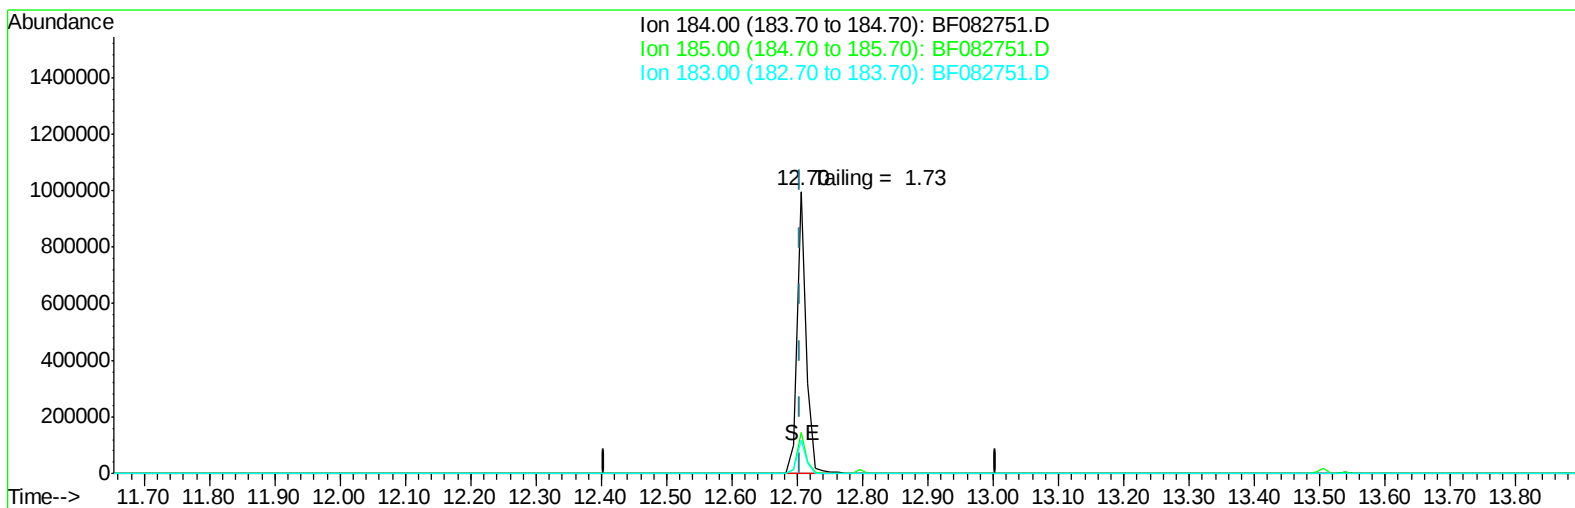

TIC: BF082751.D

(76) Benzidine

12.705min (+0.000) 0.00ng

response 996388

Ion	Exp%	Act%
184.00	100	100
185.00	15.00	14.64
183.00	12.00	12.00
0.00	0.00	0.00