


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF110715\
 Data File : BF082751.D
 Acq On : 6 Nov 2015 9:51
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Nov 07 02:32:49 2015

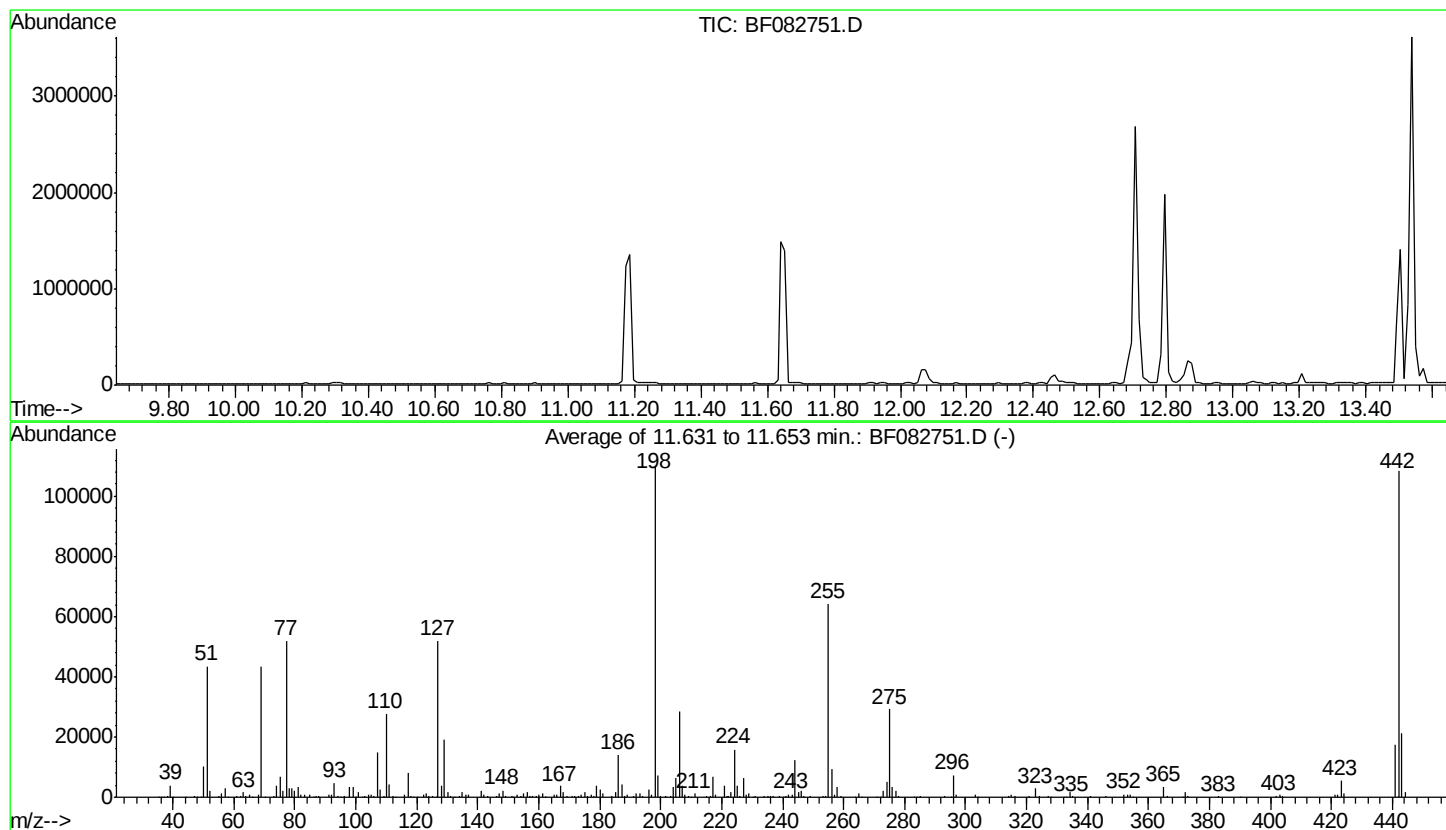

AutoFind: Scans 835, 836, 837; Background Corrected with Scan 832

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.5	43503	PASS
68	69	0.00	2	1.8	761	PASS
69	198	0.00	100	39.4	43368	PASS
70	69	0.00	2	0.4	159	PASS
127	198	10	80	47.2	52003	PASS
197	198	0.00	2	0.8	875	PASS
198	198	100	100	100.0	110144	PASS
199	198	5	9	6.7	7344	PASS
275	198	10	60	26.5	29152	PASS
365	198	1	100	3.2	3537	PASS
441	442	0.01	24	16.2	17621	PASS
442	198	50	100	98.6	108549	PASS
443	442	15	24	19.5	21217	PASS