


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF110715\
 Data File : BF082761.D
 Acq On : 6 Nov 2015 15:07
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Nov 07 02:32:49 2015

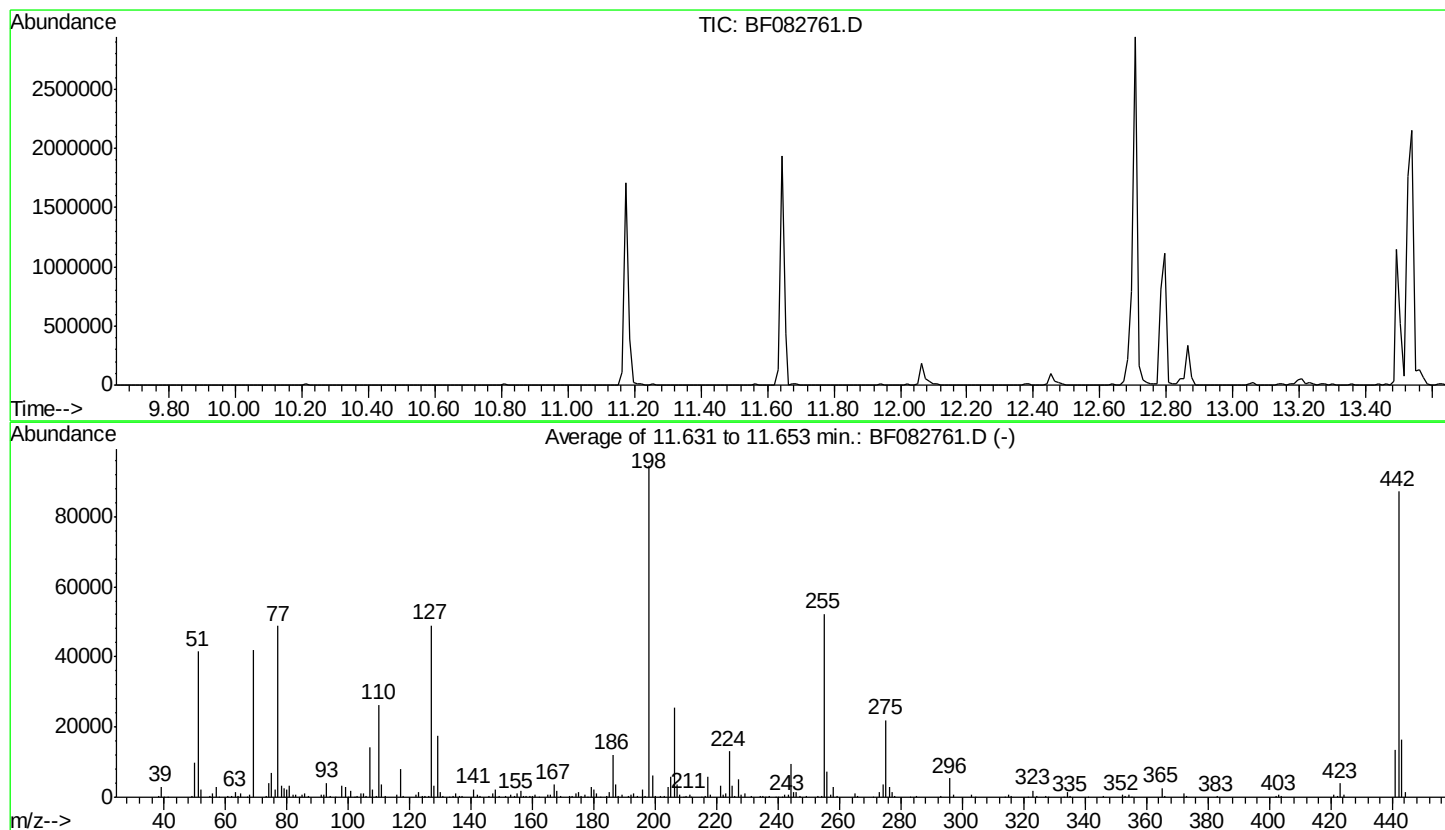

AutoFind: Scans 835, 836, 837; Background Corrected with Scan 832

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.9	41452	PASS
68	69	0.00	2	1.4	599	PASS
69	198	0.00	100	44.4	42000	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.8	48929	PASS
197	198	0.00	2	0.5	519	PASS
198	198	100	100	100.0	94493	PASS
199	198	5	9	6.5	6142	PASS
275	198	10	60	23.2	21919	PASS
365	198	1	100	2.8	2649	PASS
441	442	0.01	24	15.7	13653	PASS
442	198	50	100	92.2	87097	PASS
443	442	15	24	19.1	16594	PASS