


Data Path : Z:\HPCHEM1\BNA F\DATA\BF110716\
 Data File : BF091049.D
 Acq On : 7 Nov 2016 12:15
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 08 12:59:29 2016

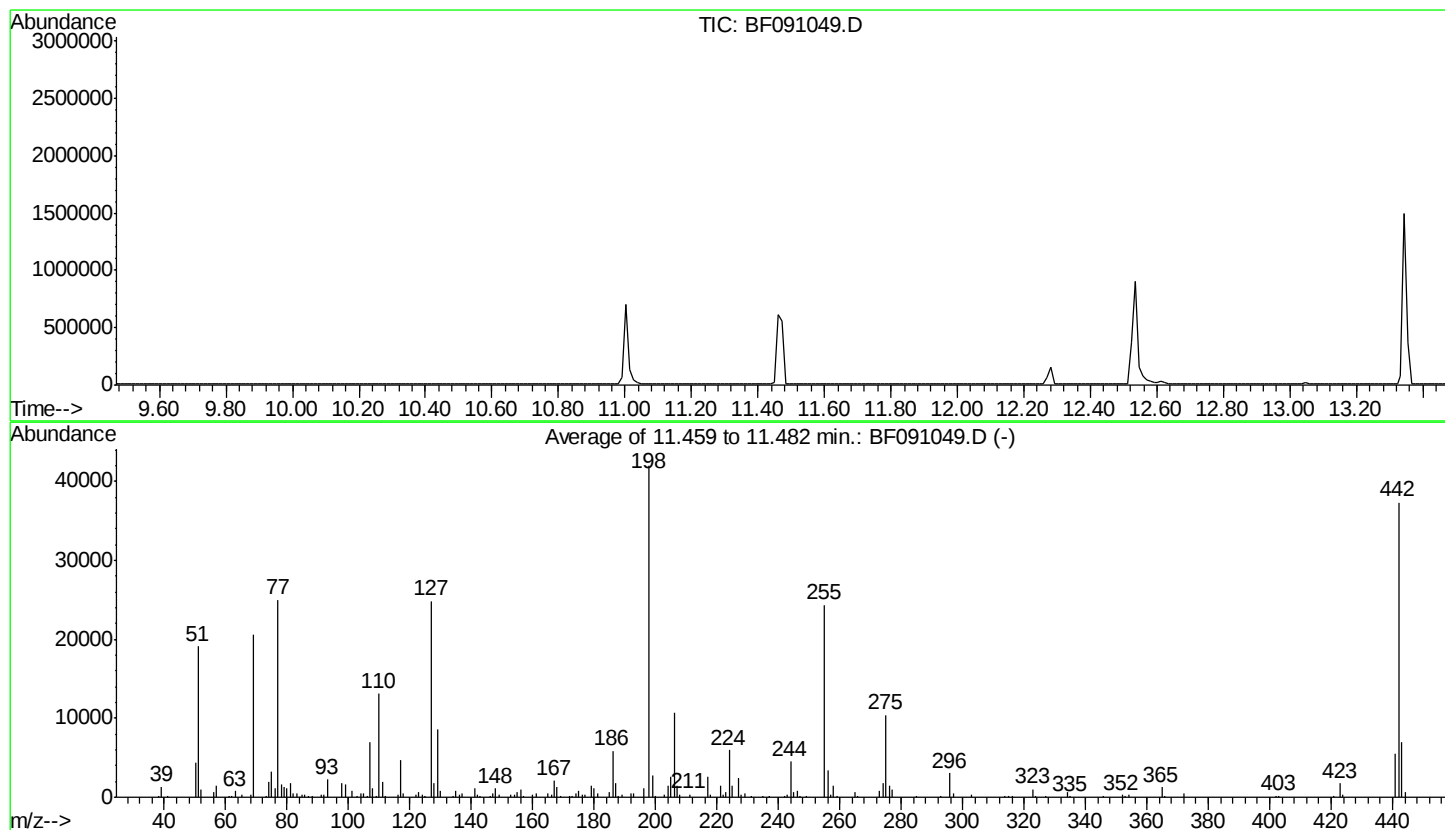

AutoFind: Scans 855, 856, 857; Background Corrected with Scan 851

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.5	19141	PASS
68	69	0.00	2	1.3	278	PASS
69	198	0.00	100	49.1	20615	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	59.1	24853	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	42027	PASS
199	198	5	9	6.7	2808	PASS
275	198	10	60	24.8	10442	PASS
365	198	1	100	3.1	1283	PASS
441	442	0.01	24	14.8	5536	PASS
442	198	50	100	88.9	37370	PASS
443	442	15	24	18.6	6968	PASS