
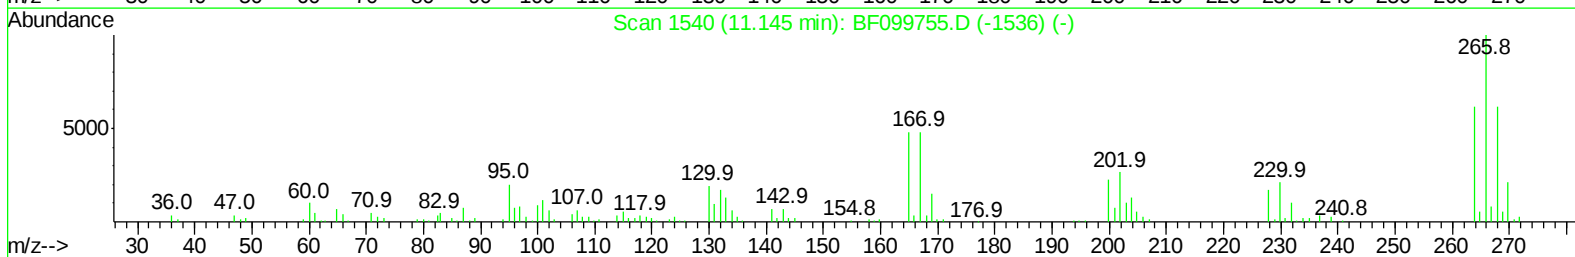
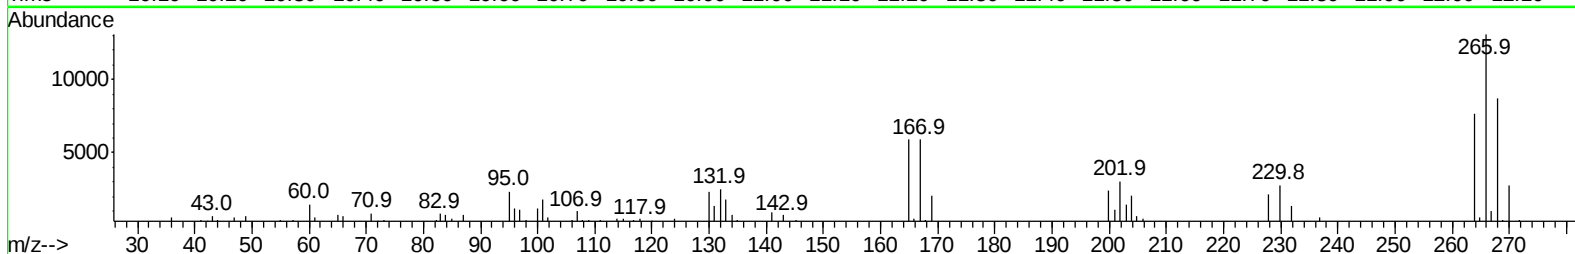


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF110717\
Data File : BF100276.D
Acq On : 7 Nov 2017 11:35
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 07 23:56:14 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF102317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 07 02:59:38 2017
Response via : Initial Calibration

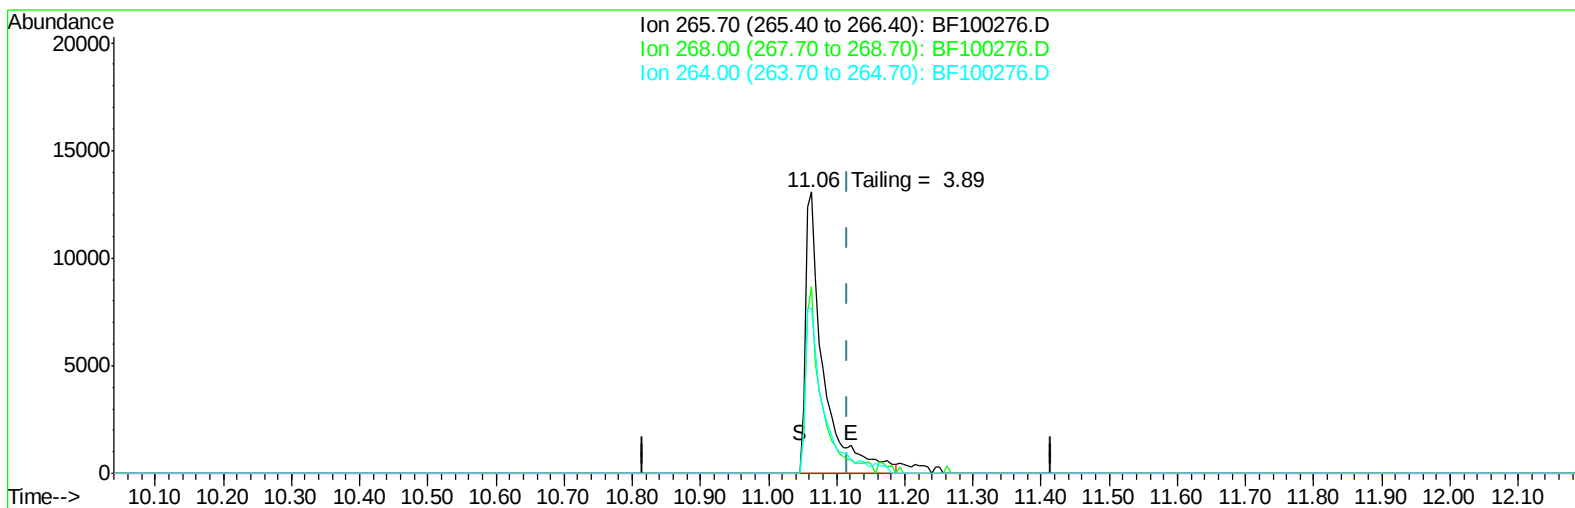

TIC: BF100276.D

(69) Pentachlorophenol (C)




11.063min (-0.053) 37347.65ng

response 24235

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	66.57
264.00	61.90	58.74
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF110717\
Data File : BF100276.D
Acq On : 7 Nov 2017 11:35
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 07 23:56:14 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF102317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 07 02:59:38 2017
Response via : Initial Calibration

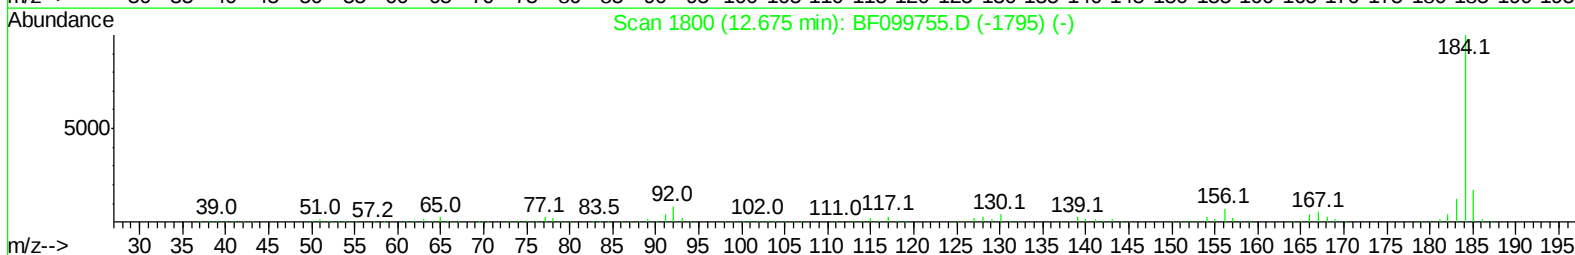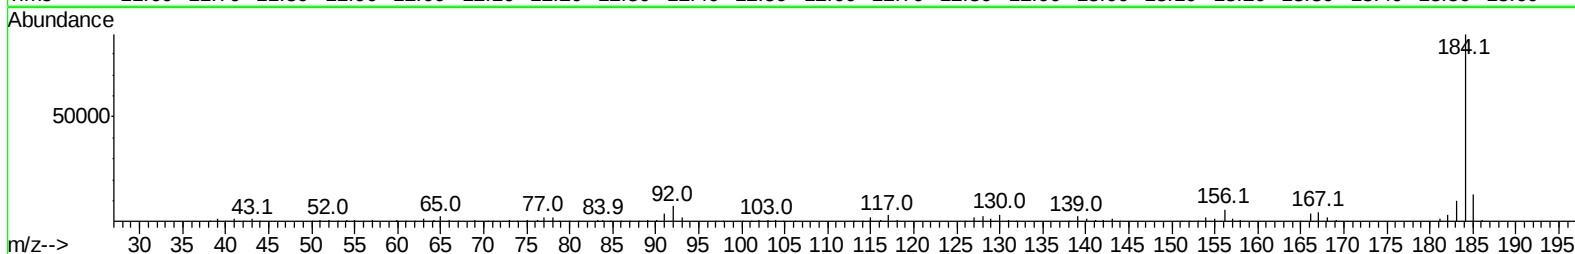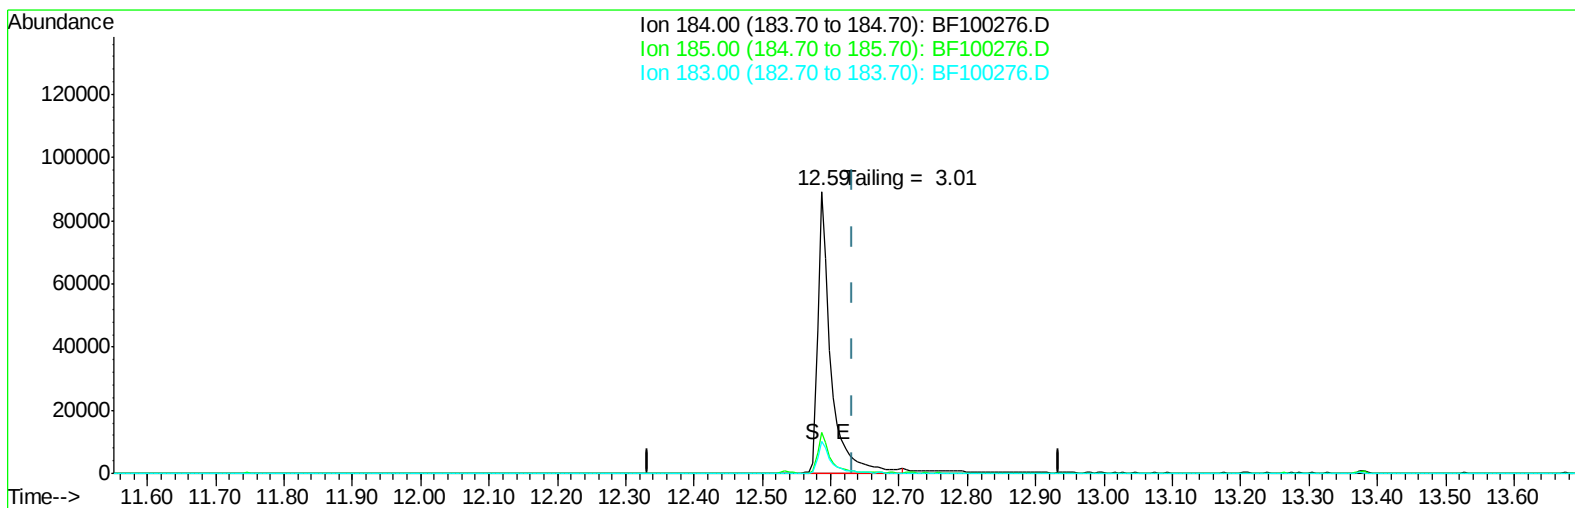

TIC: BF100276.D

(76) Benzidine

12.586min (-0.047) 0.00ng

response 118136

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.47
183.00	11.60	11.58
0.00	0.00	0.00