


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA F\Data\BF110717\
 Data File : BF100276.D
 Acq On : 7 Nov 2017 11:35
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 07 14:29:49 2017

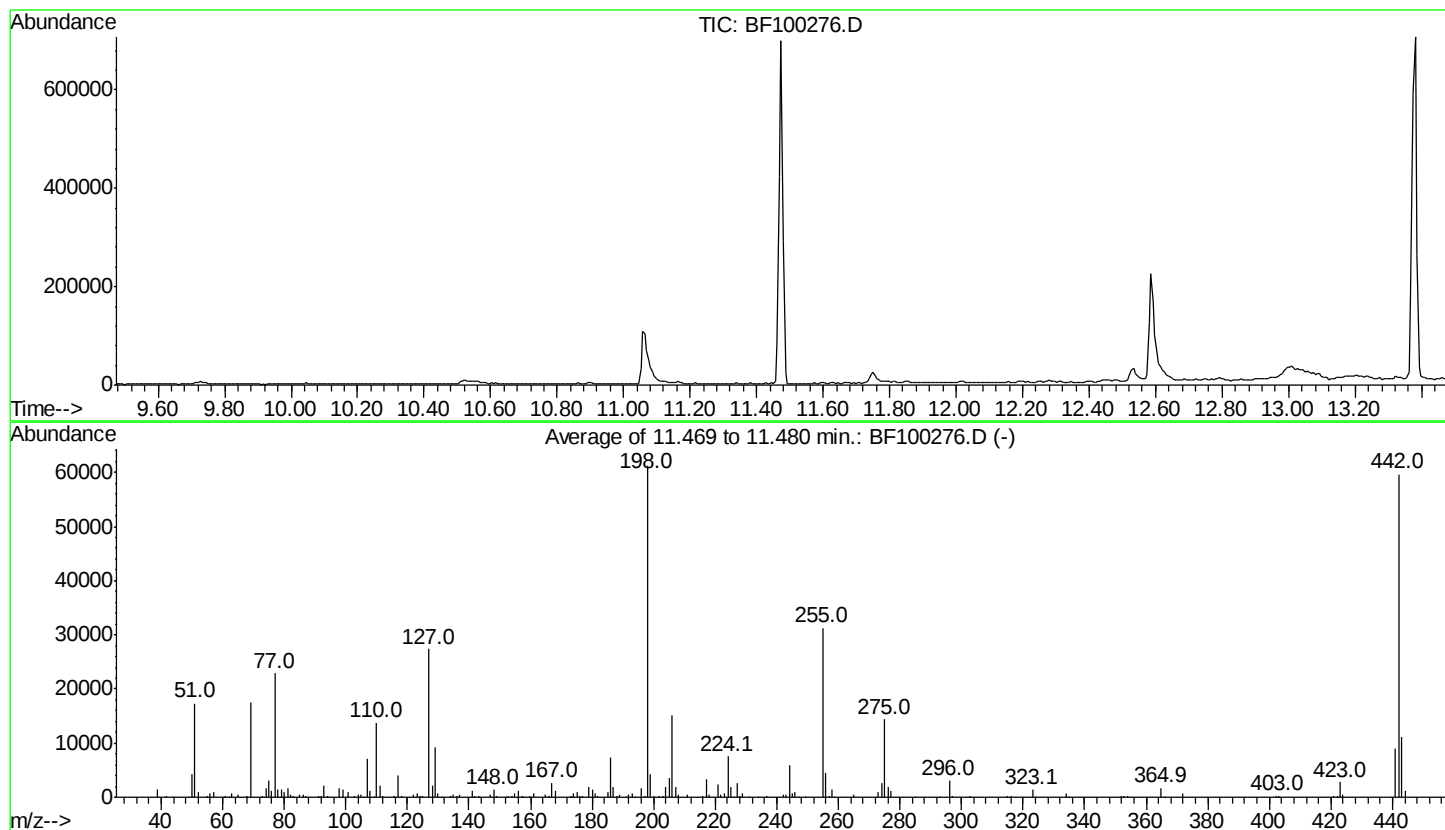

AutoFind: Scans 1595, 1596, 1597; Background Corrected with Scan 1590

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.2	17279	PASS
68	69	0.00	2	1.9	336	PASS
69	198	0.00	100	28.6	17489	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.8	27411	PASS
197	198	0.00	2	0.5	314	PASS
198	198	100	100	100.0	61248	PASS
199	198	5	9	6.8	4180	PASS
275	198	10	60	23.5	14386	PASS
365	198	1	100	2.8	1718	PASS
441	443	0.01	100	81.8	9080	PASS
442	198	50	100	97.4	59672	PASS
443	442	15	24	18.6	11101	PASS