


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110722\
 Data File : BF131035.D
 Acq On : 07 Nov 2022 09:48
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 08 01:40:43 2022

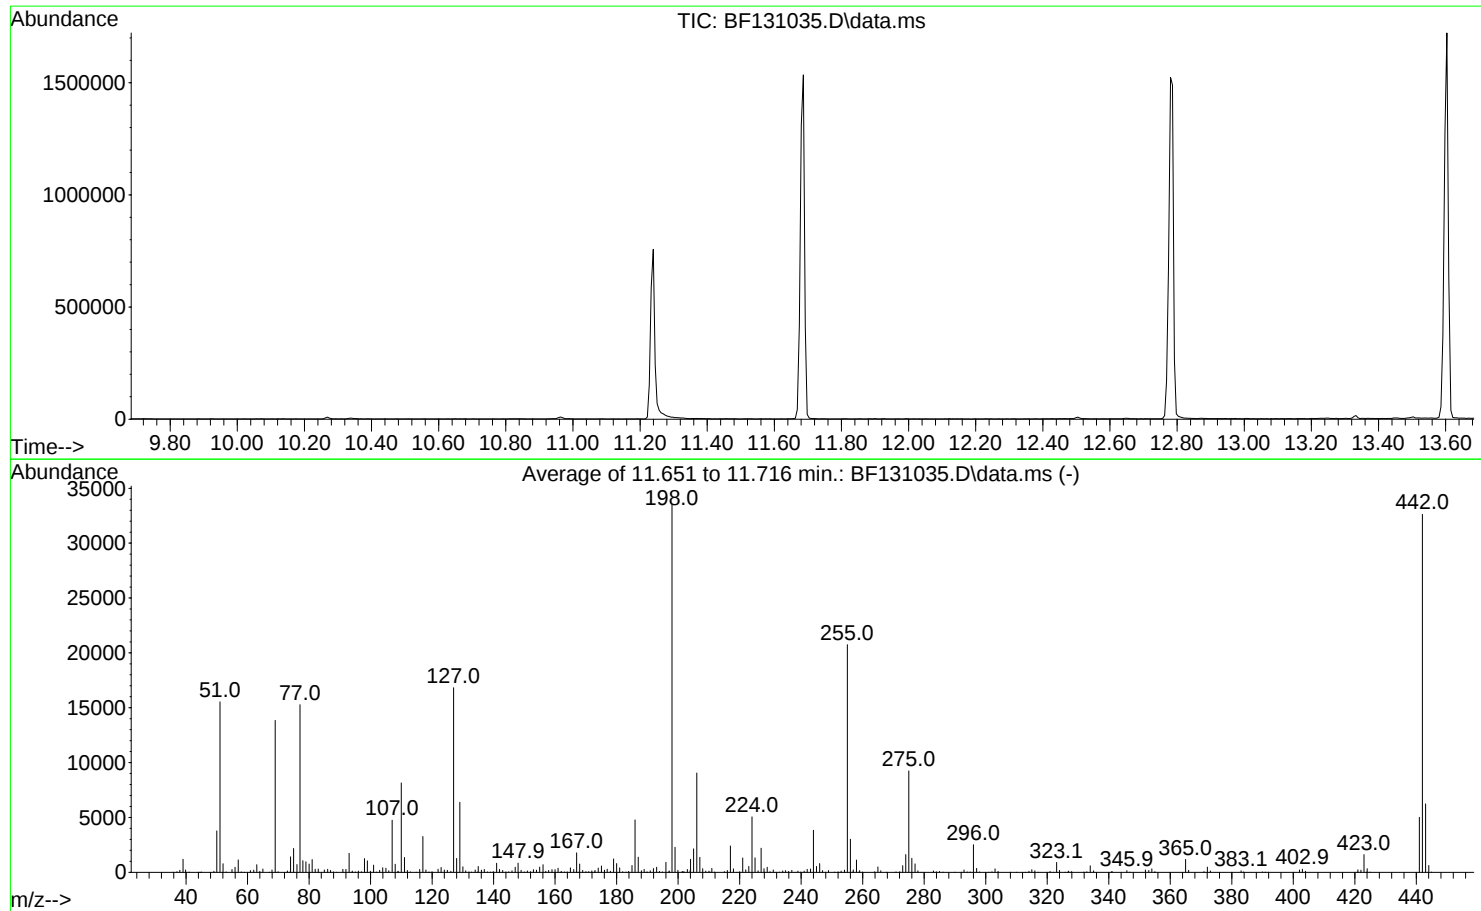




AutoFind: Averaged scan 1626 to 1637; Bkg corrected with scan 1625

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.4	15547	PASS
68	69	0.00	2	1.5	213	PASS
69	198	0.00	100	41.3	13845	PASS
70	69	0.00	2	0.4	59	PASS
127	198	10	80	50.2	16816	PASS
197	198	0.00	2	0.4	120	PASS
198	198	100	100	100.0	33528	PASS
199	198	5	9	6.8	2289	PASS
275	198	10	60	27.5	9233	PASS
365	198	1	100	3.5	1177	PASS
441	198	0.01	100	14.9	5012	PASS
442	442	50	100	100.0	32632	PASS
443	442	15	24	19.1	6231	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110722\
 Data File : BF131035.D
 Acq On : 07 Nov 2022 09:48
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Nov 08 04:31:42 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 08 01:40:43 2022
 Response via : Initial Calibration

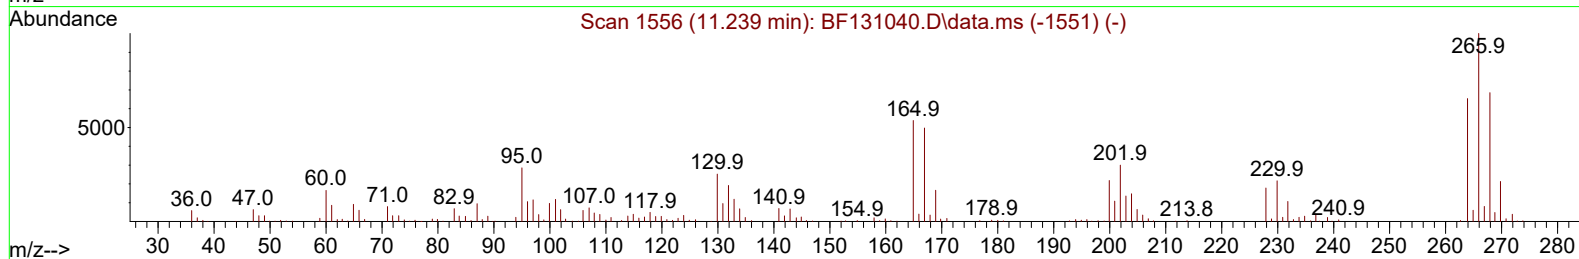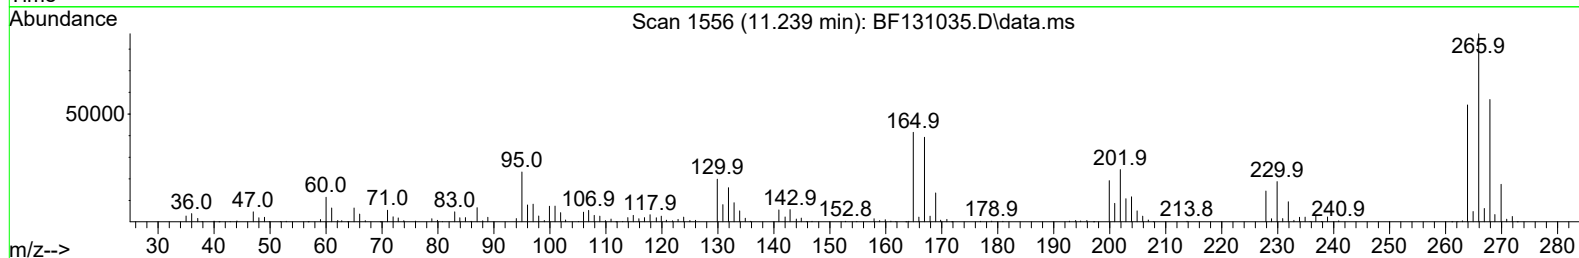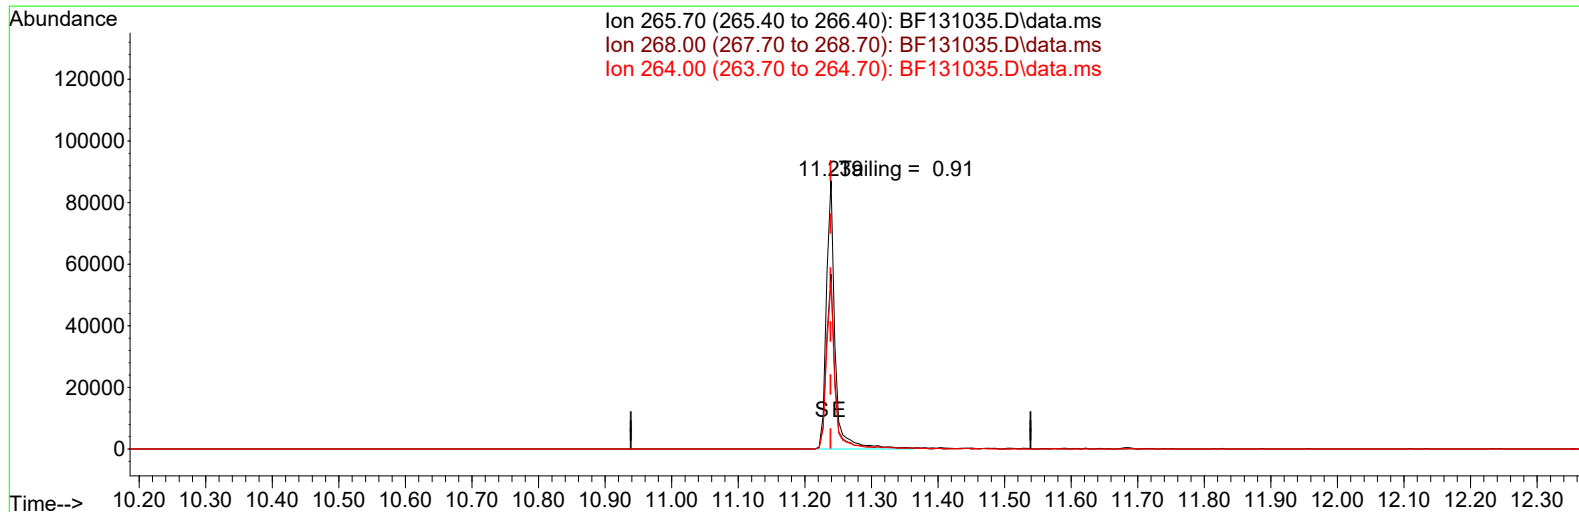

TIC: BF131035.D\data.ms

(70) Pentachlorophenol (C)

11.239min (+ 0.000) 21462.75 ng




response 79067

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	68.50	65.09
264.00	65.40	62.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110722\
Data File : BF131035.D
Acq On : 07 Nov 2022 09:48
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 08 04:31:42 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 08 01:40:43 2022
Response via : Initial Calibration

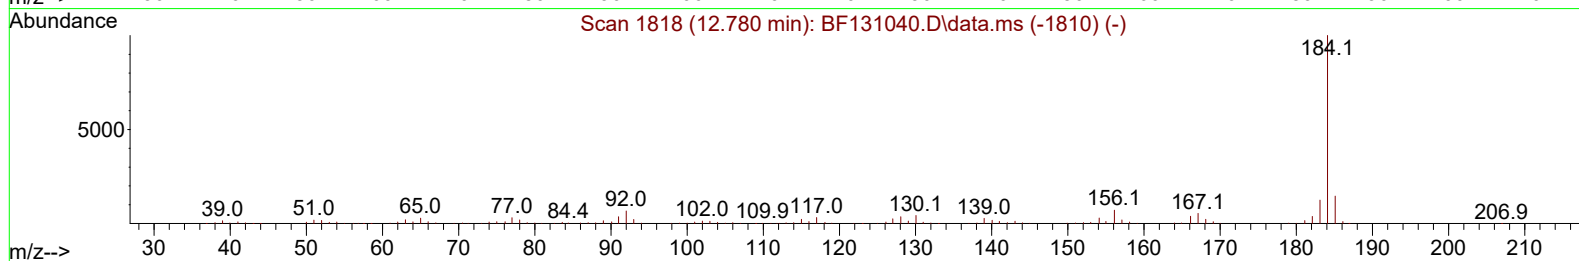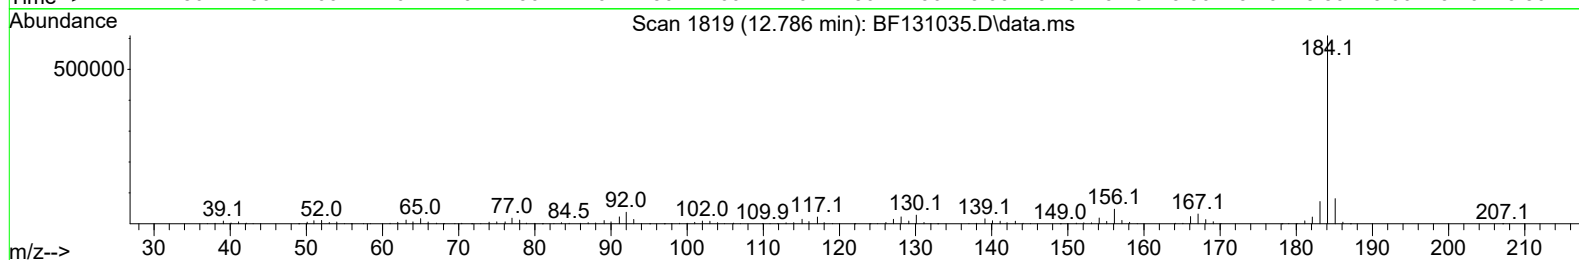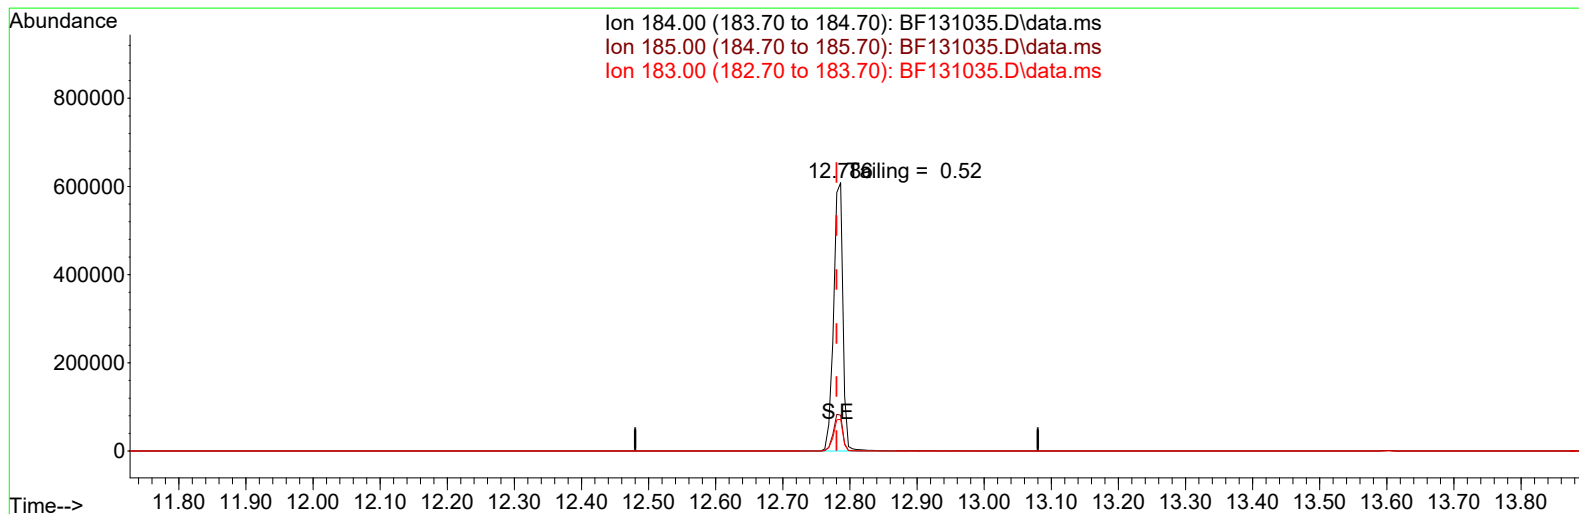

TIC: BF131035.D\data.ms

(77) Benzidine

12.786min (+ 0.006) 0.00 ng

response 588057

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	13.39
183.00	12.50	11.83
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/7/2022	BNA_F	<u>BF131035.D</u>
Compound Name	Response	Retention Time
DDT	275833	13.604
DDD	3051	13.333
DDE	300	12.968
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3351	279184	1.20

Instrument :
BNA_F
ClientSampleId :
DFTPP