

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110724\
 Data File : BF140284.D
 Acq On : 07 Nov 2024 19:18
 Operator : RC/JU
 Sample : P4700-01 5X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MH-8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110524.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF140284.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.216	17	21	29	rVB2	6335	11780	1.15%	0.135%
2	3.946	306	315	320	rBV	9580	16266	1.59%	0.187%
3	5.081	504	508	513	rVB	11902	15963	1.56%	0.184%
4	5.487	569	577	587	rBV	302713	400942	39.25%	4.609%
5	6.493	743	748	766	rVB	314493	403301	39.48%	4.636%
6	6.875	808	813	819	rBV	675354	847468	82.96%	9.743%
7	7.434	900	908	913	rBV	191901	245655	24.05%	2.824%
8	8.157	1023	1031	1038	rBV	812897	1021579	100.00%	11.744%
9	8.216	1038	1041	1050	rVB7	6064	12398	1.21%	0.143%
10	8.969	1165	1169	1177	rVB	7739	11658	1.14%	0.134%
11	9.228	1209	1213	1223	rBV	326272	422368	41.34%	4.856%
12	9.310	1223	1227	1235	rVV5	8255	13495	1.32%	0.155%
13	9.569	1267	1271	1274	rBV	9103	12727	1.25%	0.146%
14	9.628	1278	1281	1286	rVB4	7922	11772	1.15%	0.135%
15	9.775	1302	1306	1310	rBV	12448	17003	1.66%	0.195%
16	9.839	1311	1317	1322	rVB3	6174	11034	1.08%	0.127%
17	9.916	1323	1330	1334	rBV	752977	930155	91.05%	10.693%
18	10.116	1359	1364	1368	rBV2	15014	21455	2.10%	0.247%
19	10.339	1395	1402	1406	rBV4	9677	19316	1.89%	0.222%
20	10.463	1419	1423	1429	rVB2	12280	16096	1.58%	0.185%
21	10.628	1446	1451	1457	rVB	29839	42454	4.16%	0.488%
22	10.704	1459	1464	1476	rVV	155576	216814	21.22%	2.492%
23	10.828	1479	1485	1491	rVB2	21559	37864	3.71%	0.435%
24	11.010	1512	1516	1519	rBV5	6605	11225	1.10%	0.129%
25	11.263	1555	1559	1562	rVV3	12708	20054	1.96%	0.231%
26	11.298	1562	1565	1571	rVB2	17194	26535	2.60%	0.305%
27	11.404	1578	1583	1591	rBV2	707783	1012290	99.09%	11.637%
28	11.481	1592	1596	1600	rVB	30870	39625	3.88%	0.456%
29	11.639	1620	1623	1629	rBV3	7026	12263	1.20%	0.141%
30	11.933	1665	1673	1678	rBV2	44448	93756	9.18%	1.078%
31	12.022	1684	1688	1695	rVB2	41138	74962	7.34%	0.862%
32	12.204	1716	1719	1721	rBV	14088	17071	1.67%	0.196%
33	12.457	1760	1762	1765	rBV	14710	17326	1.70%	0.199%
34	12.622	1785	1790	1794	rBV	240765	307619	30.11%	3.536%
35	12.851	1823	1829	1835	rBV	225000	348794	34.14%	4.010%
36	12.992	1848	1853	1860	rVB	301512	416368	40.76%	4.787%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110724\
Data File : BF140284.D
Acq On : 07 Nov 2024 19:18
Operator : RC/JU
Sample : P4700-01 5X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MH-8

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110524.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	14.051	2028	2033	2043	rBV2	607010	1019481	99.79%	11.720%
38	15.557	2285	2289	2299	rVB	318059	521737	51.07%	5.998%




Sum of corrected areas: 8698669

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110724\
Data File : BF140284.D
Acq On : 07 Nov 2024 19:18
Operator : RC/JU
Sample : P4700-01 5X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MH-8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

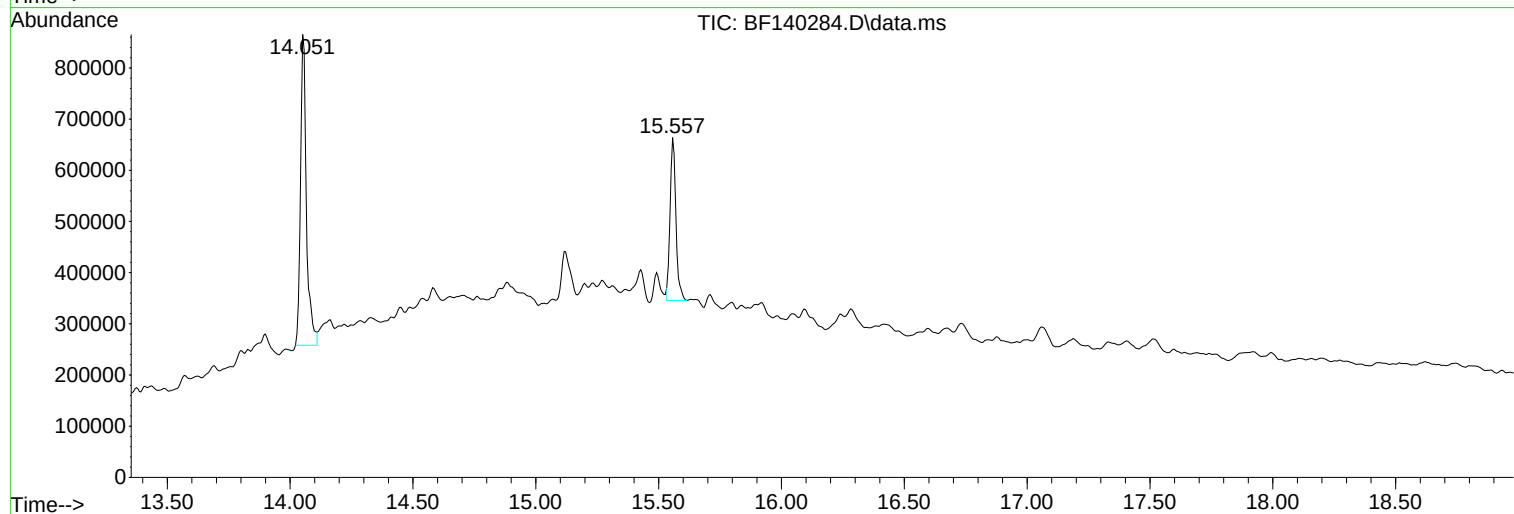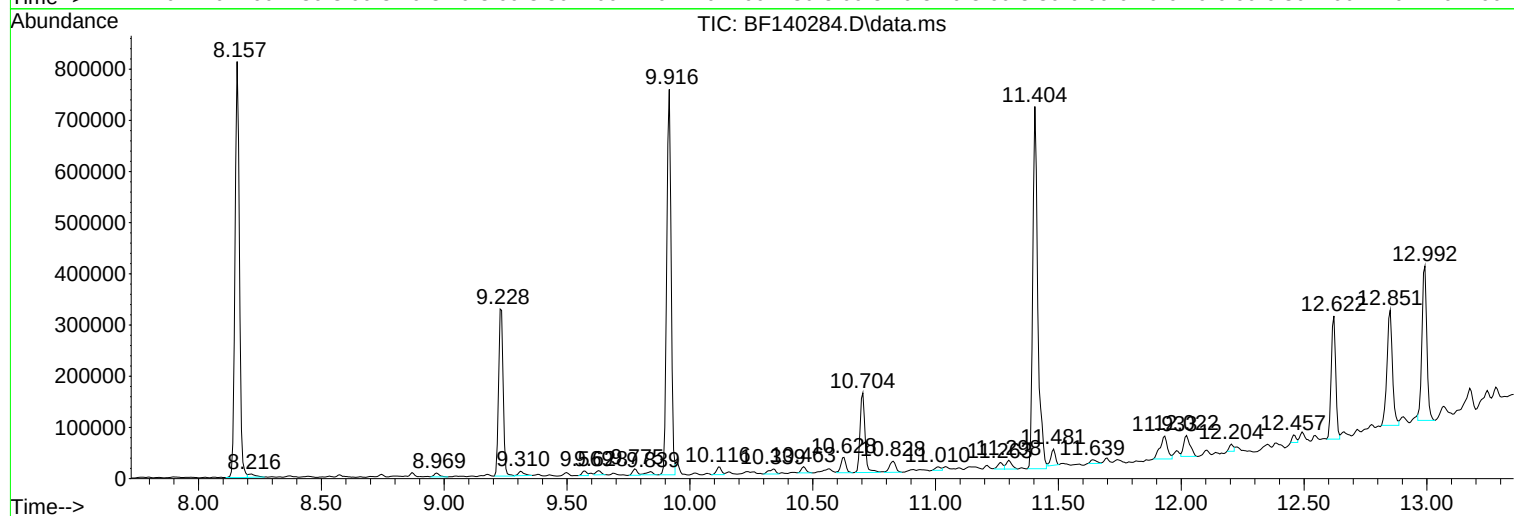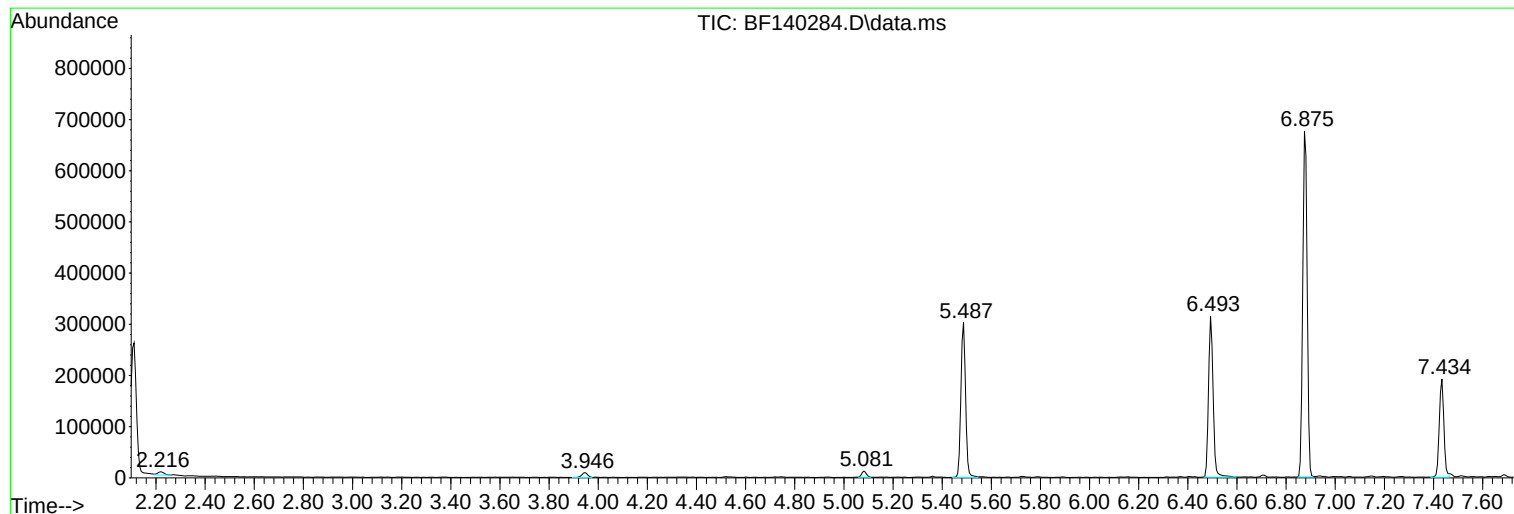

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110724\
Data File : BF140284.D
Acq On : 07 Nov 2024 19:18
Operator : RC/JU
Sample : P4700-01 5X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MH-8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110724\
Data File : BF140284.D
Acq On : 07 Nov 2024 19:18
Operator : RC/JU
Sample : P4700-01 5X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MH-8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------