


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110724\
Data File : BF140260.D
Acq On : 07 Nov 2024 08:33
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110524.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Nov 05 16:47:56 2024

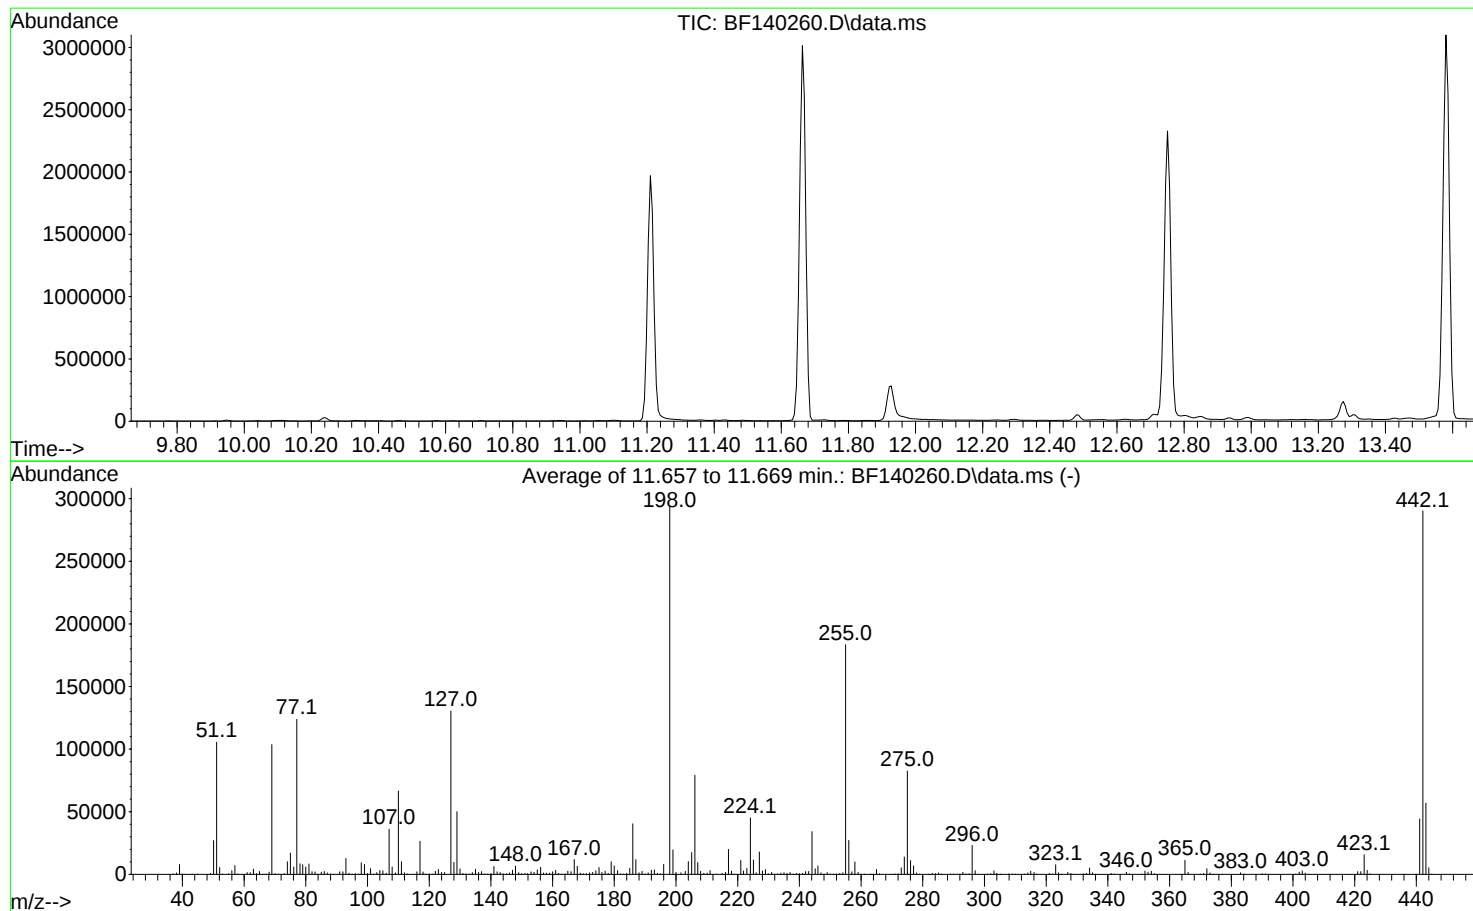




AutoFind: Scans 1626, 1627, 1628; Background Corrected with Scan 1619

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	35.9	105560	PASS
68	69	0.00	2	1.8	1838	PASS
69	198	0.00	100	35.3	103621	PASS
70	69	0.00	2	0.6	596	PASS
127	198	10	80	44.4	130427	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	293760	PASS
199	198	5	9	6.7	19592	PASS
275	198	10	60	28.1	82563	PASS
365	198	1	100	3.8	11210	PASS
441	198	0.01	100	15.1	44267	PASS
442	442	50	100	100.0	290283	PASS
443	442	15	24	19.6	56872	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110724\
Data File : BF140260.D
Acq On : 07 Nov 2024 08:33
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 07 10:53:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 05 16:47:56 2024
Response via : Initial Calibration

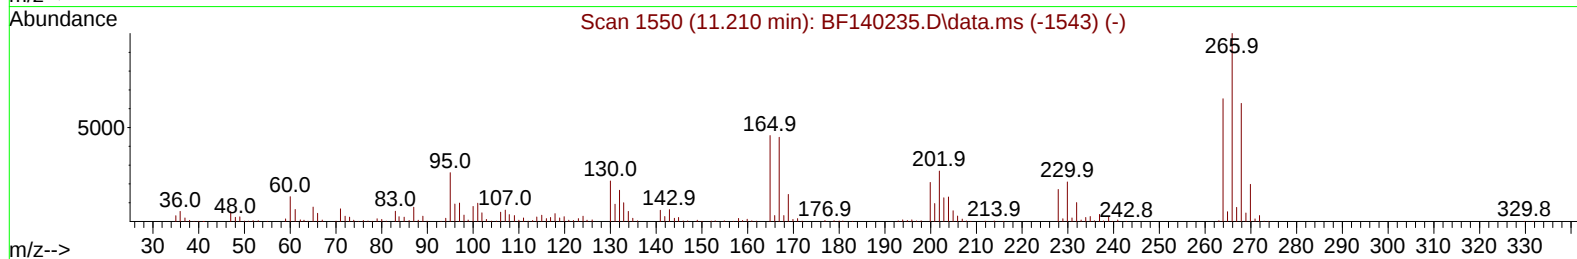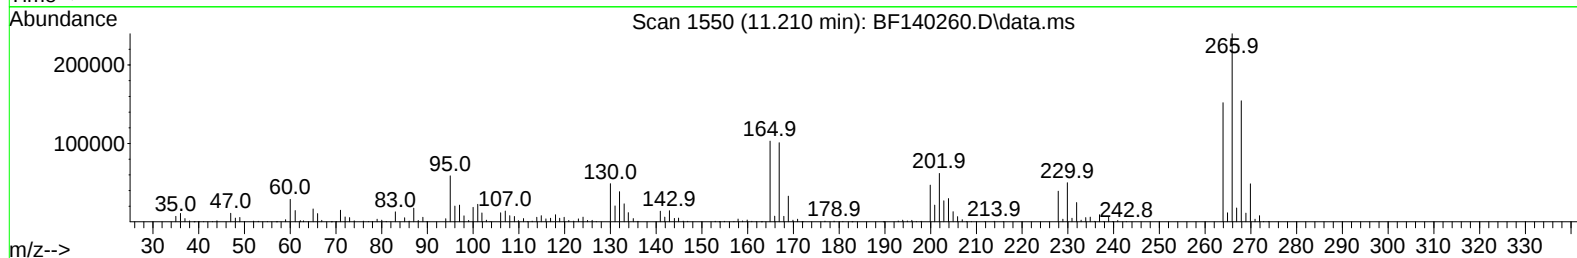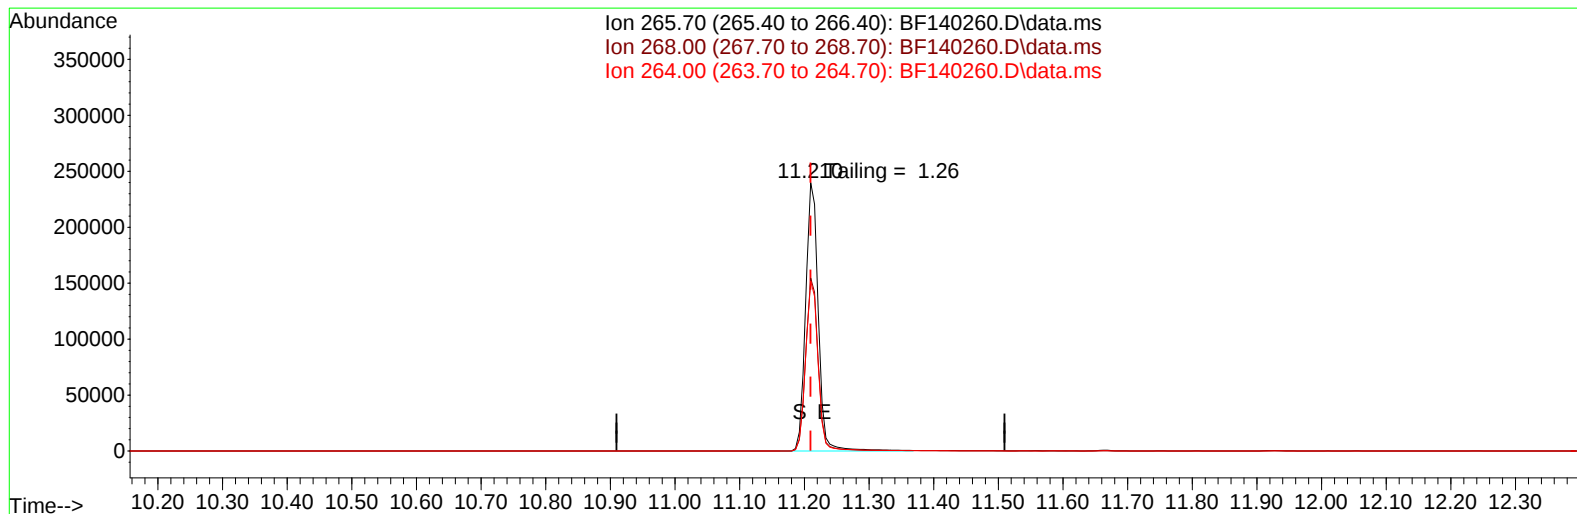

TIC: BF140260.D\data.ms

(70) Pentachlorophenol (C)

11.210min (0.000) 24111.20 ng




response 328643

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.80	64.41
264.00	65.30	63.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110724\
Data File : BF140260.D
Acq On : 07 Nov 2024 08:33
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 07 10:53:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 05 16:47:56 2024
Response via : Initial Calibration

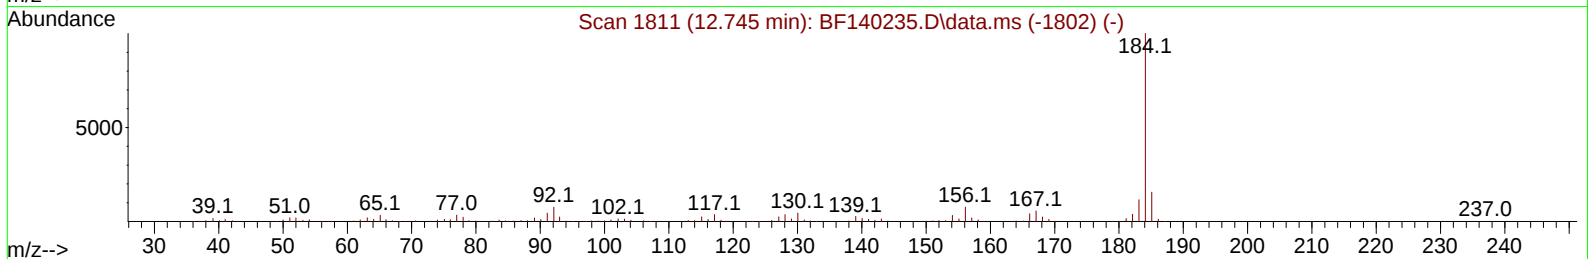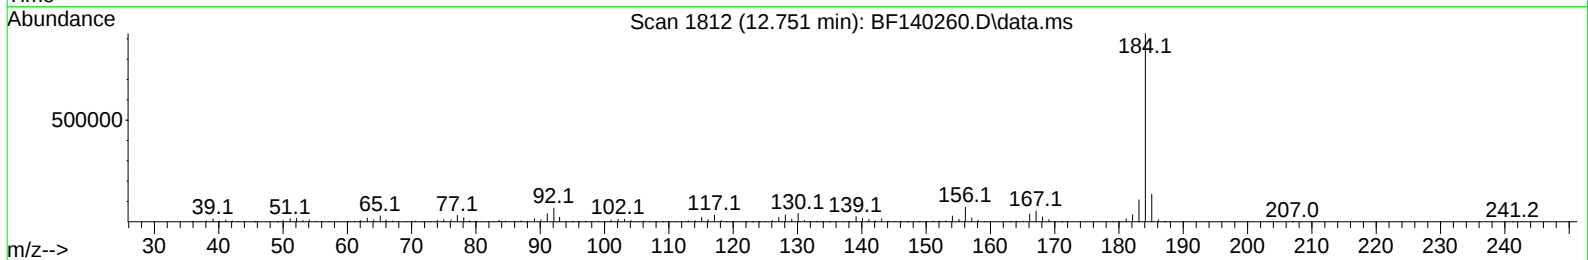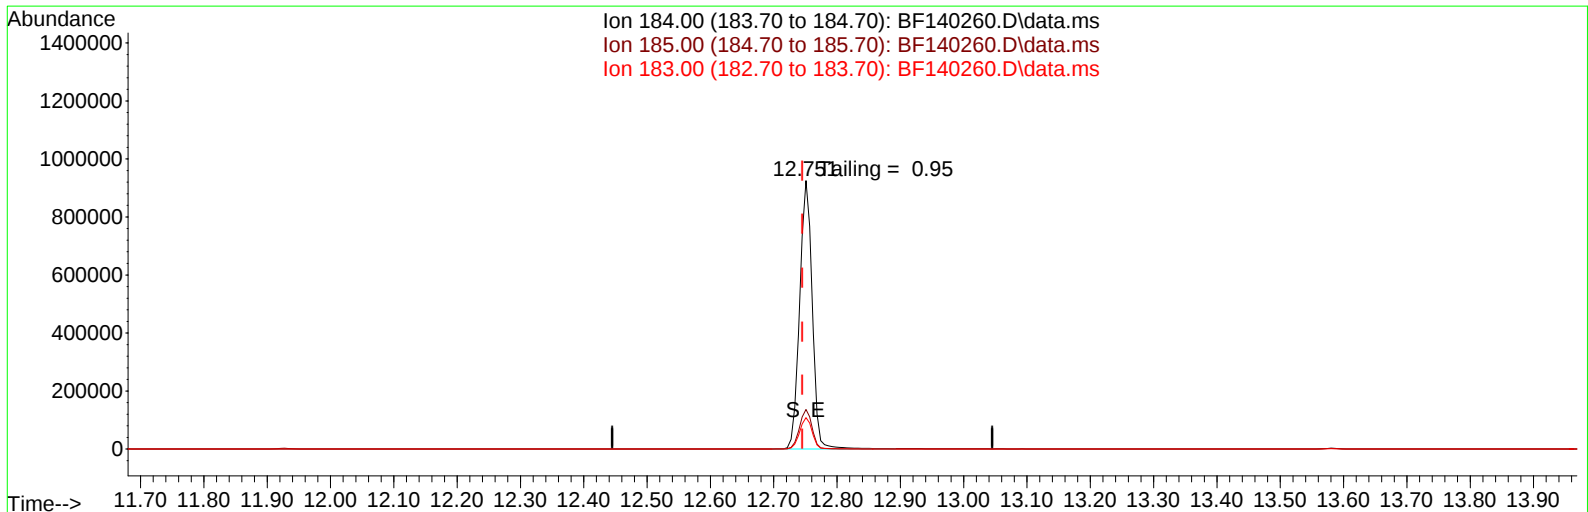

TIC: BF140260.D\data.ms

(77) Benzidine

12.751min (+ 0.006) 13054.59 ng

response 1289985

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.60	14.73
183.00	11.60	11.70
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/7/2024	BNA_F	<u>BF140260.D</u>
Compound Name	Response	Retention Time
DDT	791360	13.58
DDD	41940	13.274
DDE	2893	12.933
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
44833	836193	5.36

Instrument :
BNA_F
ClientSampleId :
DFTPP