
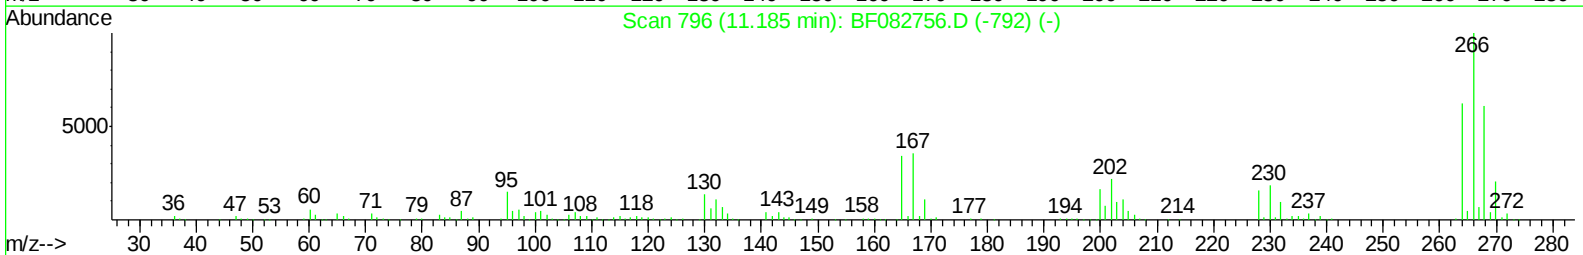
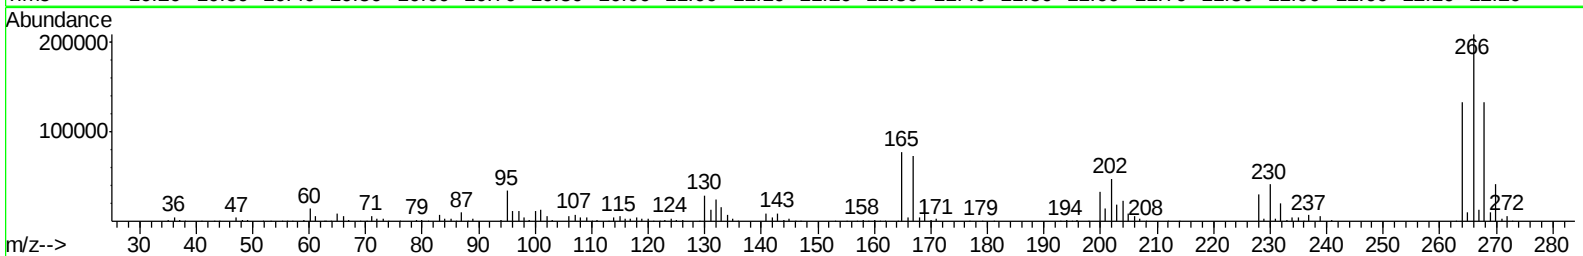


Data Path : Z:\HPCHEM1\BNA_F\Data\BF110815\
Data File : BF082812.D
Acq On : 8 Nov 2015 00:06
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 09 07:33:40 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 07 02:32:49 2015
Response via : Initial Calibration

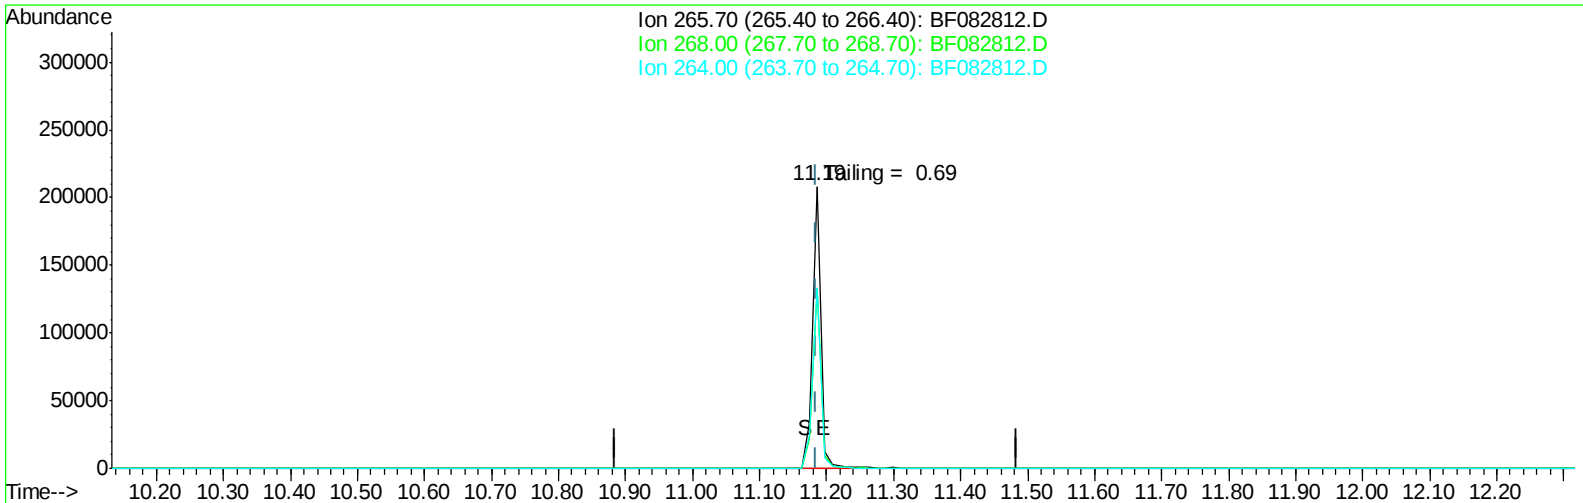

TIC: BF082812.D

(69) Pentachlorophenol (C)




11.185min (+0.000) 19055.78ng

response 180784

Ion	Exp%	Act%
265.70	100	100
268.00	63.80	64.08
264.00	63.20	64.02
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF110815\
Data File : BF082812.D
Acq On : 8 Nov 2015 00:06
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 09 07:33:40 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 07 02:32:49 2015
Response via : Initial Calibration

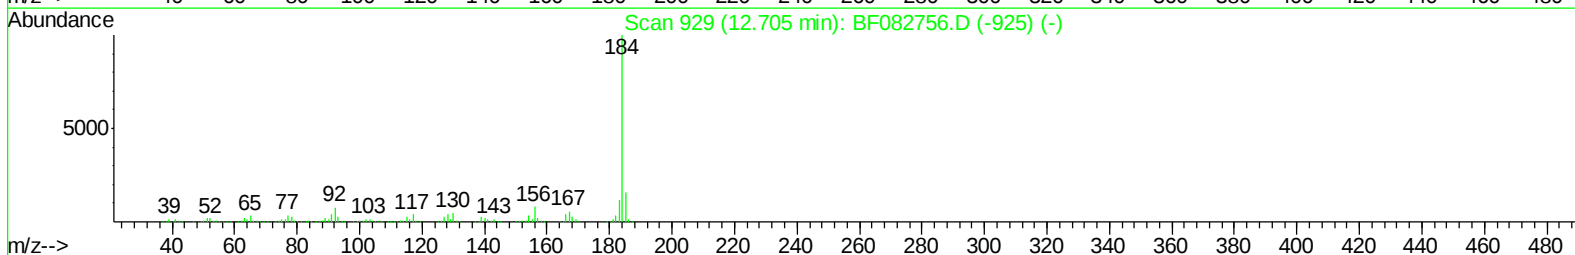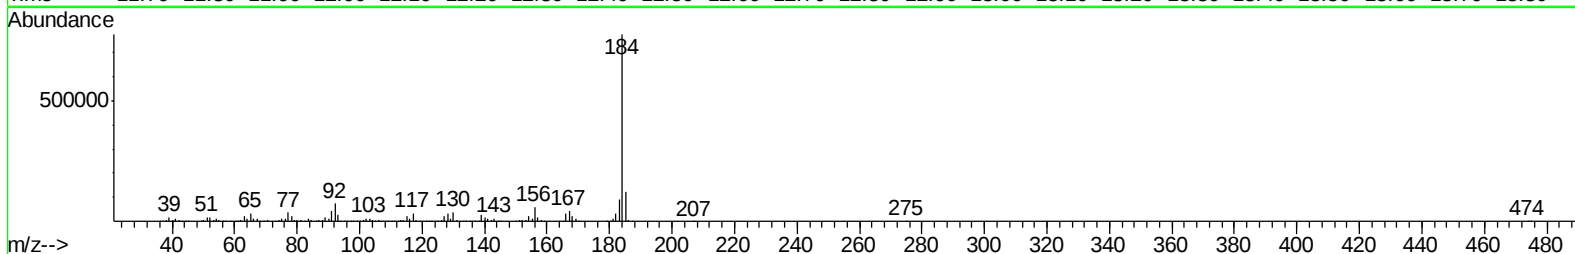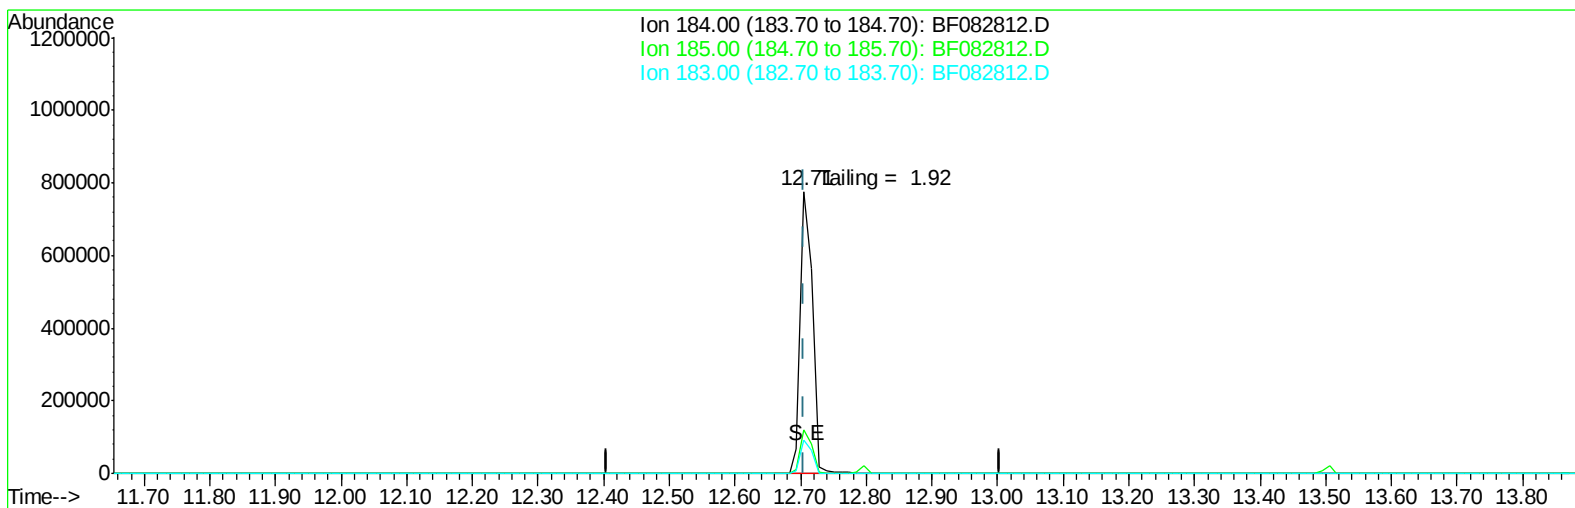

TIC: BF082812.D

(76) Benzidine

12.705min (+0.000) 23198.90ng m

response 990522

Ion	Exp%	Act%
184.00	100	100
185.00	15.00	15.51
183.00	12.00	11.77
0.00	0.00	0.00