


Data Path : Z:\HPCHEM1\BNA F\DATA\BF110815\
 Data File : BF082812.D
 Acq On : 8 Nov 2015 00:06
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Nov 07 02:32:49 2015

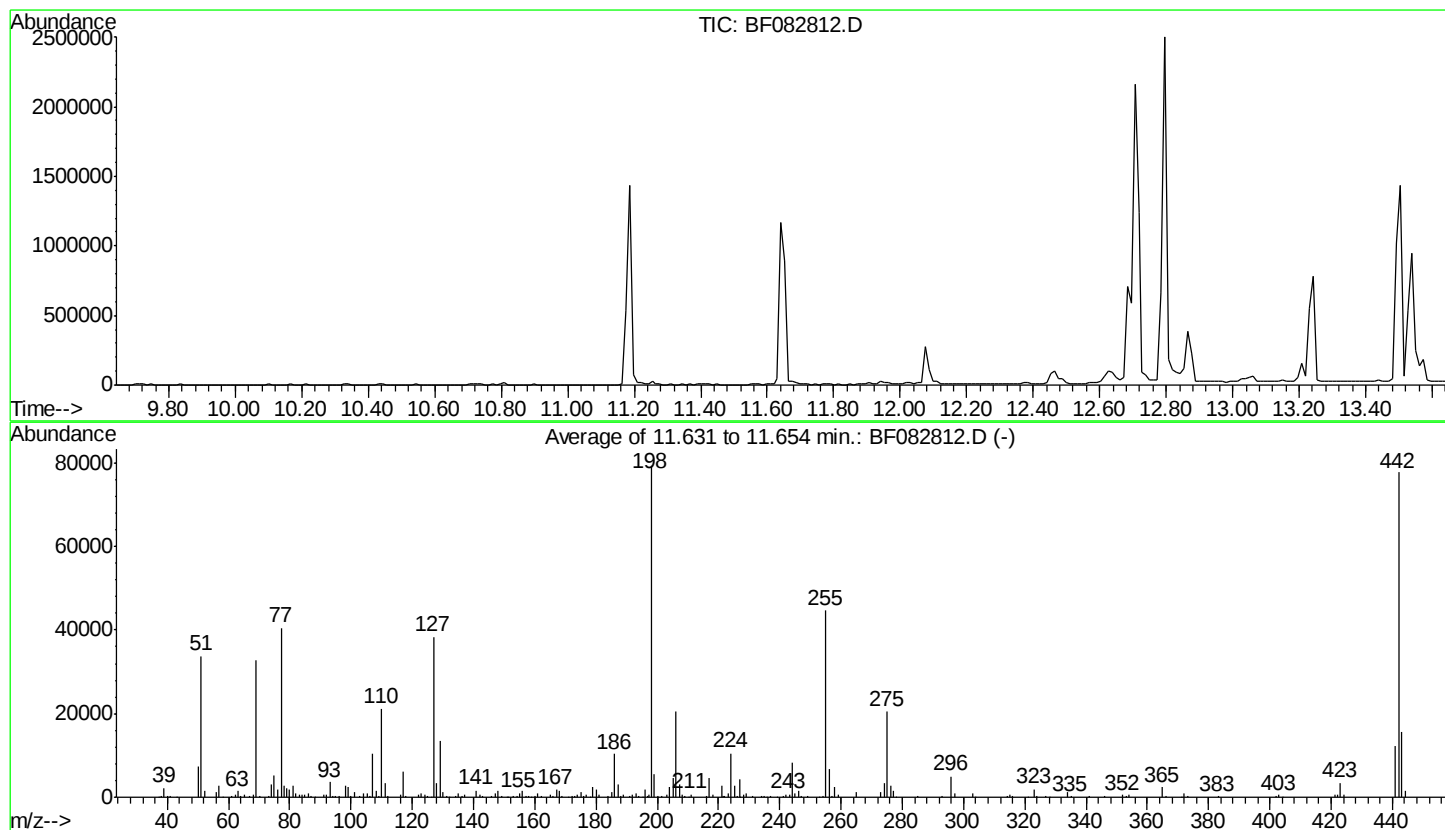

AutoFind: Scans 835, 836, 837; Background Corrected with Scan 832

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.5	33756	PASS
68	69	0.00	2	1.7	551	PASS
69	198	0.00	100	41.4	32839	PASS
70	69	0.00	2	0.5	178	PASS
127	198	10	80	48.3	38335	PASS
197	198	0.00	2	0.6	476	PASS
198	198	100	100	100.0	79346	PASS
199	198	5	9	7.0	5551	PASS
275	198	10	60	25.8	20485	PASS
365	198	1	100	3.0	2410	PASS
441	442	0.01	24	15.8	12282	PASS
442	198	50	100	98.1	77852	PASS
443	442	15	24	20.0	15567	PASS