
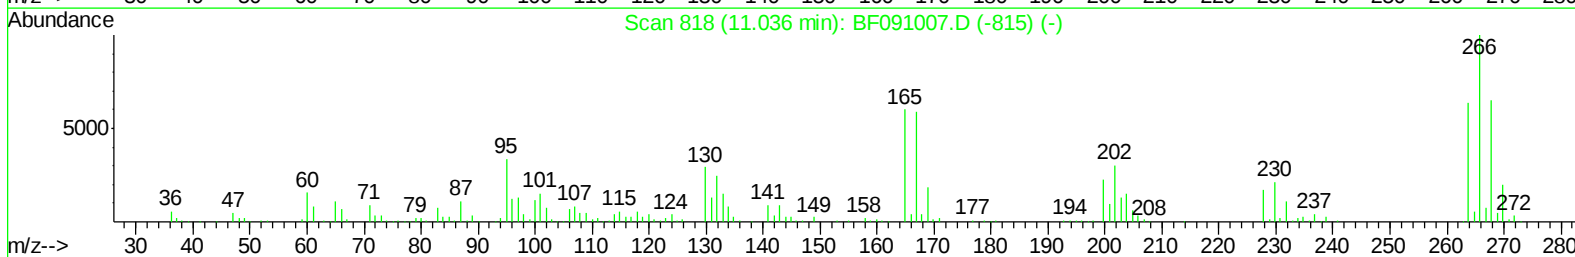
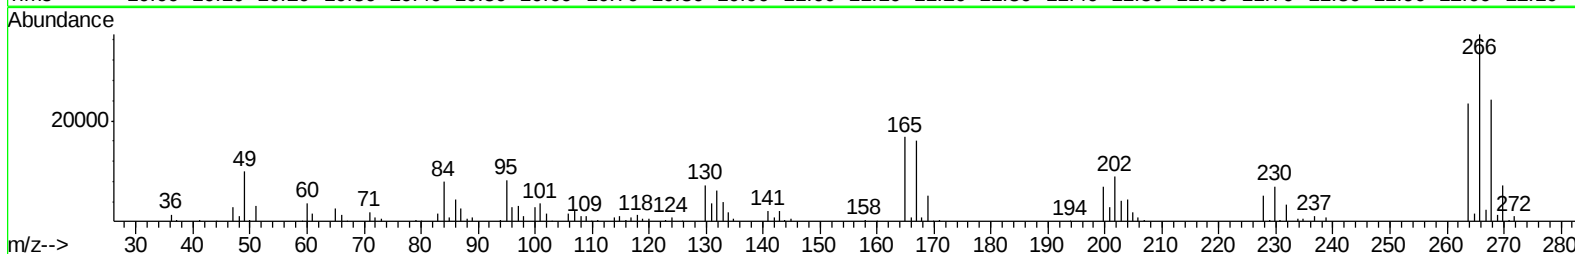


Data Path : Z:\HPCHEM1\BNA F\DATA\BF110816\
Data File : BF091075.D
Acq On : 8 Nov 2016 10:58
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 09 16:22:00 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 08 12:59:29 2016
Response via : Initial Calibration

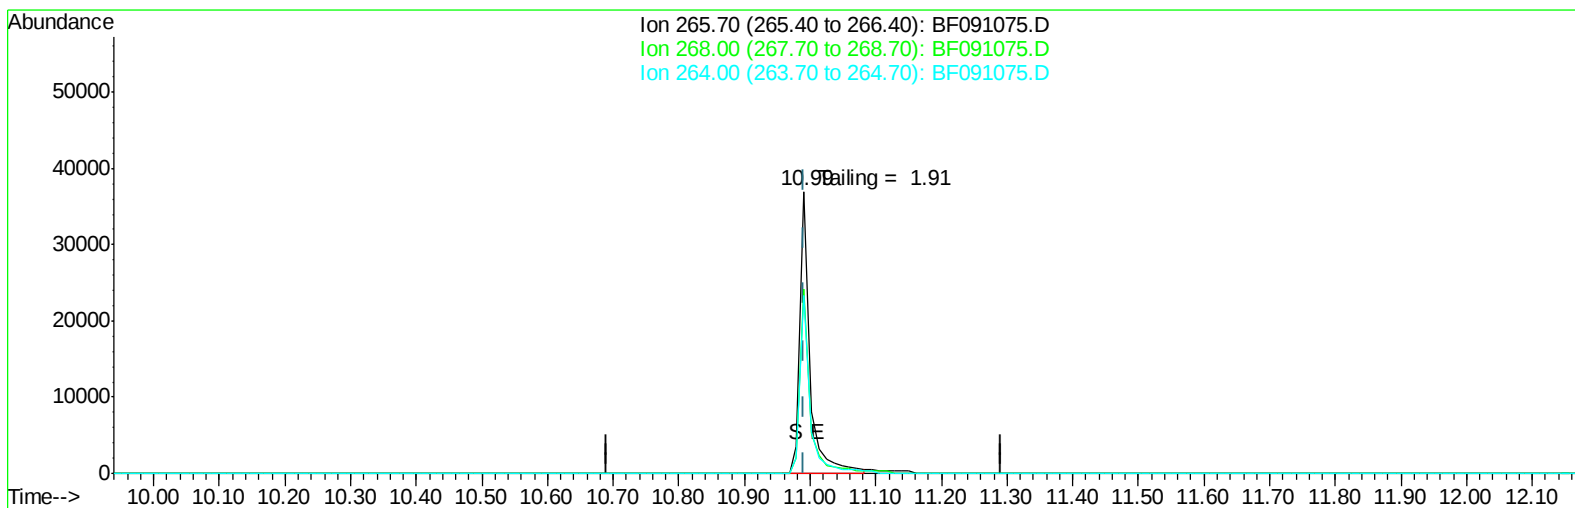

TIC: BF091075.D

(69) Pentachlorophenol (C)




10.991min (+0.000) 0.00ng

response 41261

Ion	Exp%	Act%
265.70	100	100
268.00	65.10	65.65
264.00	63.90	63.29
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF110816\
Data File : BF091075.D
Acq On : 8 Nov 2016 10:58
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 09 16:22:00 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 08 12:59:29 2016
Response via : Initial Calibration

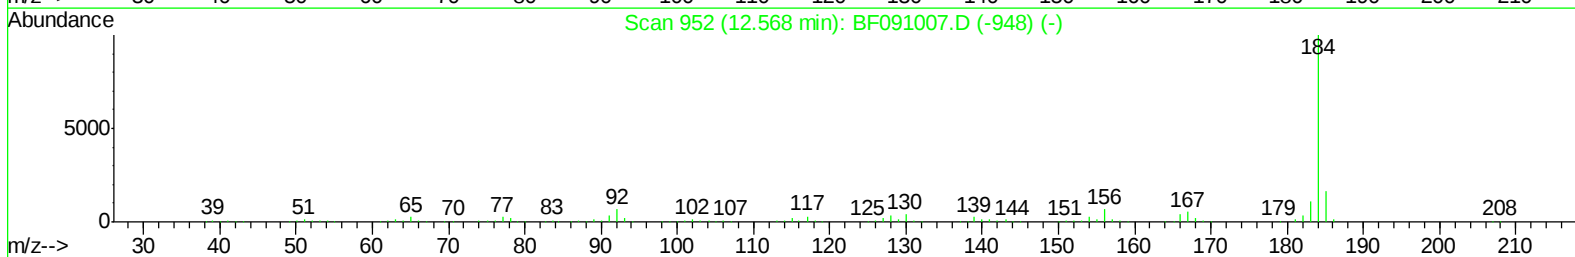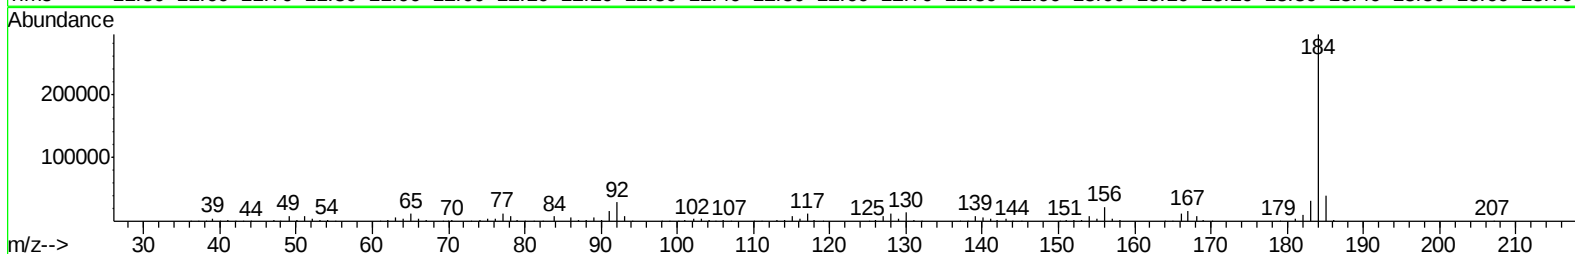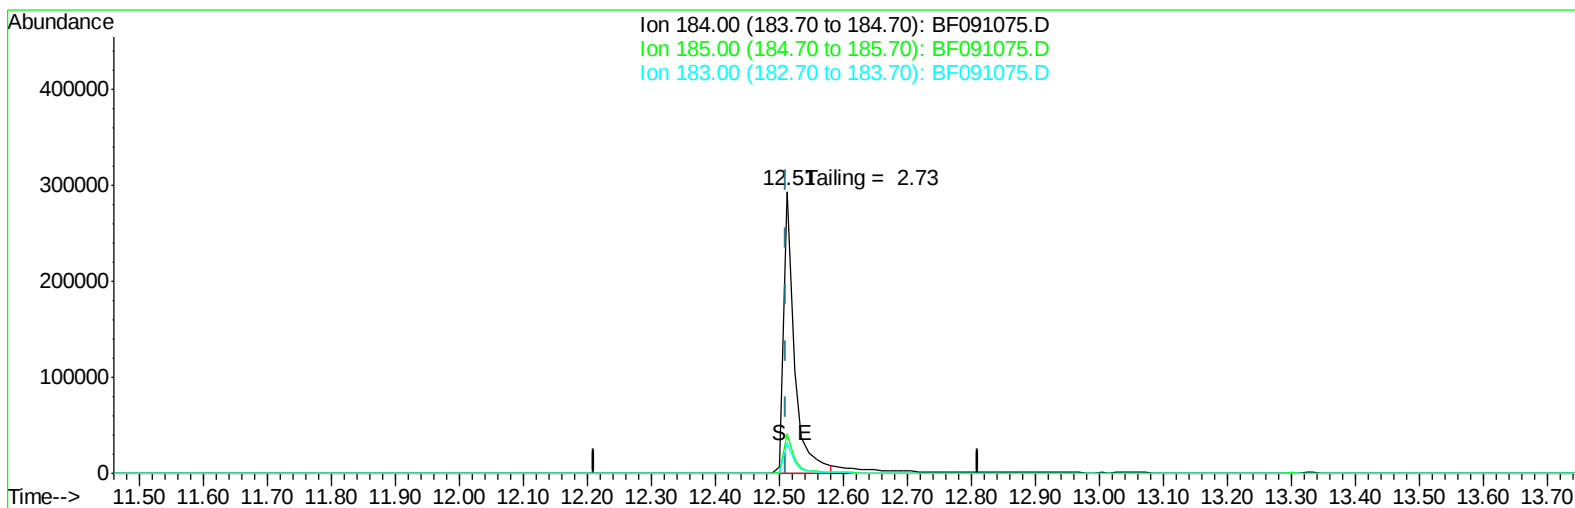

TIC: BF091075.D

(76) Benzidine

12.511min (+0.000) 13851.32ng

response 377834

Ion	Exp%	Act%
184.00	100	100
185.00	16.20	14.07
183.00	10.90	11.10
0.00	0.00	0.00