
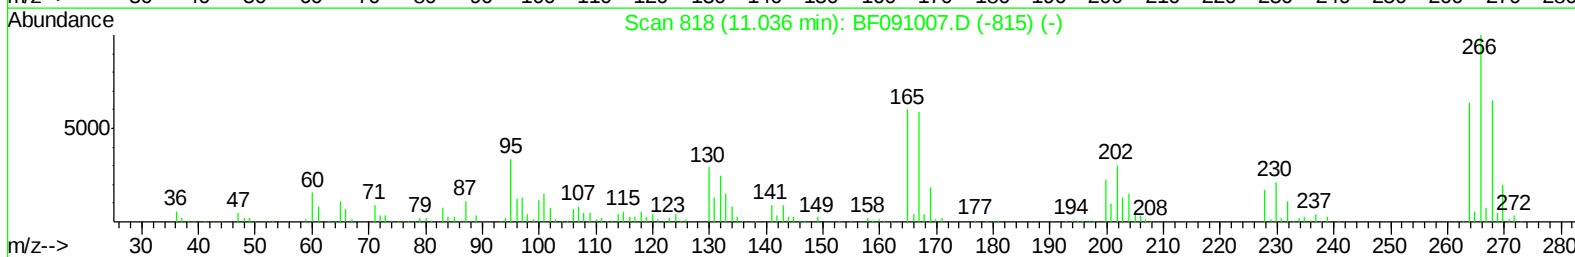
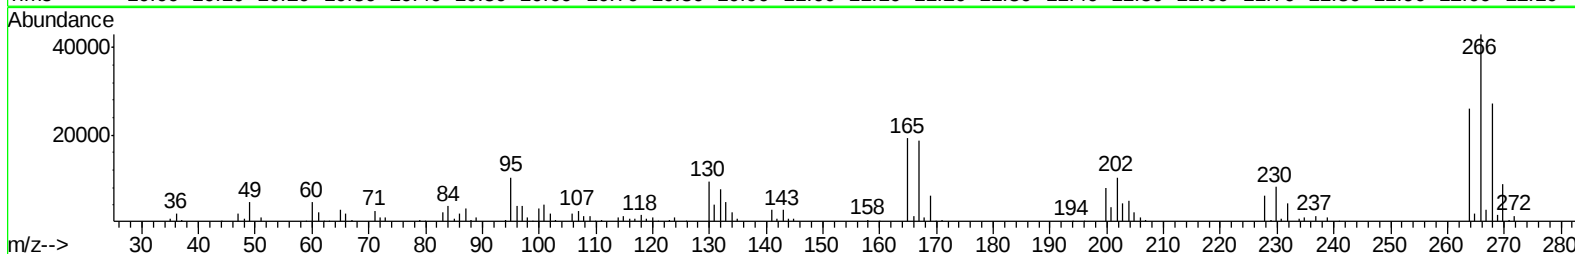


Data Path : Z:\HPCHEM1\BNA F\DATA\BF110816\
Data File : BF091080.D
Acq On : 8 Nov 2016 13:20
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 09 16:22:55 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 08 12:59:29 2016
Response via : Initial Calibration

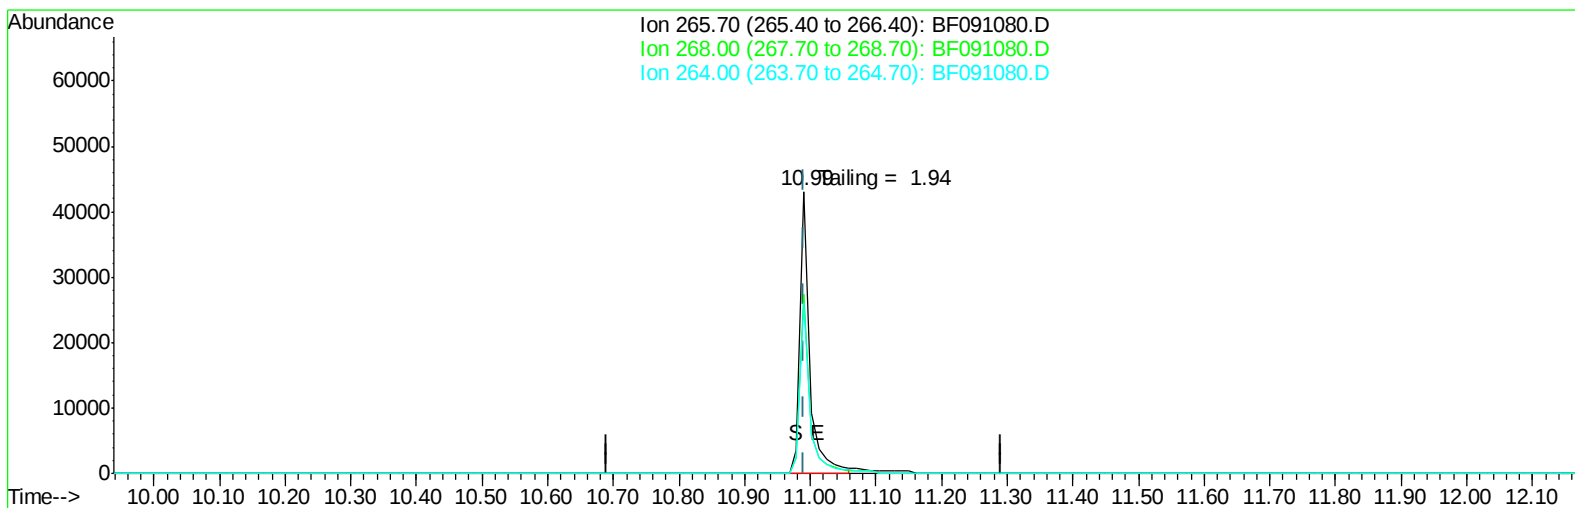

TIC: BF091080.D

(69) Pentachlorophenol (C)




10.991min (-0.000) 44569.39ng

response 47330

Ion	Exp%	Act%
265.70	100	100
268.00	65.10	63.43
264.00	63.90	60.49
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF110816\
Data File : BF091080.D
Acq On : 8 Nov 2016 13:20
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 09 16:22:55 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 08 12:59:29 2016
Response via : Initial Calibration

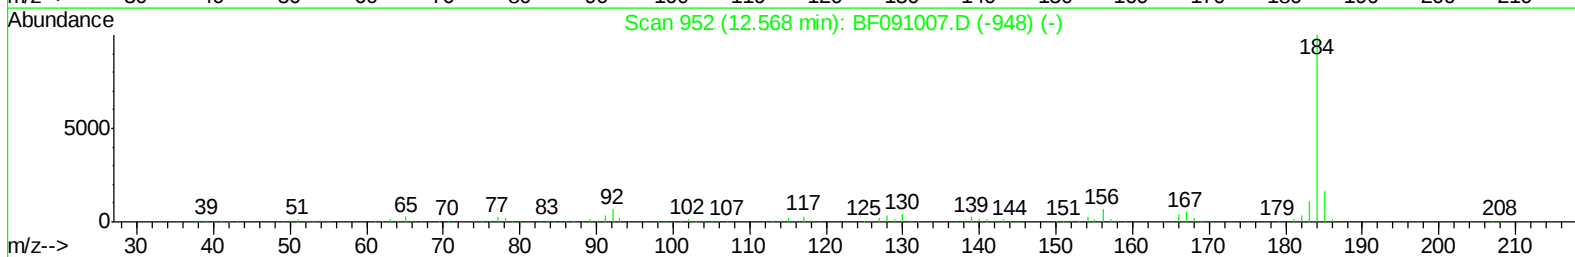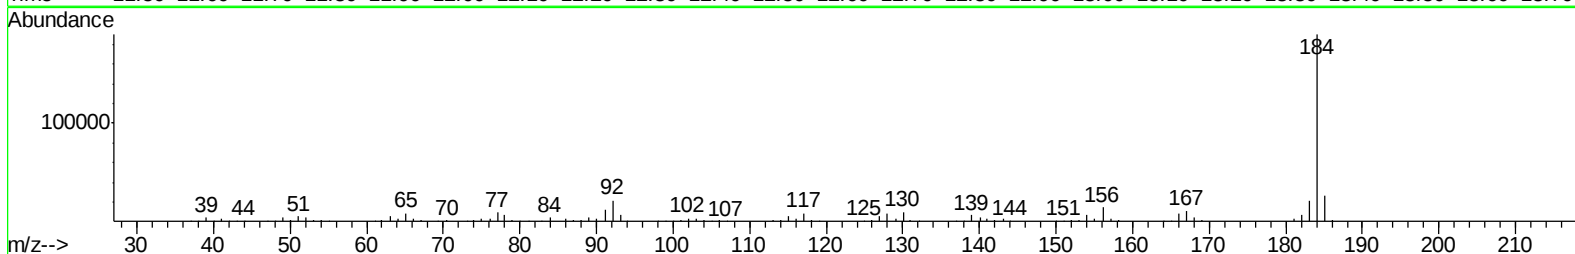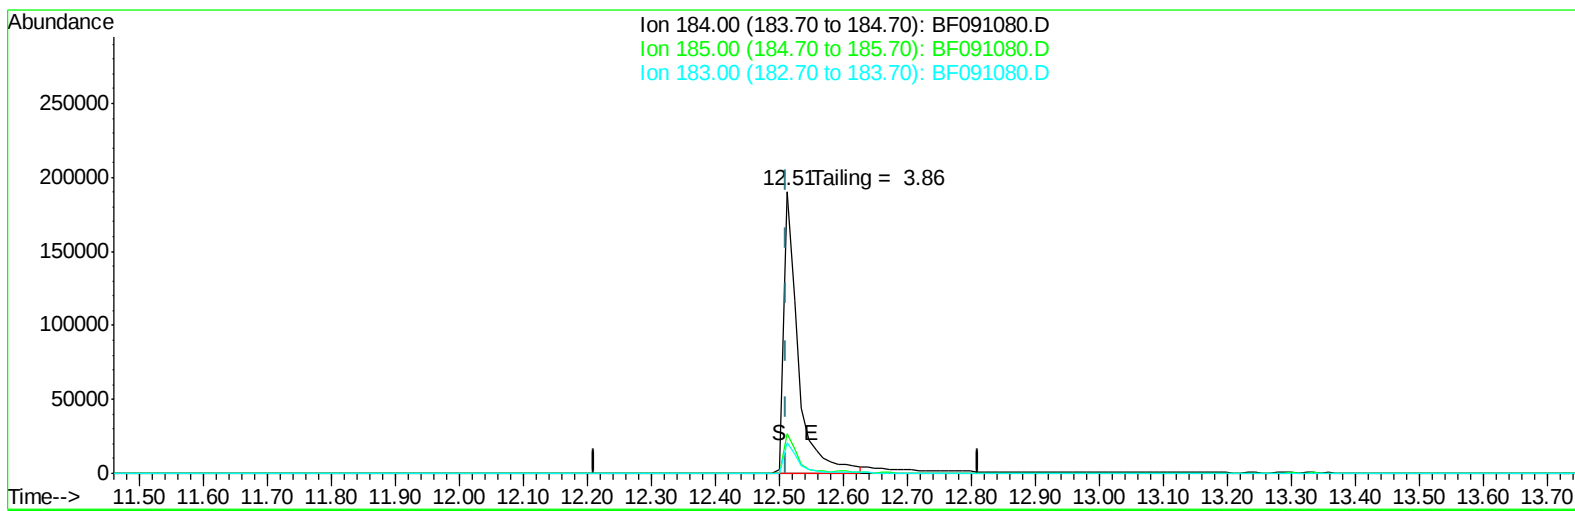

TIC: BF091080.D

(76) Benzidine

12.511min (-0.000) 42948.45ng

response 315673

Ion	Exp%	Act%
184.00	100	100
185.00	16.20	14.05
183.00	10.90	11.05
0.00	0.00	0.00