

Data Path : Z:\HPCHEM1\BNA F\DATA\BF110816\
 Data File : BF091093.D
 Acq On : 8 Nov 2016 20:22
 Operator : UM/SJ
 Sample : H5581-08
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DRW2

Quant Time: Nov 09 02:28:55 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110316.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 08 12:59:29 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.66	152	170716	20.00	ng	0.00
21) Naphthalene-d8	7.95	136	712076	20.00	ng	0.00
38) Acenaphthene-d10	9.70	164	393162	20.00	ng	0.00
63) Phenanthrene-d10	11.17	188	609955	20.00	ng	0.00
75) Chrysene-d12	13.80	240	448272	20.00	ng	-0.01
86) Perylene-d12	15.19	264	320515	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.25	112	684646	66.23	ng	0.01
7) Phenol-d6	6.32	99	562508	40.09	ng	0.00
23) Nitrobenzene-d5	7.23	82	1194446	91.50	ng	-0.01
41) 2,4,6-Tribromophenol	10.49	330	466612	131.28	ng	0.00
44) 2-Fluorobiphenyl	9.02	172	1858212	81.37	ng	-0.01
78) Terphenyl-d14	12.76	244	2008208	111.79	ng	0.00
Target Compounds						
83) Bis(2-ethylhexyl)phthalate	13.80	149	58983	3.10	ng	Qvalue # 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF110816\
Data File : BF091093.D
Acq On : 8 Nov 2016 20:22
Operator : UM/SJ
Sample : H5581-08
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DRW2

Quant Time: Nov 09 02:28:55 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 08 12:59:29 2016
Response via : Initial Calibration

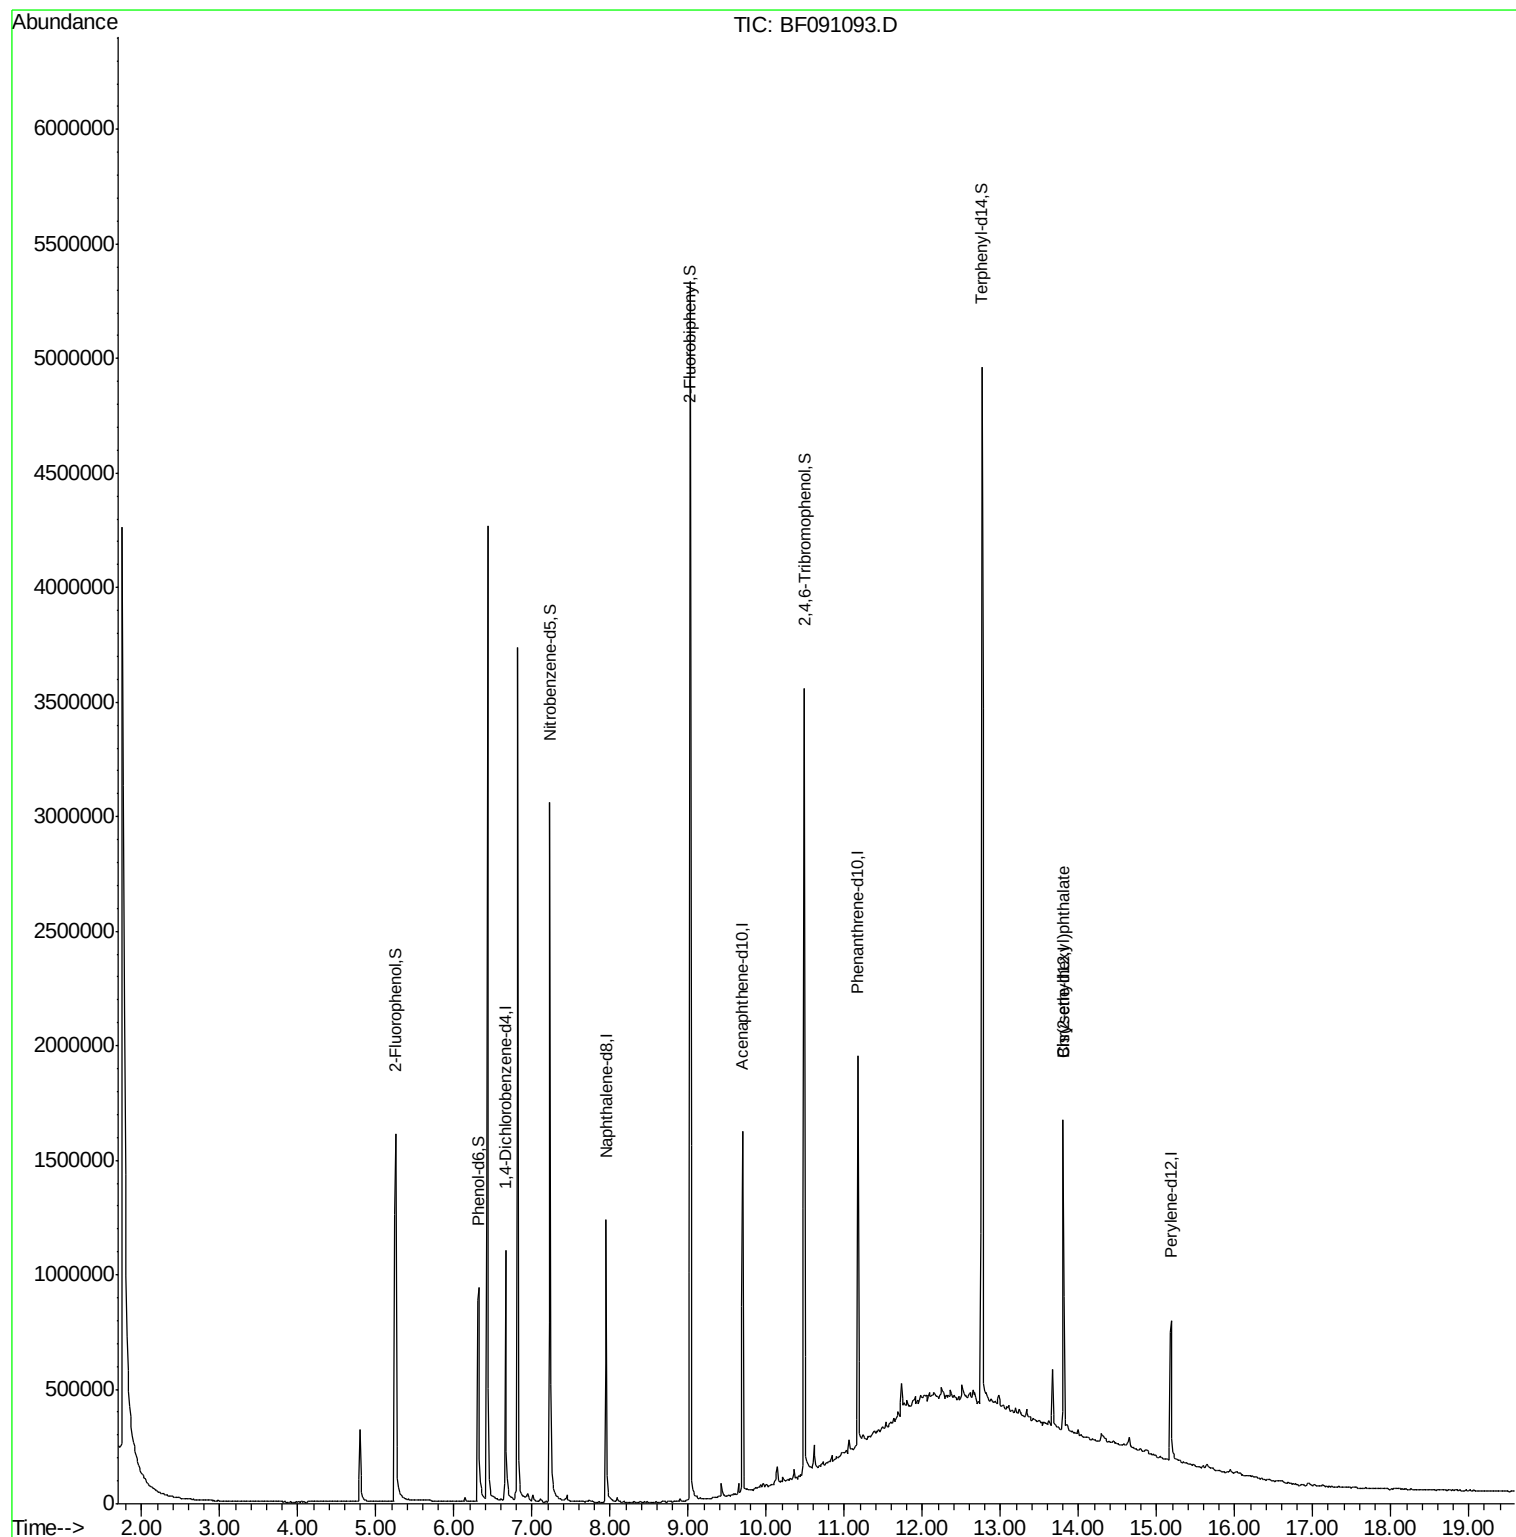

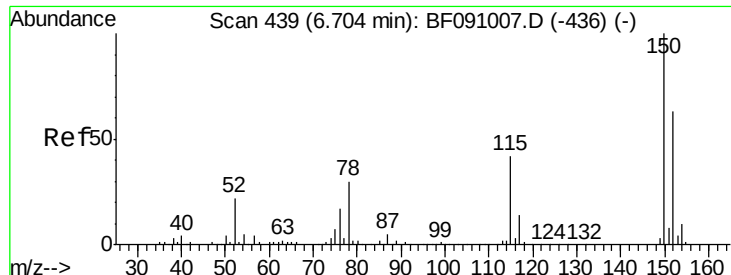

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.66 min Scan# 435

Delta R.T. -0.00 min

Lab File: BF091093.D

Acq: 8 Nov 2016 20:22

Instrument :

BNA_F

ClientSampleId :

DRW2


Tot Ion:152 Resp: 170716

Ion Ratio Lower Upper

152 100

150 159.2 126.8 190.2




115 67.7 53.3 79.9

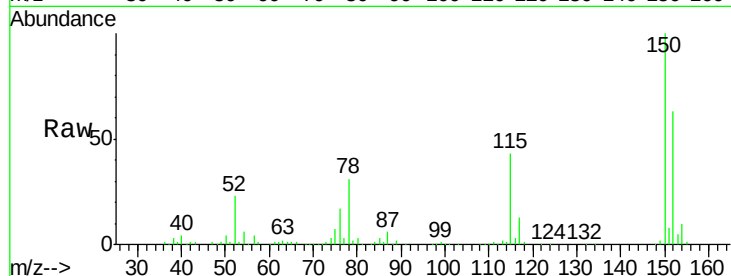

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

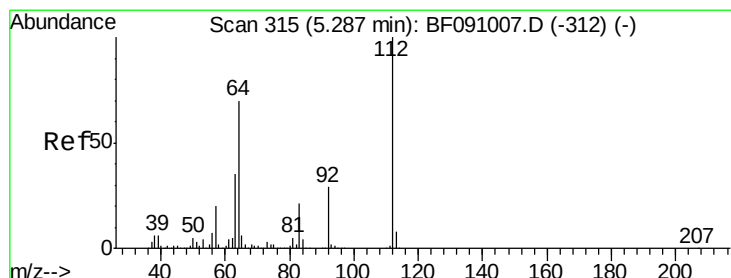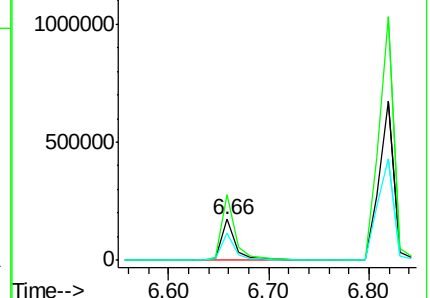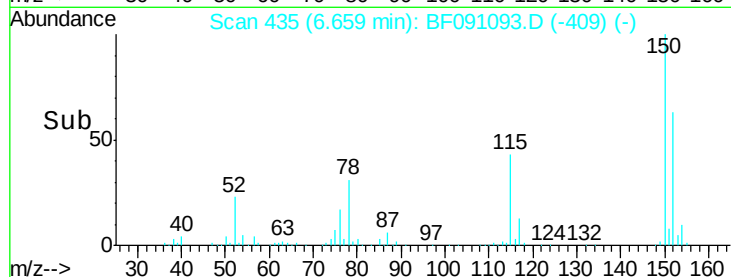

#5

2-Fluorophenol

Concen: 66.23 ng

RT: 5.25 min Scan# 312

Delta R.T. 0.01 min

Lab File: BF091093.D

Acq: 8 Nov 2016 20:22


Tgt Ion:112 Resp: 684646

Ion Ratio Lower Upper

112 100

64 55.5 55.8 83.6#



63 27.7 28.0 42.0#

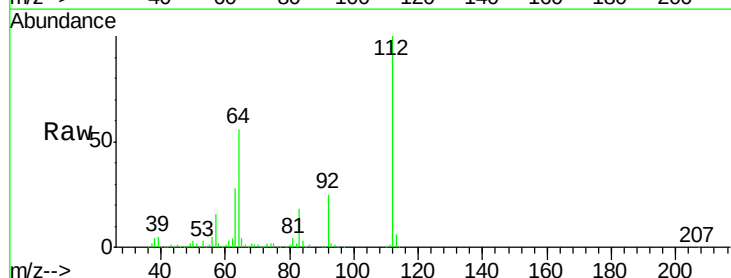


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

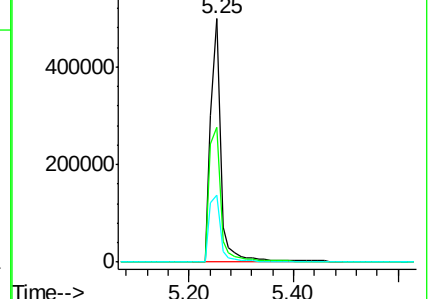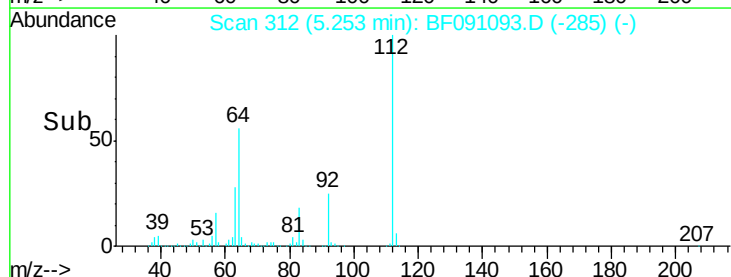

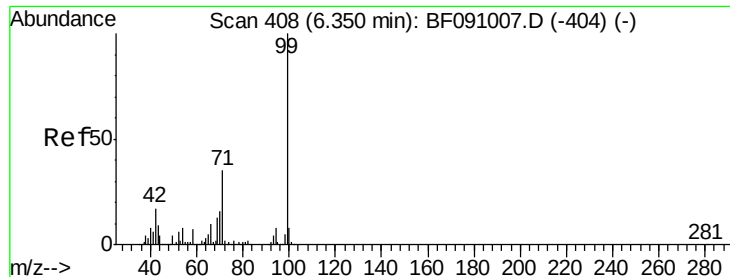

#7

Phenol-d6

Concen: 40.09 ng

RT: 6.32 min Scan# 405

Delta R.T. -0.00 min

Lab File: BF091093.D

Acq: 8 Nov 2016 20:22

Instrument :

BNA_F

ClientSampleId :

DRW2


Tot Ion: 99 Resp: 562508

Ion Ratio Lower Upper




99 100

42 13.8 13.9 20.9#

71 29.8 27.8 41.8

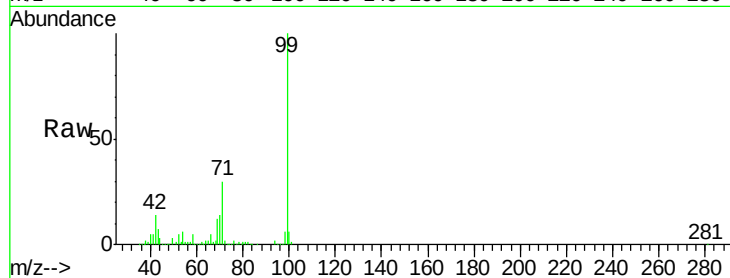

Abundance Ion 99.00 (98.70 to 99.70): BF0
Ion 42.00 (41.70 to 42.70): BF0
Ion 71.00 (70.70 to 71.70): BF0

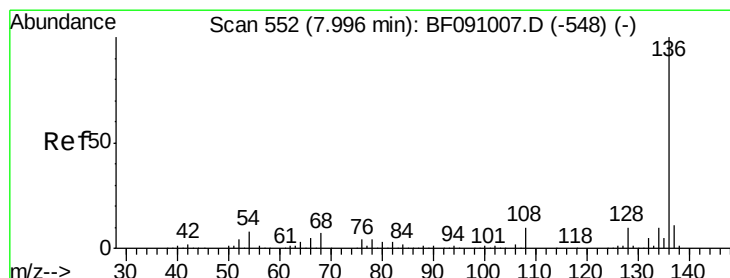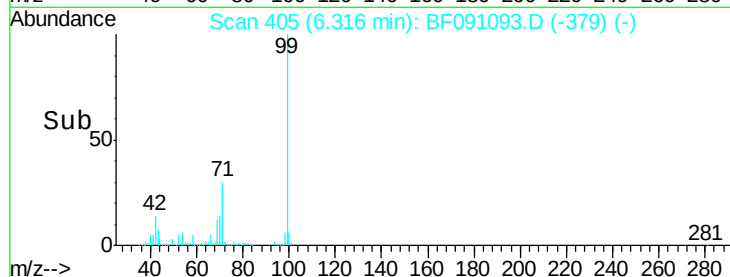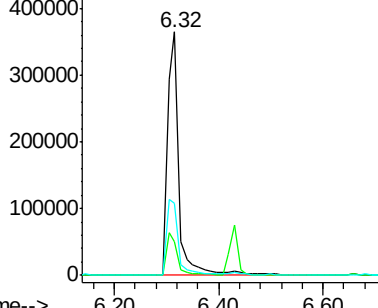

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.95 min Scan# 548

Delta R.T. -0.00 min

Lab File: BF091093.D

Acq: 8 Nov 2016 20:22

Tgt Ion: 136 Resp: 712076


Ion Ratio Lower Upper

136 100



137 10.9 8.9 13.3


54 6.8 6.2 9.2

68 6.0 5.5 8.3

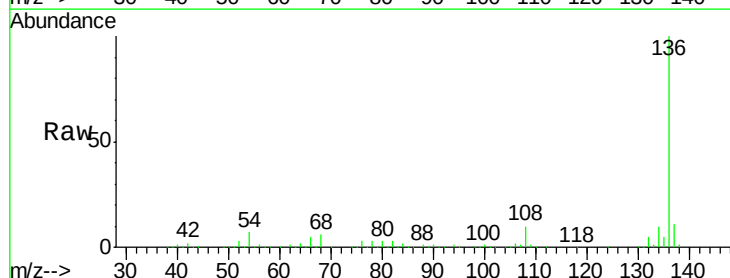

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF0
Ion 68.00 (67.70 to 68.70): BF0

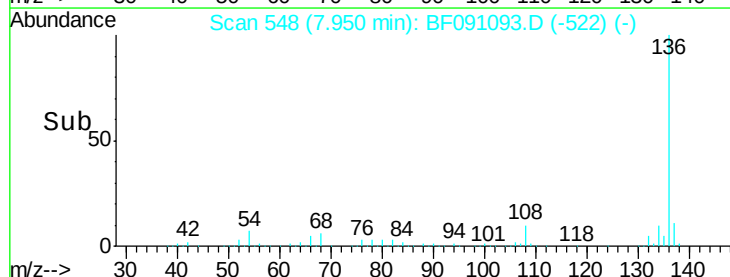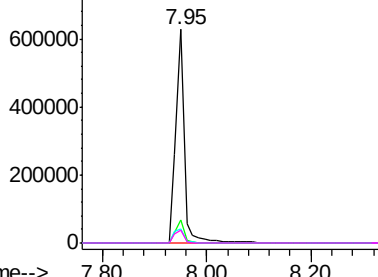


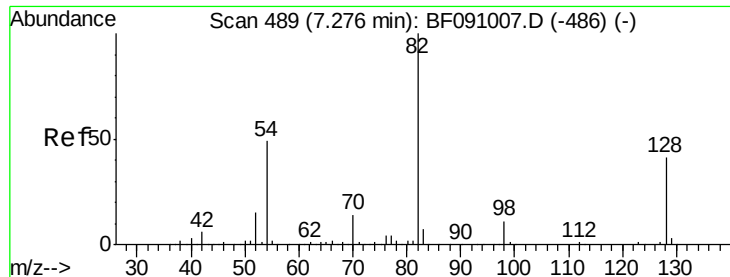




#23
 Nitrobenzene-d5
 Concen: 91.50 ng
 RT: 7.23 min Scan# 485
 Delta R.T. -0.01 min
 Lab File: BF091093.D
 Acq: 8 Nov 2016 20:22

Instrument :
 BNA_F
 ClientSampleID :
 DRW2

Tot Ion: 82 Resp: 1194446
 Ion Ratio Lower Upper
 82 100
 128 40.3 32.4 48.6
 54 49.6 39.2 58.8

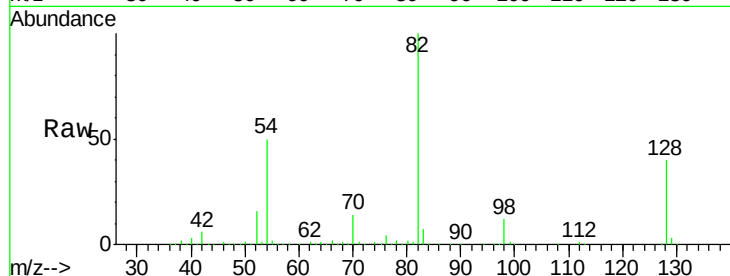


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): B
 Ion 54.00 (53.70 to 54.70): BF0

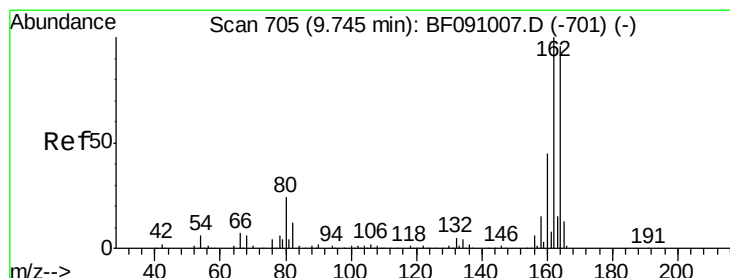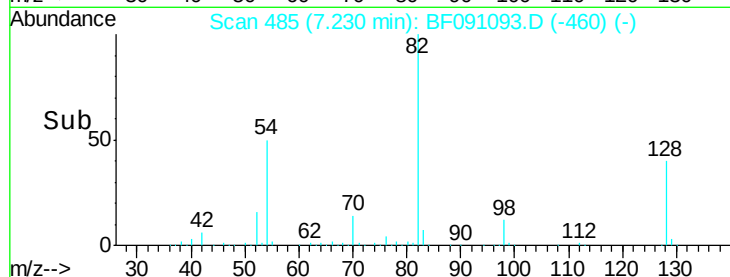
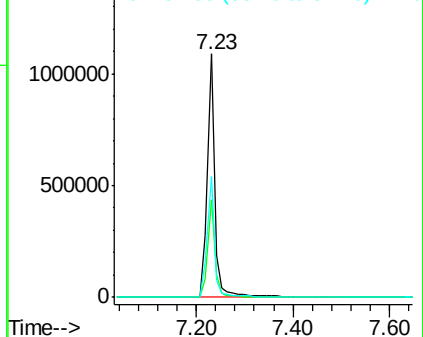



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.70 min Scan# 701
 Delta R.T. -0.00 min
 Lab File: BF091093.D
 Acq: 8 Nov 2016 20:22

Tgt Ion: 164 Resp: 393162
 Ion Ratio Lower Upper
 164 100
 162 103.1 83.6 125.4
 160 46.6 37.9 56.9

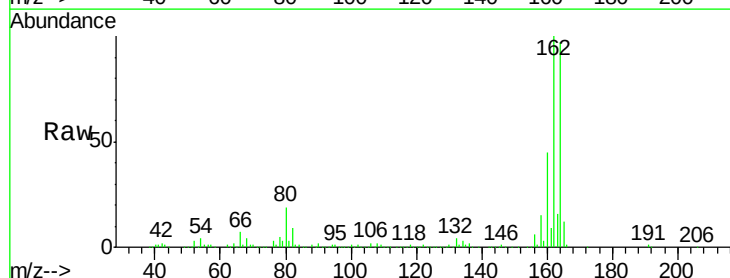

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

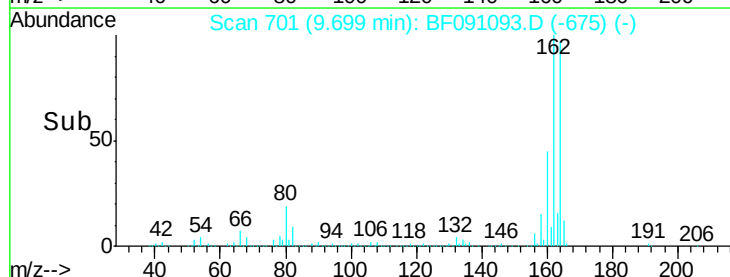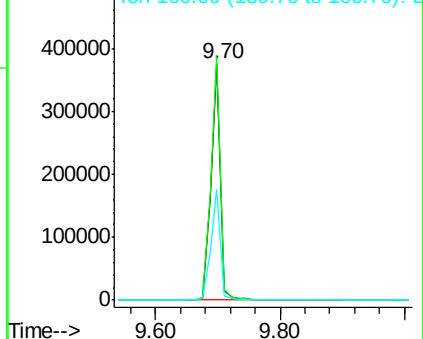


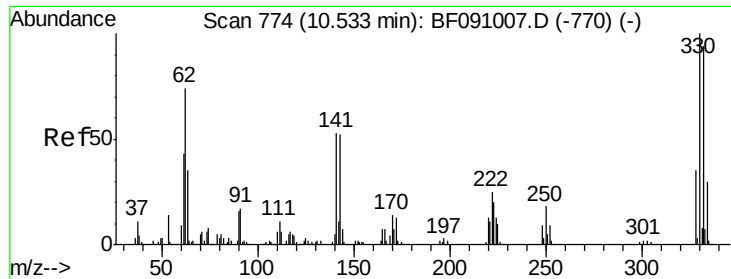




#41
 2,4,6-Tribromophenol
 Concen: 131.28 ng
 RT: 10.49 min Scan# 770
 Delta R.T. -0.00 min
 Lab File: BF091093.D
 Acq: 8 Nov 2016 20:22

Instrument :
 BNA_F
 ClientSampleId :
 DRW2

Tot Ion:330 Resp: 466612
 Ion Ratio Lower Upper
 330 100
 332 96.1 75.9 113.9
 141 37.0 36.1 54.1

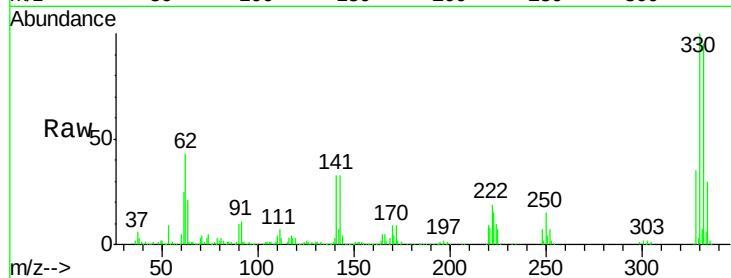


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

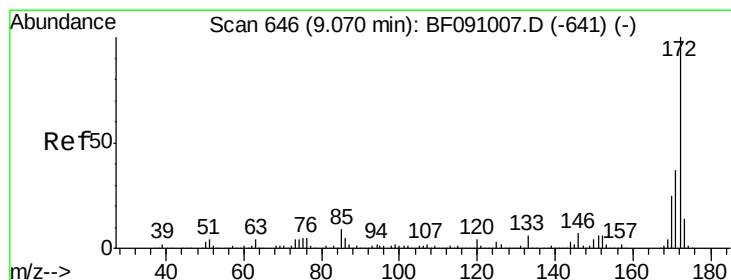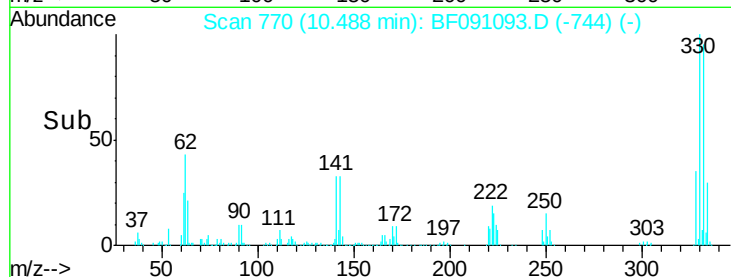
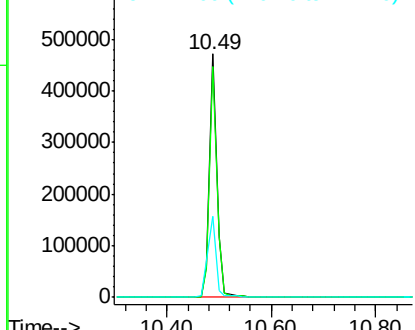



#44
 2-Fluorobiphenyl
 Concen: 81.37 ng
 RT: 9.02 min Scan# 642
 Delta R.T. -0.01 min
 Lab File: BF091093.D
 Acq: 8 Nov 2016 20:22

Tgt Ion:172 Resp: 1858212
 Ion Ratio Lower Upper
 172 100
 171 37.4 29.8 44.6
 170 25.8 20.3 30.5

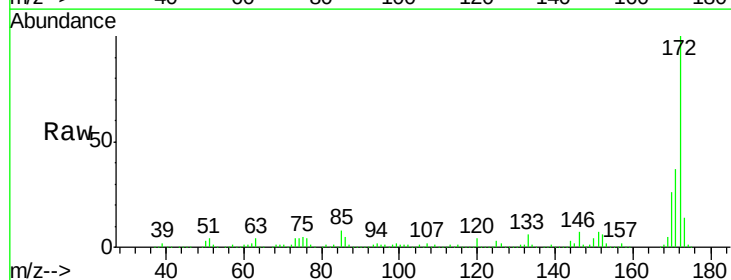

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

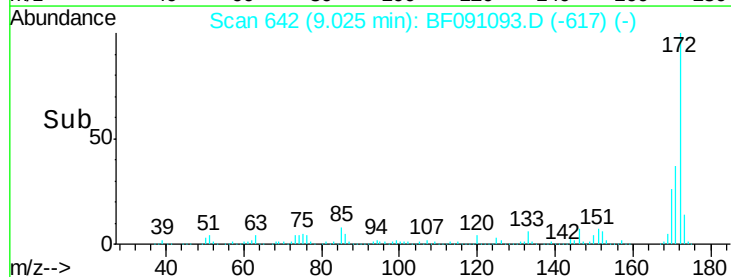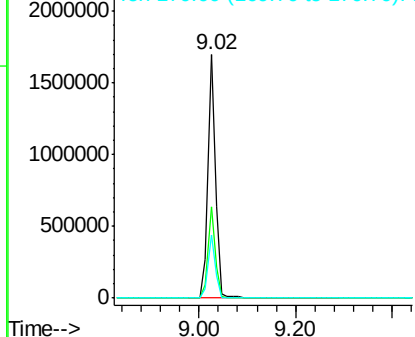

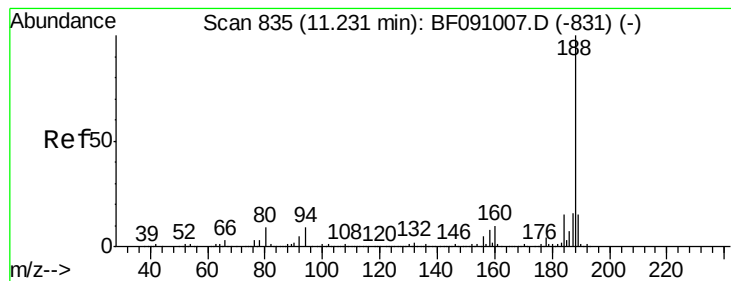

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.17 min Scan# 830

Delta R.T. -0.00 min

Lab File: BF091093.D

Acq: 8 Nov 2016 20:22

Instrument :

BNA_F

ClientSampleId :

DRW2


Tot Ion:188 Resp: 609955

Ion Ratio Lower Upper

188 100

94 13.7 7.0 10.4#




80 15.1 7.5 11.3#

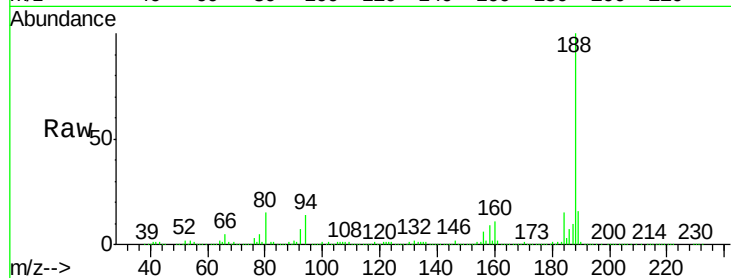

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

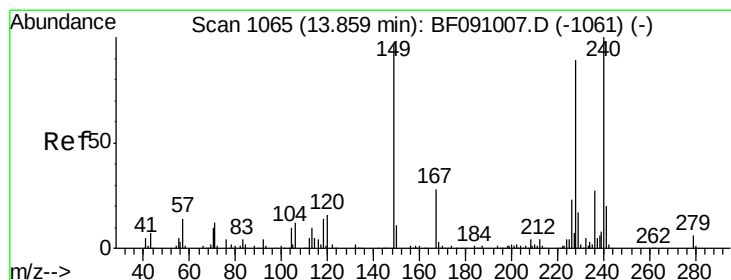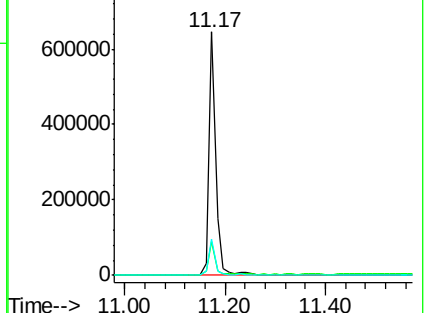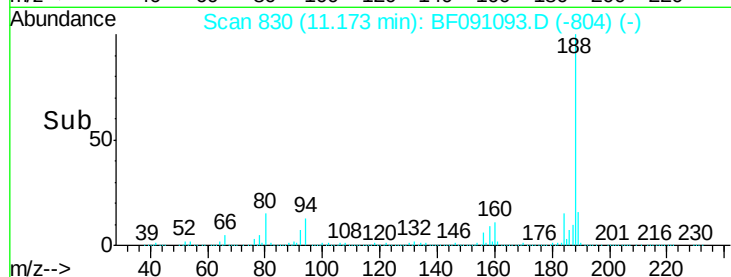

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.80 min Scan# 1060

Delta R.T. -0.01 min

Lab File: BF091093.D

Acq: 8 Nov 2016 20:22


Tgt Ion:240 Resp: 448272

Ion Ratio Lower Upper

240 100

120 19.0 12.9 19.3



236 27.4 21.9 32.9

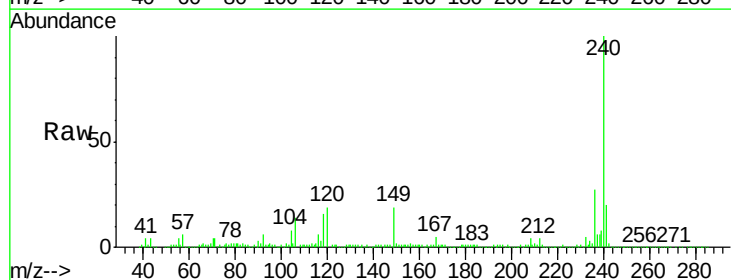


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

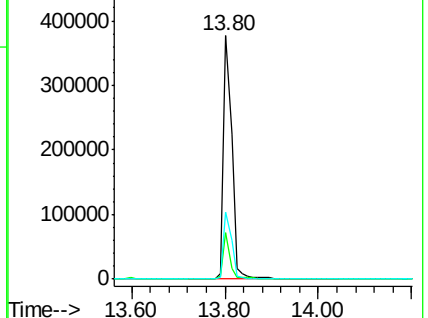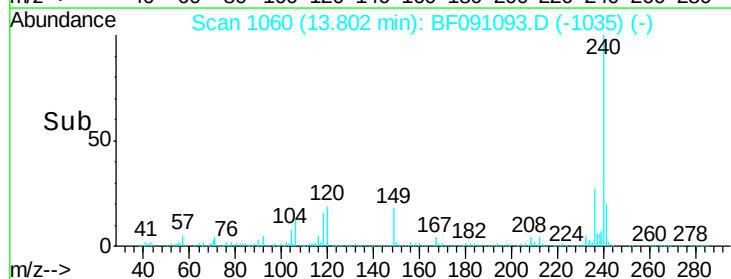

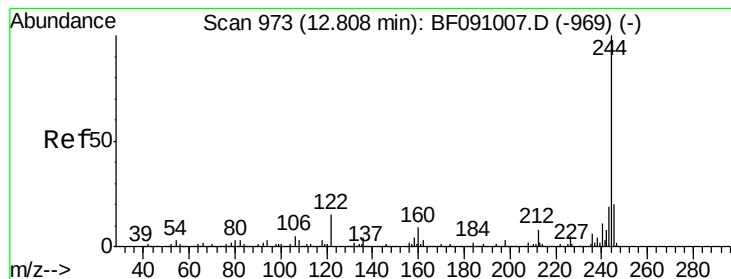

#78

Terphenyl-d14

Concen: 111.79 ng

RT: 12.76 min Scan# 969

Delta R.T. -0.00 min

Lab File: BF091093.D

Acq: 8 Nov 2016 20:22

Instrument :

BNA_F

ClientSampleId :

DRW2


Tot Ion:244 Resp: 2008208

Ion Ratio Lower Upper

244 100

212 7.9 6.4 9.6




122 14.2 12.3 18.5

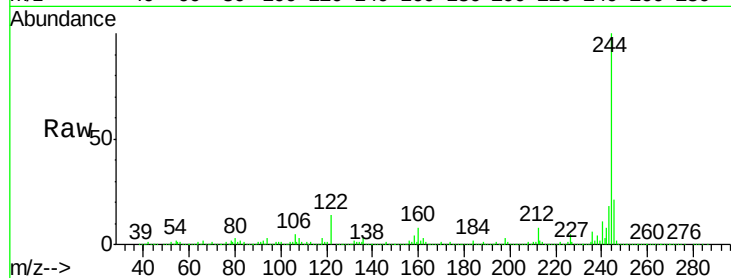

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

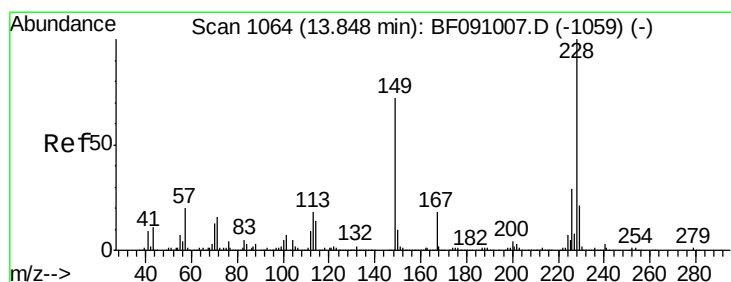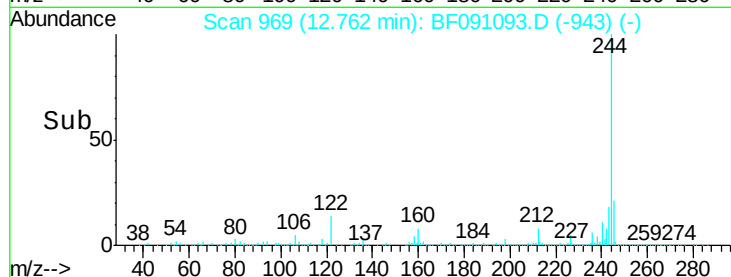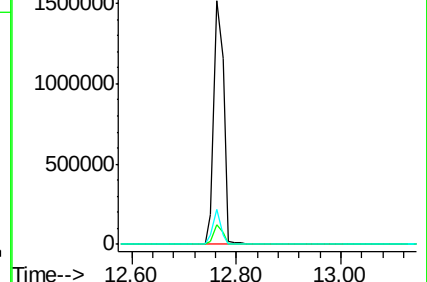

#83

Bis(2-ethylhexyl)phthalate

Concen: 3.10 ng

RT: 13.80 min Scan# 1060

Delta R.T. -0.00 min

Lab File: BF091093.D

Acq: 8 Nov 2016 20:22


Tgt Ion:149 Resp: 58983

Ion Ratio Lower Upper

149 100

167 25.5 20.4 30.6



279 2.4 1.6 2.4#



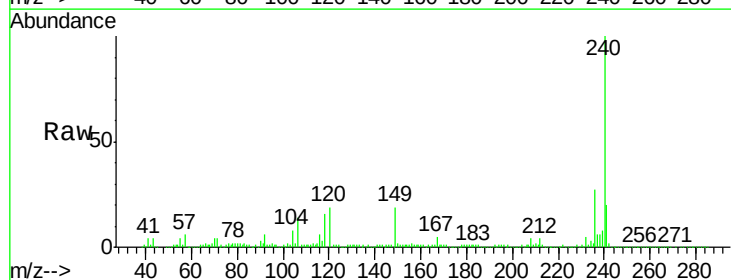


Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

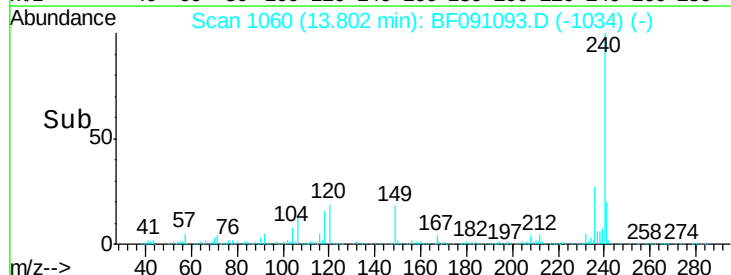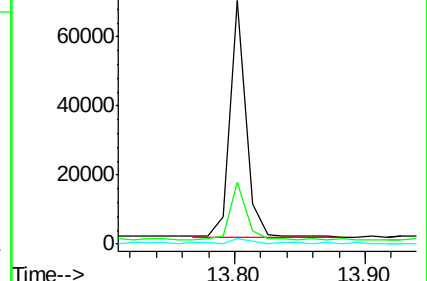

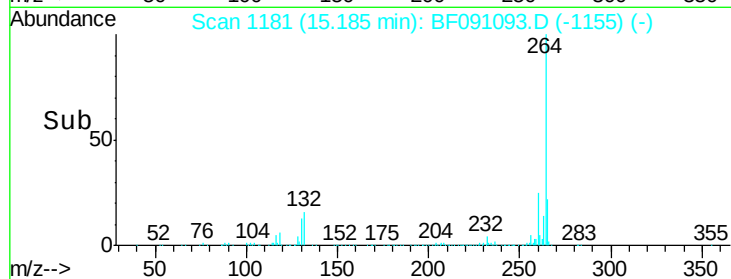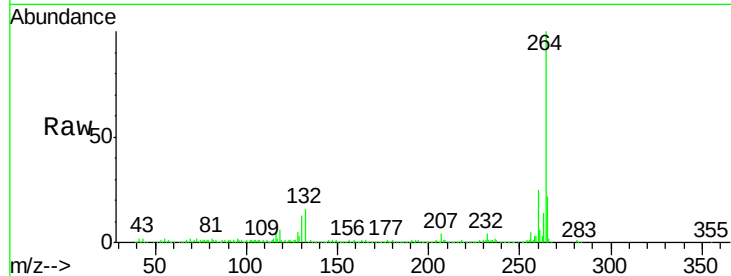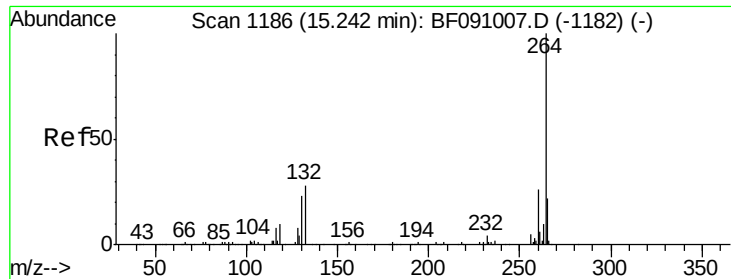

#86
 Pervlene-d12
 Concen: 20.00 ng
 RT: 15.19 min Scan# 1181
 Delta R.T. -0.00 min
 Lab File: BF091093.D
 Acq: 8 Nov 2016 20:22

Instrument :
 BNA_F
 ClientSampleId :
 DRW2

Tot Ion	Ratio	Lower	Upper
264	100		
260	25.3	20.6	30.8
265	21.8	17.8	26.8

