

Data Path : Z:\HPCHEM1\BNA F\DATA\BF110816\
 Data File : BF091095.D
 Acq On : 8 Nov 2016 21:17
 Operator : UM/SJ
 Sample : PB94606BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB94606BL

Quant Time: Nov 09 02:32:09 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110316.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 08 12:59:29 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.66	152	178352	20.00	ng	0.00
21) Naphthalene-d8	7.95	136	720370	20.00	ng	0.00
38) Acenaphthene-d10	9.70	164	384682	20.00	ng	0.00
63) Phenanthrene-d10	11.17	188	657357	20.00	ng	0.00
75) Chrysene-d12	13.80	240	516547	20.00	ng	-0.01
86) Perylene-d12	15.19	264	368198	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.25	112	1303131	120.67	ng	0.01
7) Phenol-d6	6.32	99	1552741	105.93	ng	0.00
23) Nitrobenzene-d5	7.23	82	1105605	83.72	ng	-0.01
41) 2,4,6-Tribromophenol	10.49	330	440228	126.58	ng	0.00
44) 2-Fluorobiphenyl	9.02	172	1669016	74.70	ng	-0.01
78) Terphenyl-d14	12.76	244	1798094	86.87	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF110816\
Data File : BF091095.D
Acq On : 8 Nov 2016 21:17
Operator : UM/SJ
Sample : PB94606BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB94606BL

Quant Time: Nov 09 02:32:09 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 08 12:59:29 2016
Response via : Initial Calibration

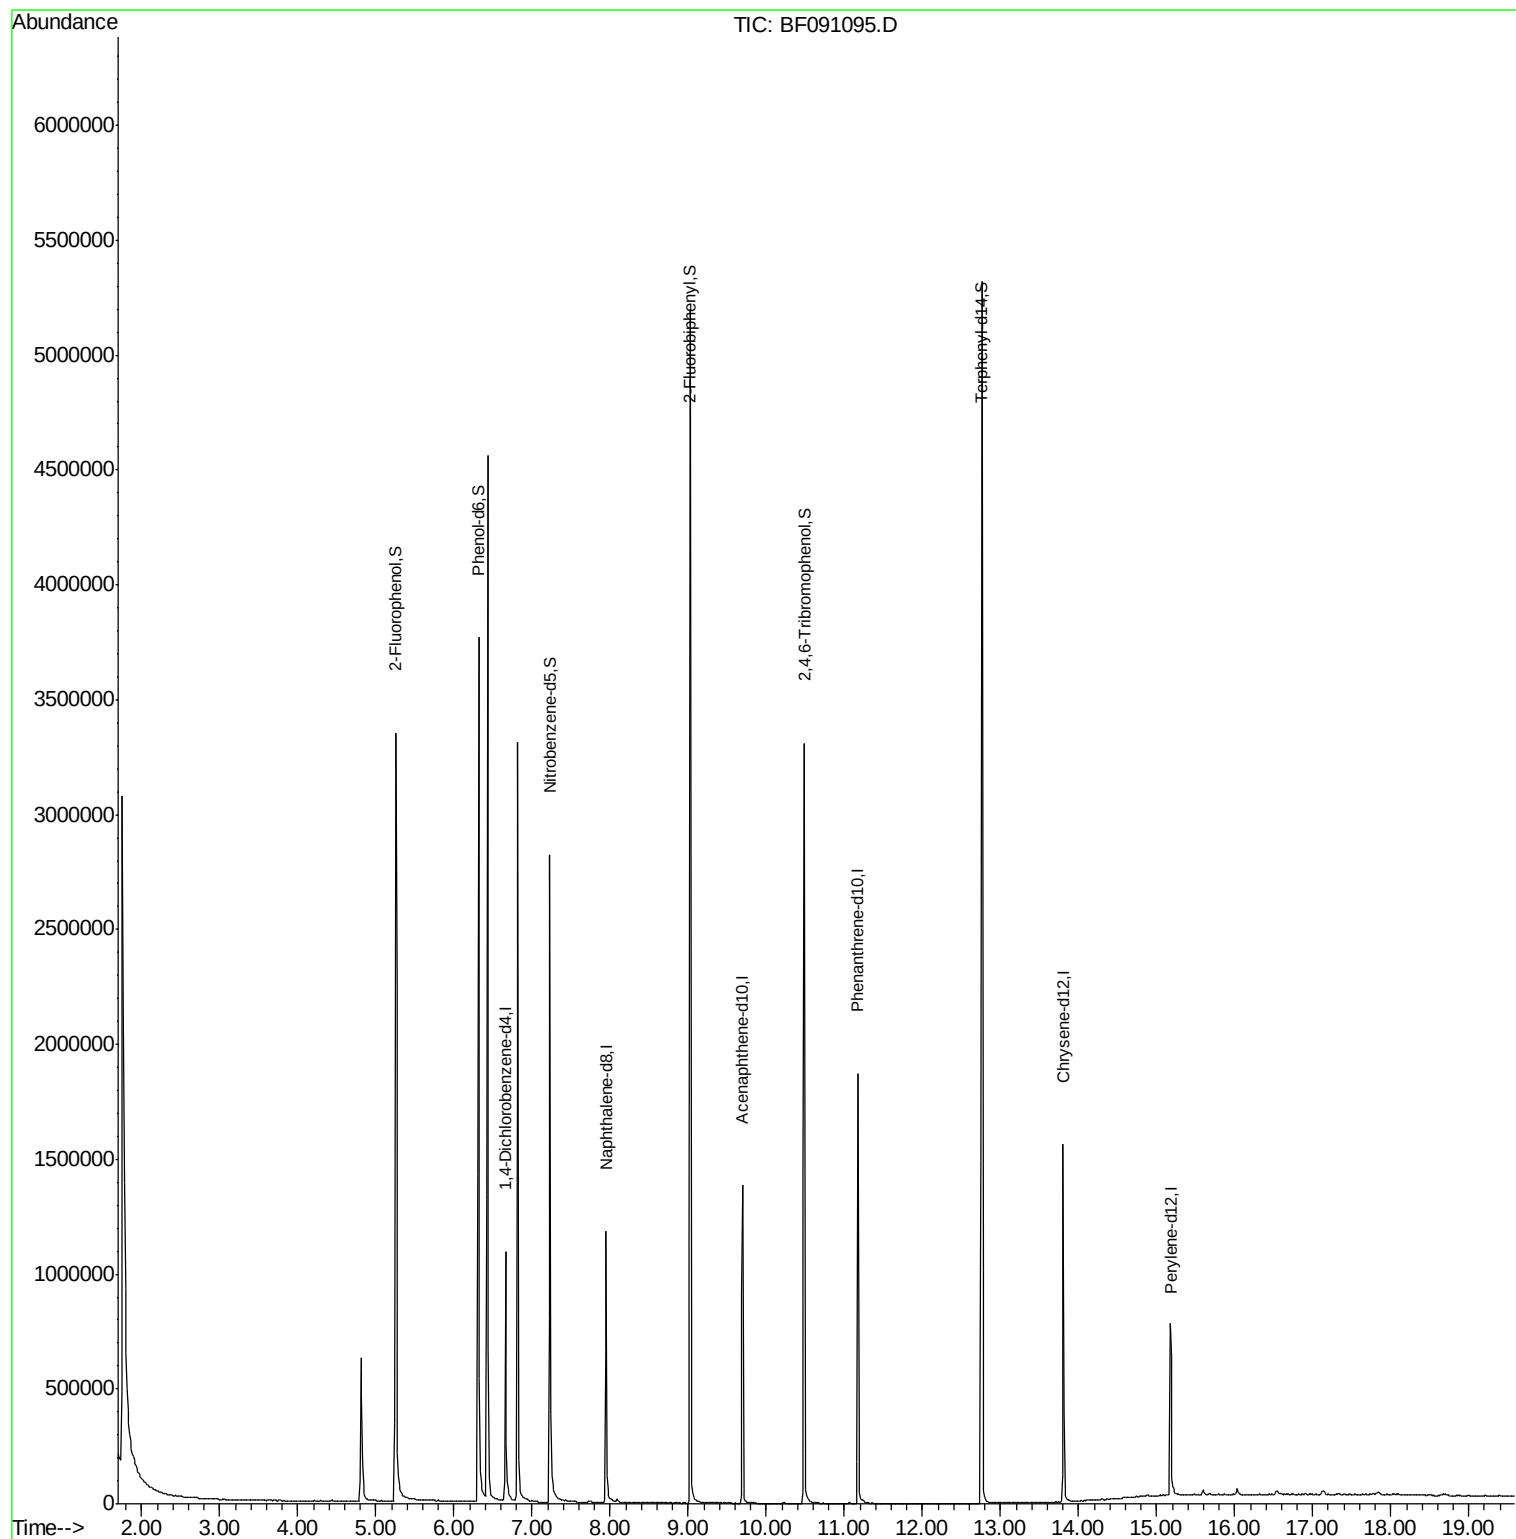




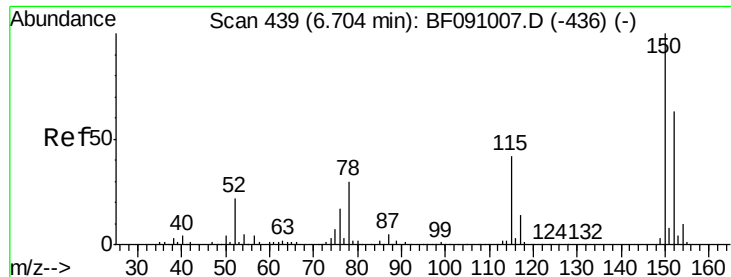


#1

1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.66 min Scan# 435
Delta R.T. 0.00 min
Lab File: BF091095.D
Acq: 8 Nov 2016 21:17

Instrument :
BNA_F
ClientSampleId :
PB94606BL




Tot Ion:152 Resp: 178352
Ion Ratio Lower Upper
152 100
150 156.7 126.8 190.2
115 67.1 53.3 79.9

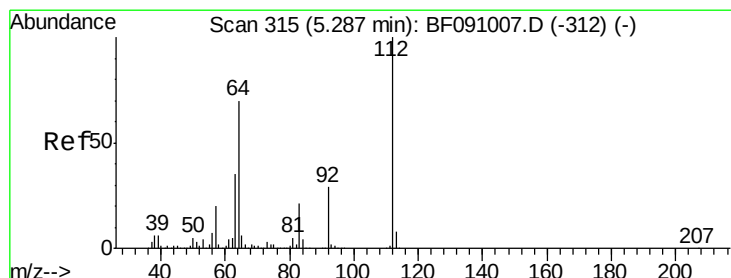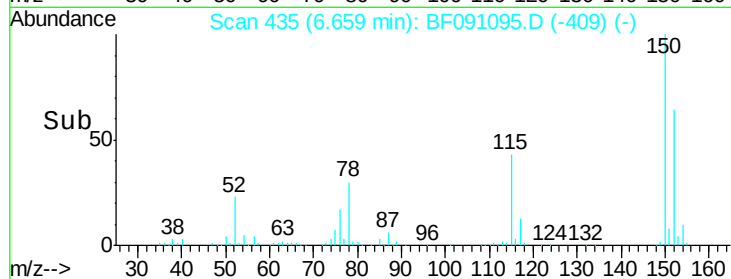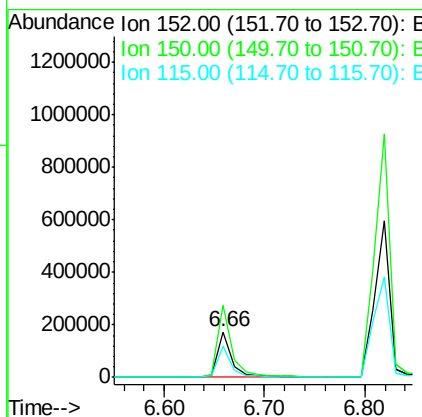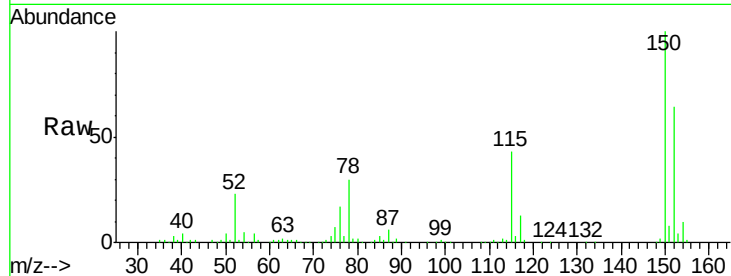


#5

2-Fluorophenol
Concen: 120.67 ng
RT: 5.25 min Scan# 312
Delta R.T. 0.01 min
Lab File: BF091095.D
Acq: 8 Nov 2016 21:17

Tgt Ion:112 Resp: 1303131
Ion Ratio Lower Upper
112 100
64 69.0 55.8 83.6
63 34.8 28.0 42.0

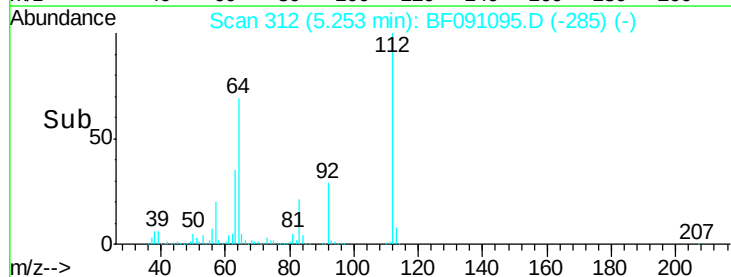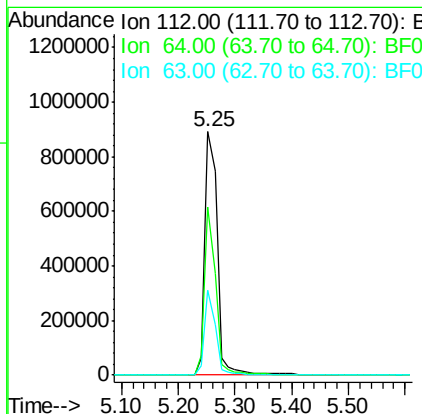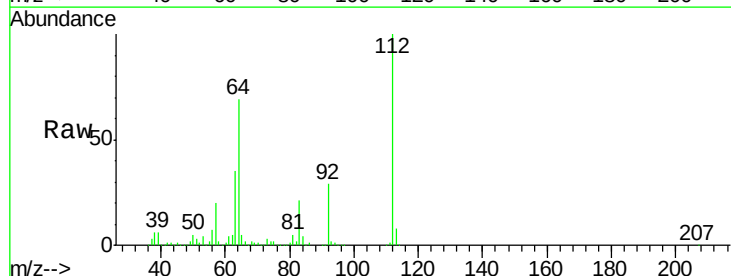

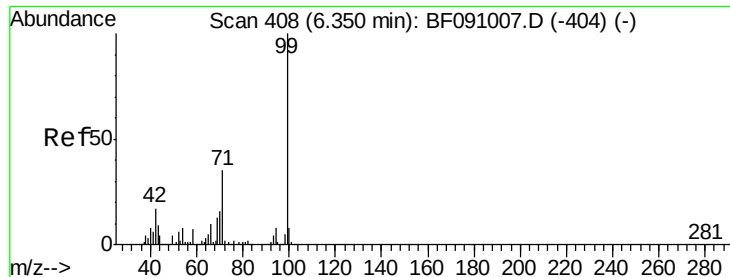

#7

Phenol-d6

Concen: 105.93 ng

RT: 6.32 min Scan# 405

Delta R.T. 0.00 min

Lab File: BF091095.D

Acq: 8 Nov 2016 21:17

Instrument :

BNA_F

ClientSampleId :

PB94606BL


Tot Ion: 99 Resp: 1552741

Ion Ratio Lower Upper

99 100

42 17.4 13.9 20.9




71 34.5 27.8 41.8

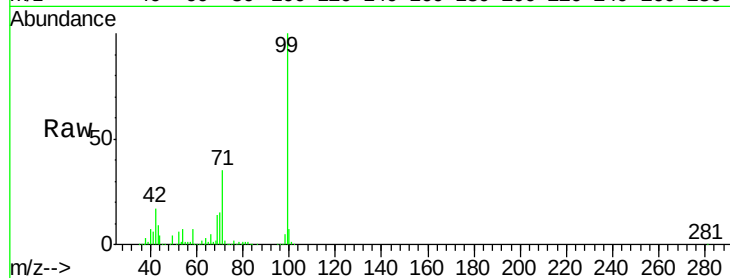

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

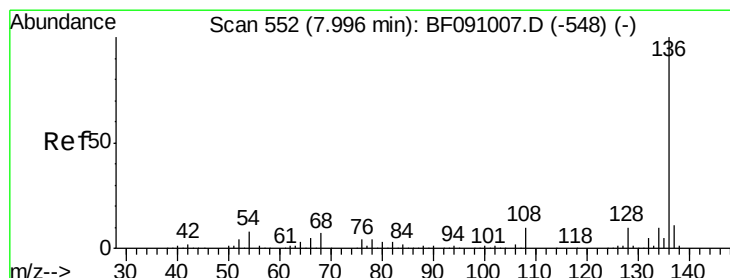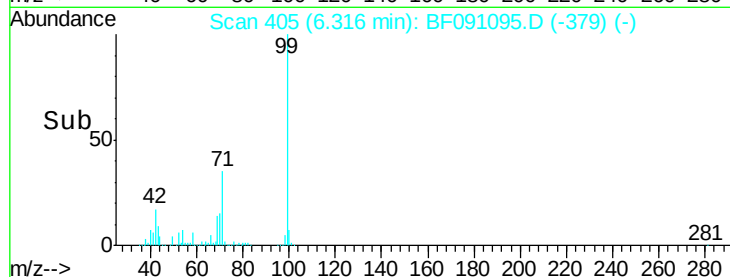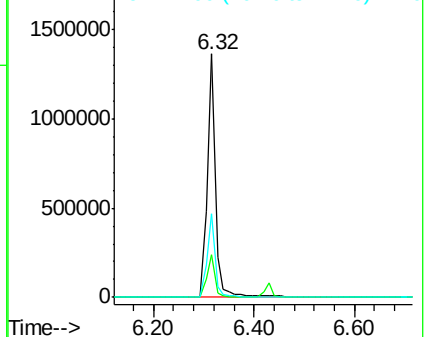

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.95 min Scan# 548

Delta R.T. 0.00 min

Lab File: BF091095.D

Acq: 8 Nov 2016 21:17

Tgt Ion: 136 Resp: 720370


Ion Ratio Lower Upper

136 100

137 10.9 8.9 13.3

54 6.7 6.2 9.2

68 5.8 5.5 8.3


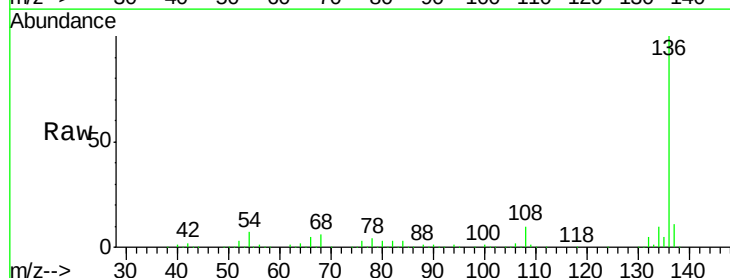



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

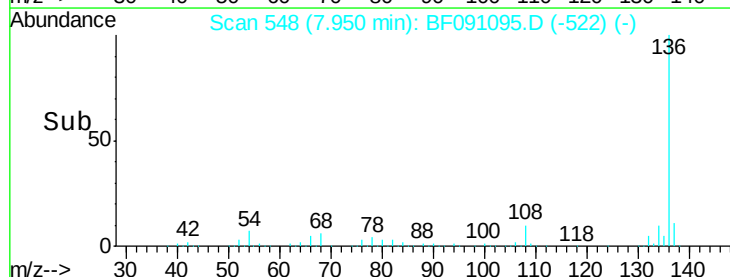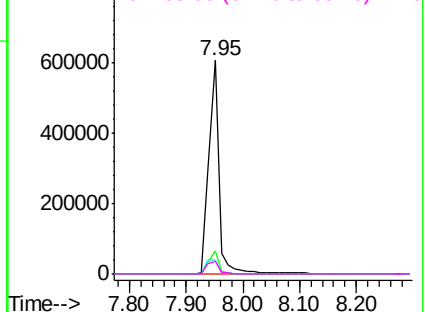


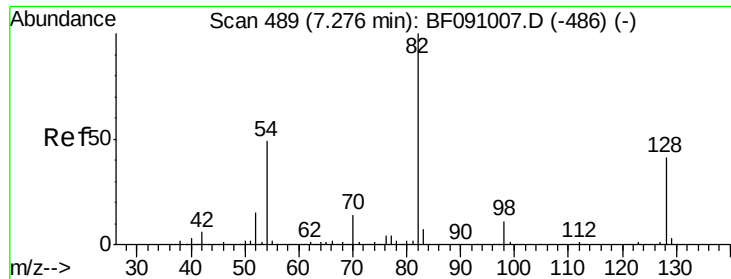




#23
Nitrobenzene-d5
Concen: 83.72 ng
RT: 7.23 min Scan# 485
Delta R.T. -0.01 min
Lab File: BF091095.D
Acq: 8 Nov 2016 21:17

Instrument :
BNA_F
ClientSampleId :
PB94606BL

Tot Ion: 82 Resp: 1105605
Ion Ratio Lower Upper
82 100
128 41.3 32.4 48.6
54 48.9 39.2 58.8

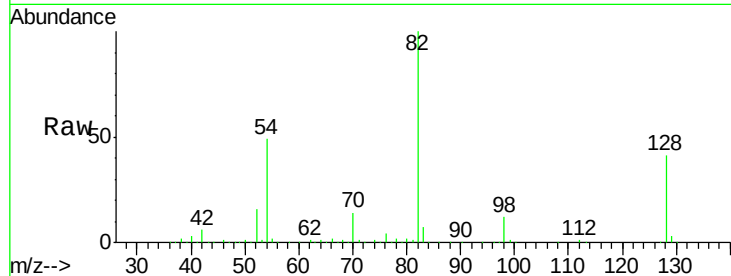


Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): BF0
Ion 54.00 (53.70 to 54.70): BF0

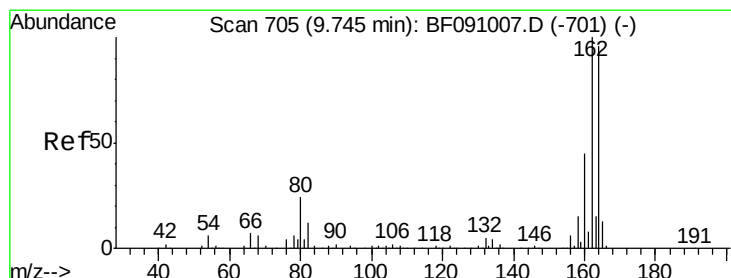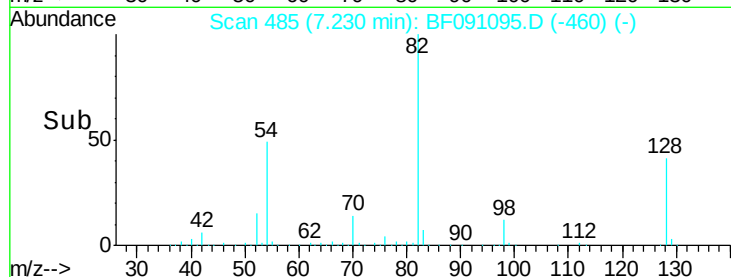
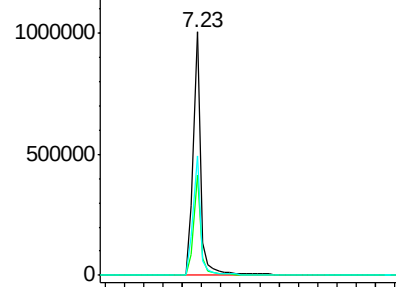



#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.70 min Scan# 701
Delta R.T. 0.00 min
Lab File: BF091095.D
Acq: 8 Nov 2016 21:17

Tgt Ion:164 Resp: 384682
Ion Ratio Lower Upper
164 100
162 103.2 83.6 125.4
160 46.7 37.9 56.9

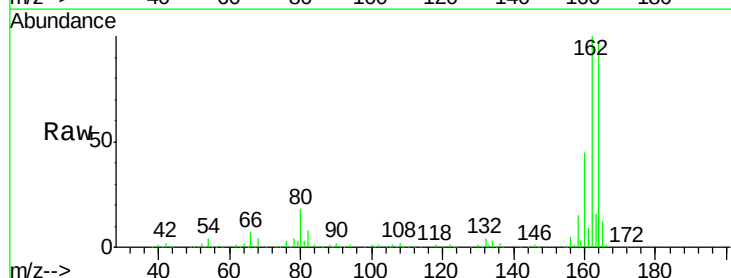

Abundance Ion 164.00 (163.70 to 164.70): BF0
Ion 162.00 (161.70 to 162.70): BF0
Ion 160.00 (159.70 to 160.70): BF0

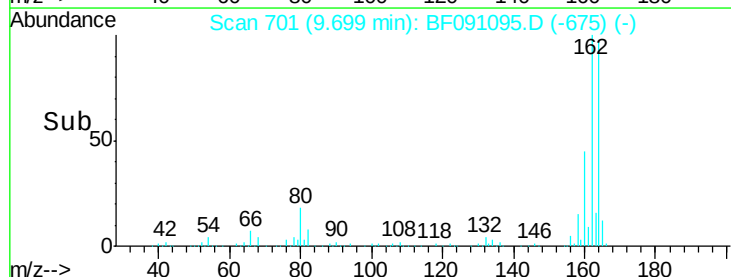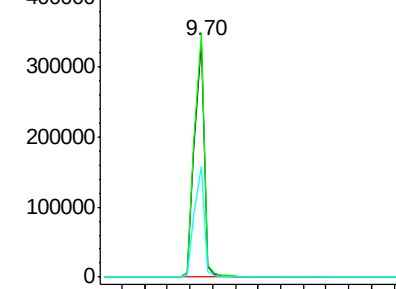


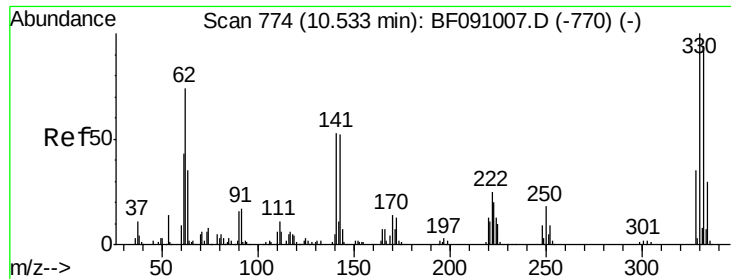




#41
 2,4,6-Tribromophenol
 Concen: 126.58 ng
 RT: 10.49 min Scan# 770
 Delta R.T. 0.00 min
 Lab File: BF091095.D
 Acq: 8 Nov 2016 21:17

Instrument :
 BNA_F
 ClientSampleId :
 PB94606BL

Tot Ion	Ratio	Lower	Upper
330	100		
332	94.8	75.9	113.9
141	39.0	36.1	54.1

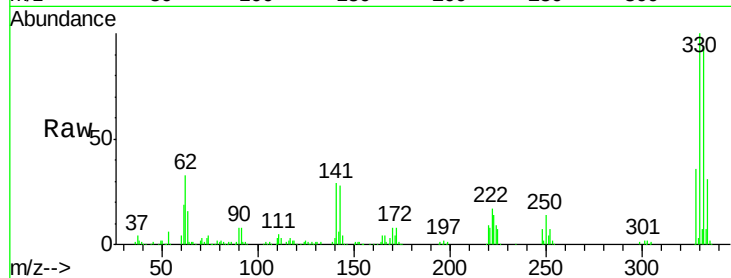


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

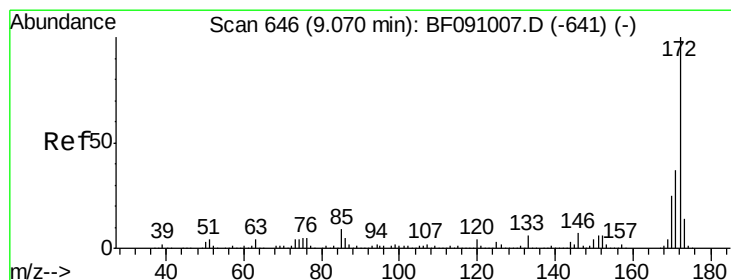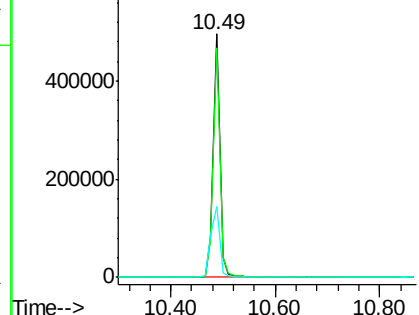
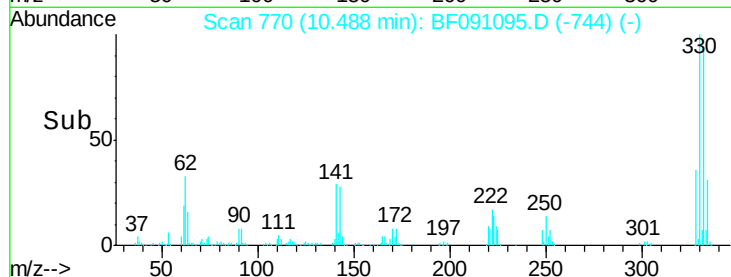



#44
 2-Fluorobiphenyl
 Concen: 74.70 ng
 RT: 9.02 min Scan# 642
 Delta R.T. -0.01 min
 Lab File: BF091095.D
 Acq: 8 Nov 2016 21:17

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.3	29.8	44.6
170	25.6	20.3	30.5

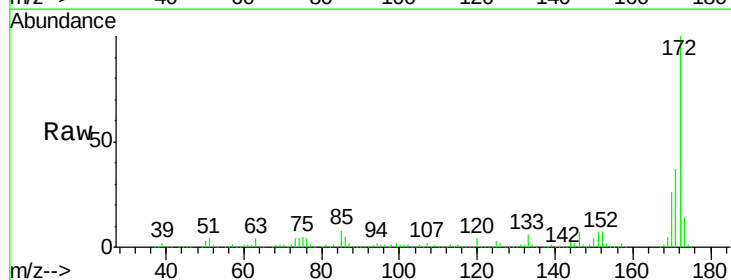

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

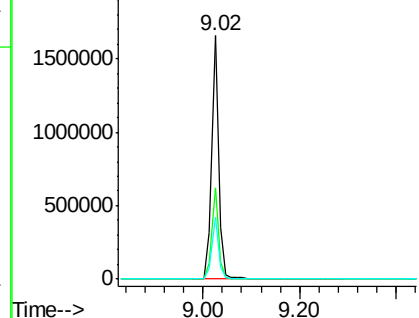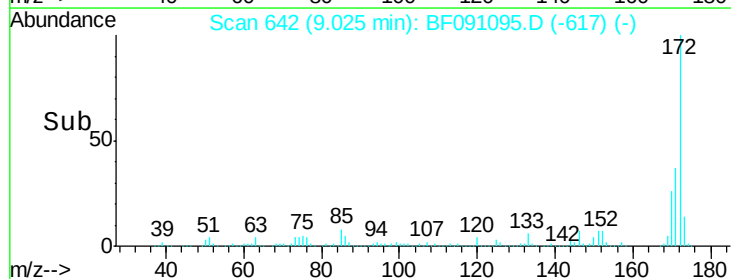


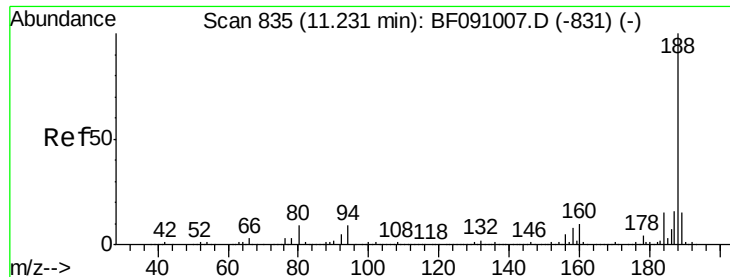




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.17 min Scan# 830
Delta R.T. 0.00 min
Lab File: BF091095.D
Acq: 8 Nov 2016 21:17

Instrument :
BNA_F
ClientSampleId :
PB94606BL

Tot Ion:188 Resp: 657357
Ion Ratio Lower Upper
188 100
94 12.4 7.0 10.4#
80 13.7 7.5 11.3#

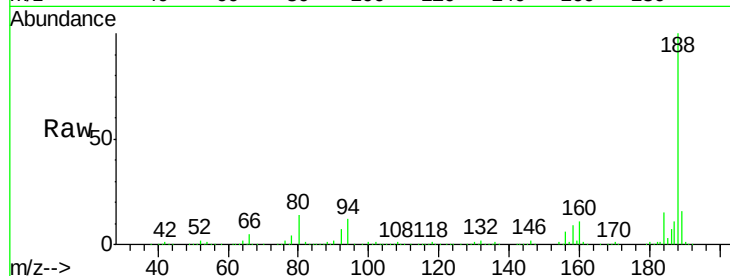


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

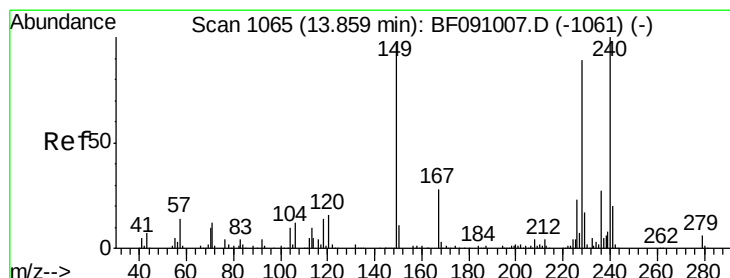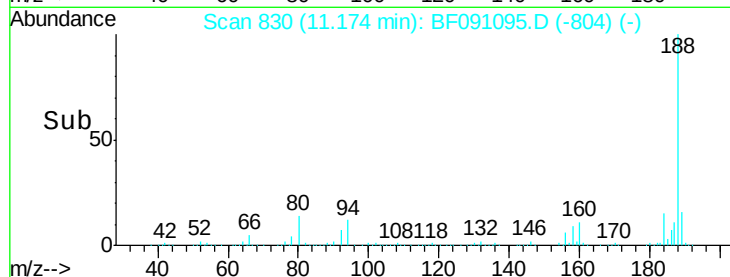
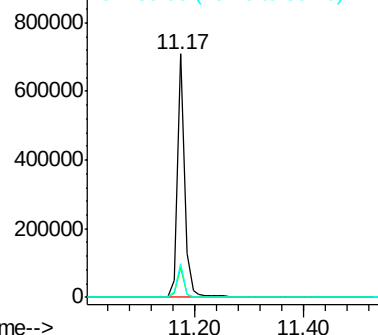



#75
Chrysene-d12
Concen: 20.00 ng
RT: 13.80 min Scan# 1060
Delta R.T. -0.01 min
Lab File: BF091095.D
Acq: 8 Nov 2016 21:17

Tgt Ion:240 Resp: 516547
Ion Ratio Lower Upper
240 100
120 16.5 12.9 19.3
236 27.6 21.9 32.9

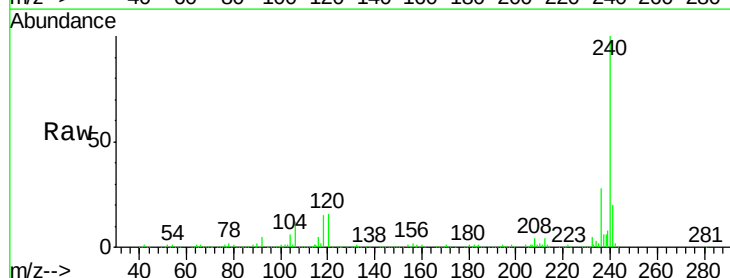

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E



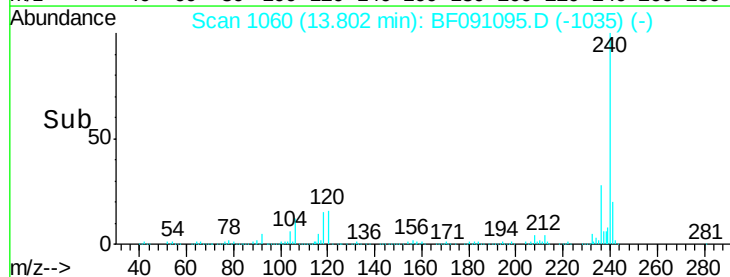
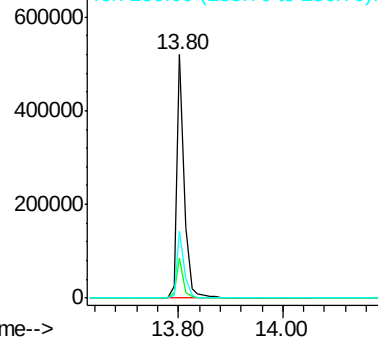


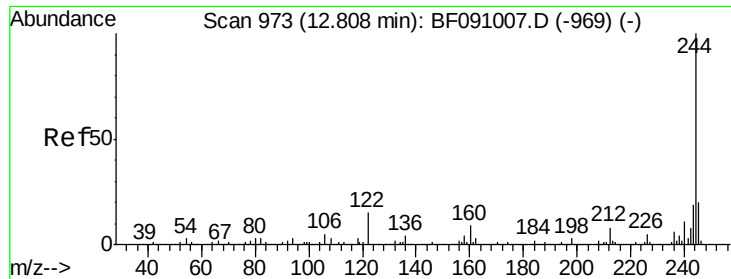

#78
 Terphenyl-d14
 Concen: 86.87 ng
 RT: 12.76 min Scan# 969
 Delta R.T. 0.00 min
 Lab File: BF091095.D
 Acq: 8 Nov 2016 21:17

Instrument :
 BNA_F
 ClientSampleId :
 PB94606BL

Tot Ion:244 Resp: 1798094
 Ion Ratio Lower Upper
 244 100
 212 7.7 6.4 9.6
 122 13.0 12.3 18.5

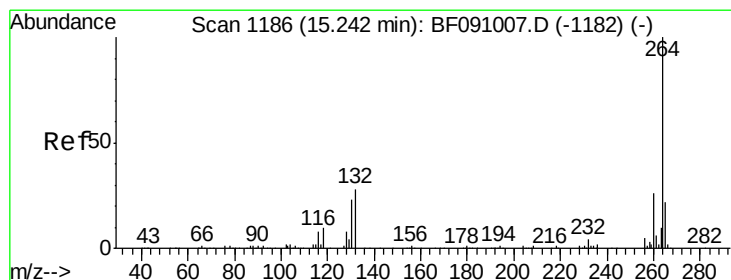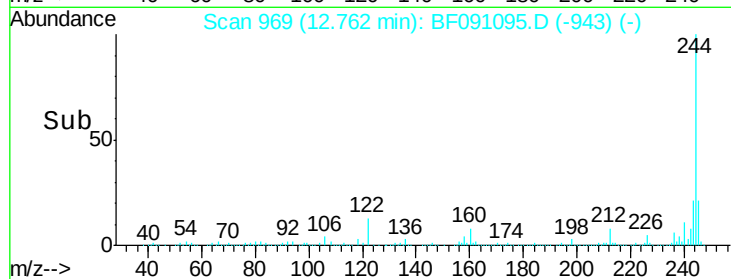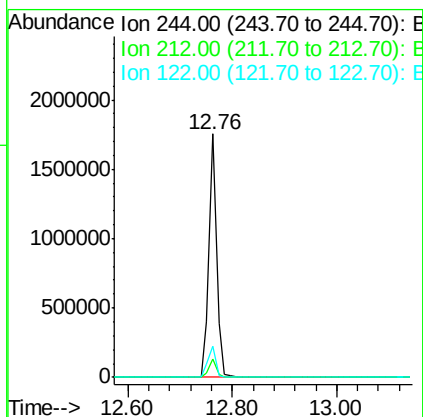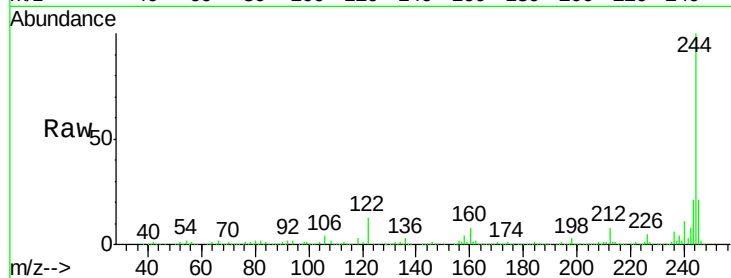

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.19 min Scan# 1181
 Delta R.T. 0.00 min
 Lab File: BF091095.D
 Acq: 8 Nov 2016 21:17

Tgt Ion:264 Resp: 368198
 Ion Ratio Lower Upper
 264 100
 260 25.0 20.6 30.8
 265 21.5 17.8 26.8

