

Data Path : Z:\HPCHEM1\BNA F\DATA\BF110816\
 Data File : BF091108.D
 Acq On : 9 Nov 2016 4:10
 Operator : UM/SJ
 Sample : H5593-04
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 NORTH-SIDEWALL

Quant Time: Nov 09 06:14:50 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110316.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 08 12:59:29 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.66	152	183126	20.00	ng	0.00
21) Naphthalene-d8	7.95	136	746762	20.00	ng	0.00
38) Acenaphthene-d10	9.70	164	370978	20.00	ng	0.00
63) Phenanthrene-d10	11.17	188	524768	20.00	ng	0.00
75) Chrysene-d12	13.80	240	361094	20.00	ng	-0.01
86) Perylene-d12	15.19	264	346438	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.25	112	1265322	114.12	ng	0.01
7) Phenol-d6	6.32	99	1584673	105.29	ng	0.00
23) Nitrobenzene-d5	7.23	82	1012586	73.97	ng	-0.01
41) 2,4,6-Tribromophenol	10.49	330	337552	100.65	ng	0.00
44) 2-Fluorobiphenyl	9.02	172	1420540	65.92	ng	-0.01
78) Terphenyl-d14	12.76	244	1092224	75.48	ng	0.00
Target Compounds						
10) Phenol	6.33	94	91798	5.51	ng	Qvalue # 73
49) Dimethylphthalate	9.42	163	294880	12.12	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF110816\
Data File : BF091108.D
Acq On : 9 Nov 2016 4:10
Operator : UM/SJ
Sample : H5593-04
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
NORTH-SIDEWALL

Quant Time: Nov 09 06:14:50 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 08 12:59:29 2016
Response via : Initial Calibration




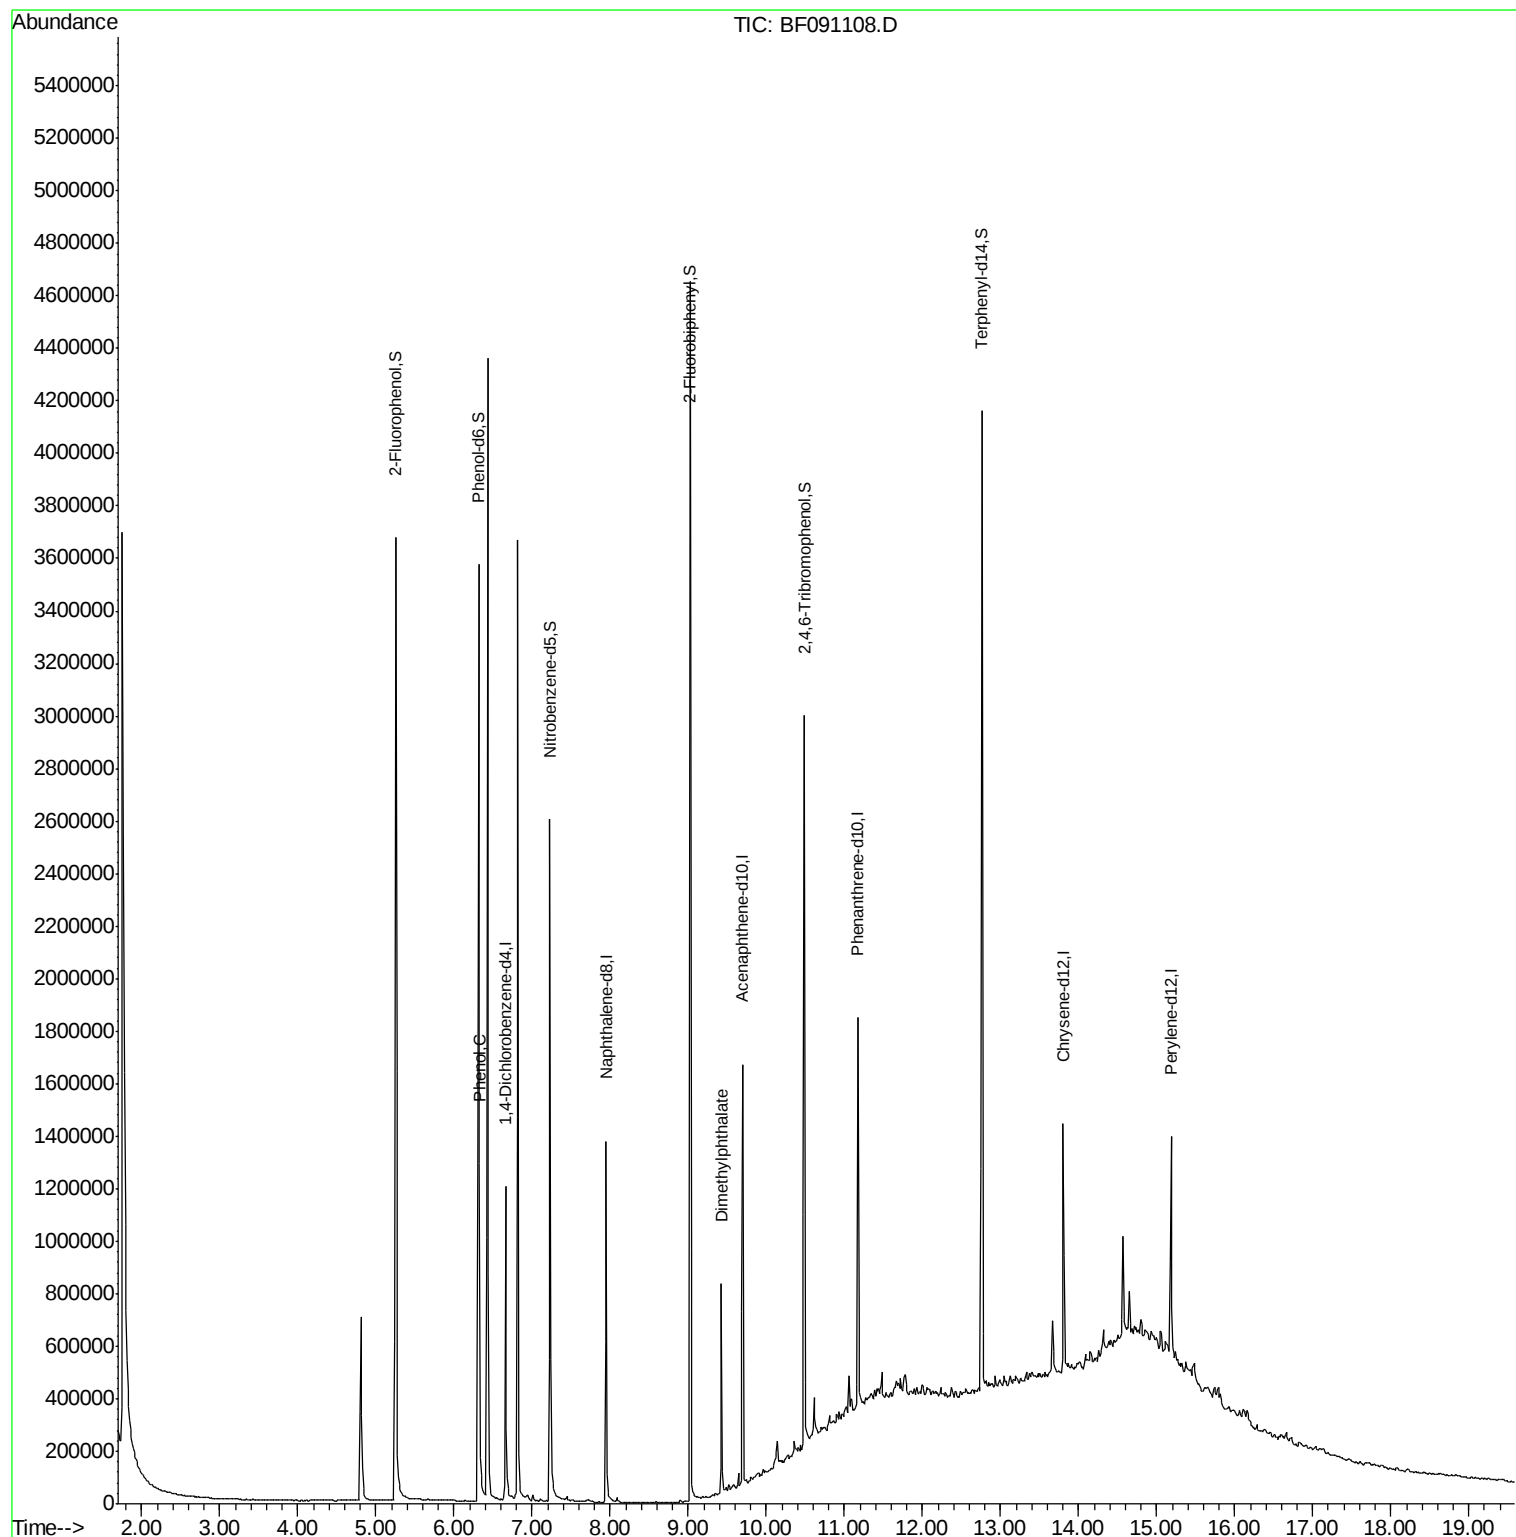


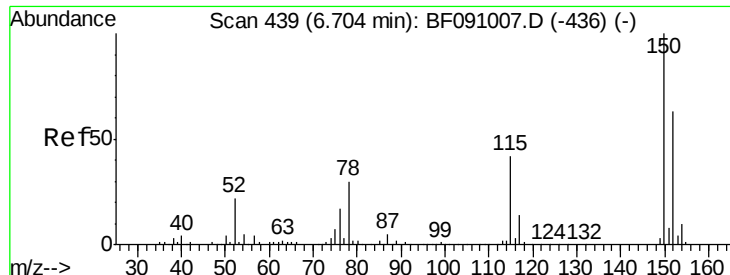

#1
 1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 6.66 min Scan# 435
 Delta R.T. 0.00 min
 Lab File: BF091108.D
 Acq: 9 Nov 2016 4:10




Instrument :
 BNA_F
 ClientSampleId :
 NORTH-SIDEWALL


Tot Ion:152 Resp: 183126
 Ion Ratio Lower Upper
 152 100
 150 158.4 126.8 190.2
 115 69.9 53.3 79.9

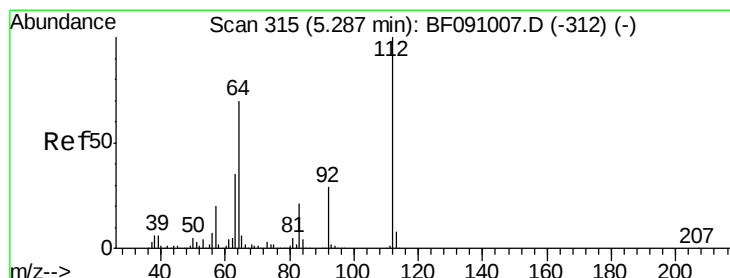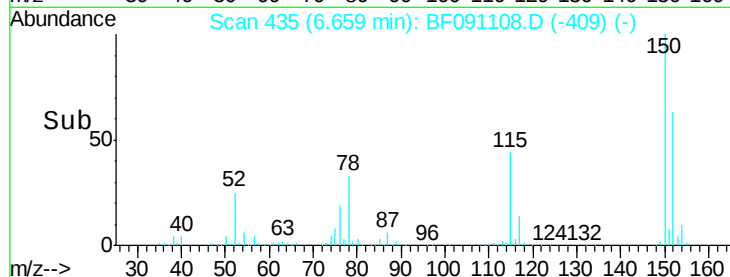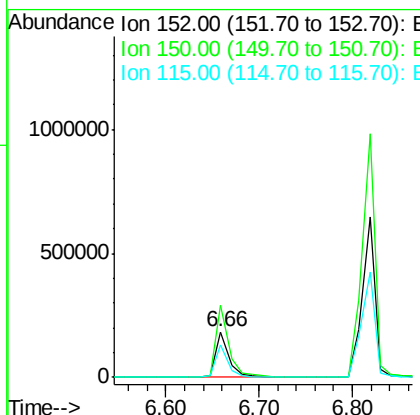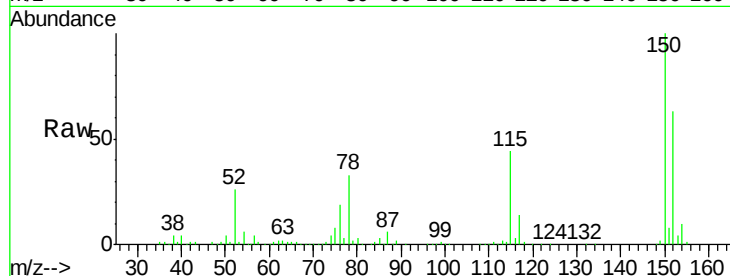

#5
 2-Fluorophenol
 Concen: 114.12 ng
 RT: 5.25 min Scan# 312
 Delta R.T. 0.01 min
 Lab File: BF091108.D
 Acq: 9 Nov 2016 4:10

Tgt Ion:112 Resp: 1265322
 Ion Ratio Lower Upper
 112 100
 64 66.9 55.8 83.6
 63 33.8 28.0 42.0

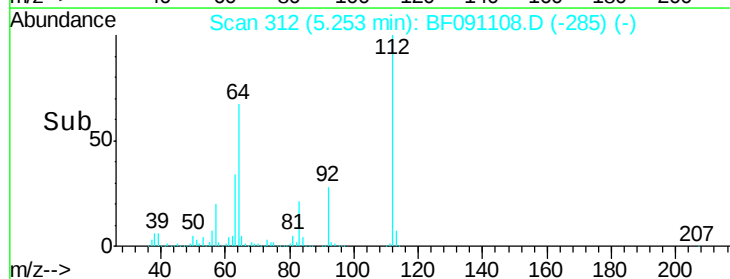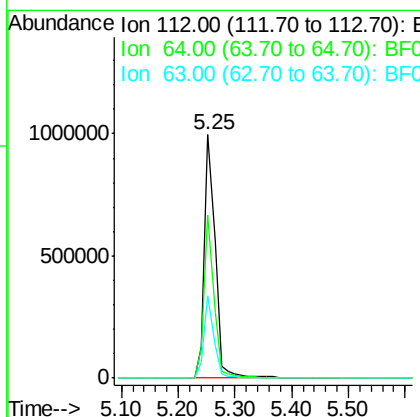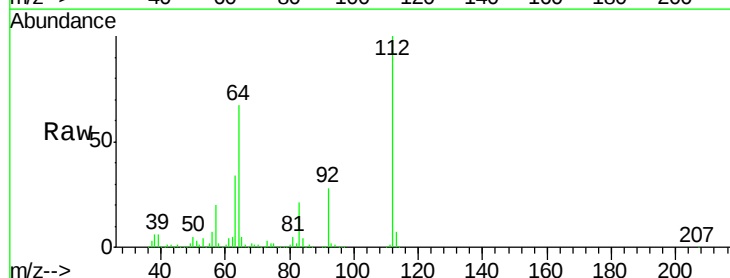

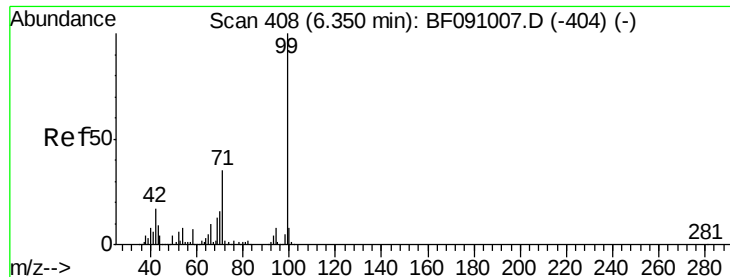

#7

Phenol-d6

Concen: 105.29 ng

RT: 6.32 min Scan# 405

Delta R.T. 0.00 min

Lab File: BF091108.D

Acq: 9 Nov 2016 4:10

Instrument :

BNA_F

ClientSampleId :

NORTH-SIDEWALL


Tot Ion: 99 Resp: 1584673

Ion Ratio Lower Upper

99 100

42 17.8 13.9 20.9




71 35.1 27.8 41.8

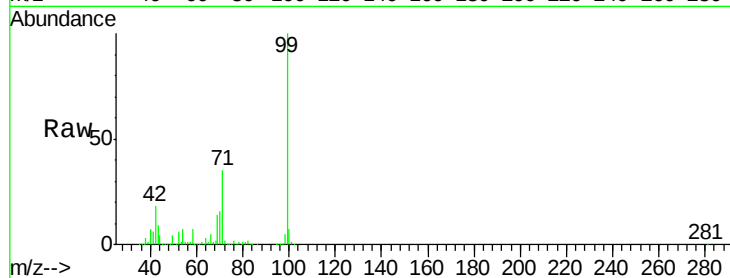

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

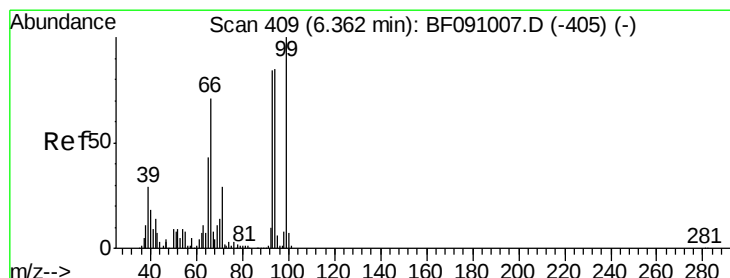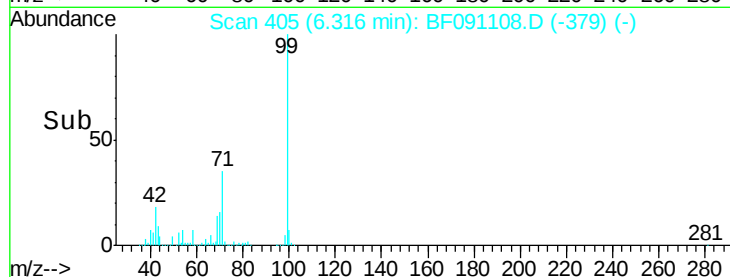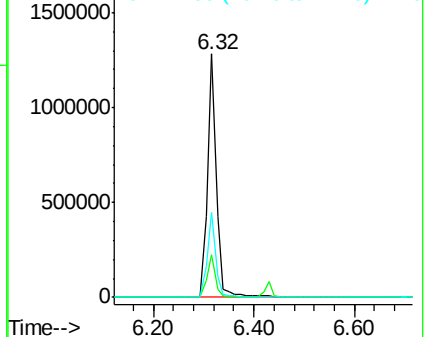

#10

Phenol

Concen: 5.51 ng

RT: 6.33 min Scan# 406

Delta R.T. 0.00 min

Lab File: BF091108.D

Acq: 9 Nov 2016 4:10


Tgt Ion: 94 Resp: 91798

Ion Ratio Lower Upper

94 100

65 34.6 30.4 70.4



66 56.0 62.9 102.9#

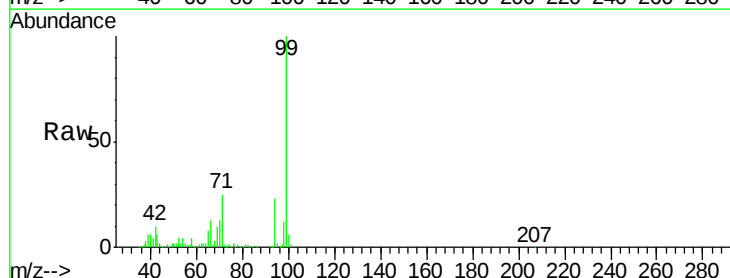


Abundance Ion 94.00 (93.70 to 94.70): BF0

Ion 65.00 (64.70 to 65.70): BF0

Ion 66.00 (65.70 to 66.70): BF0

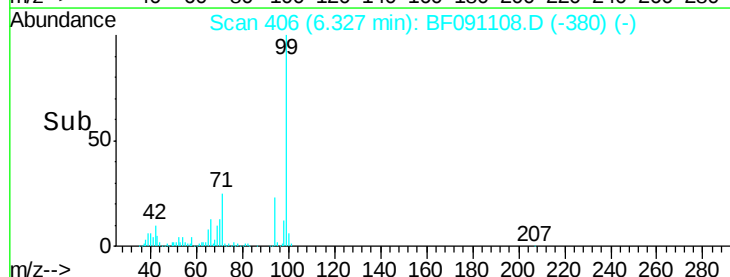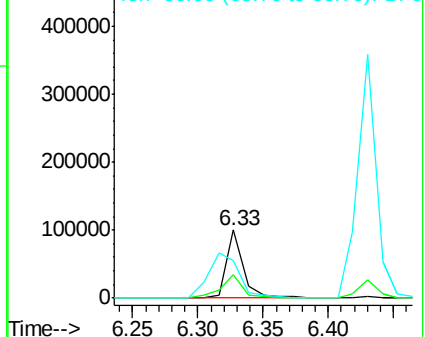


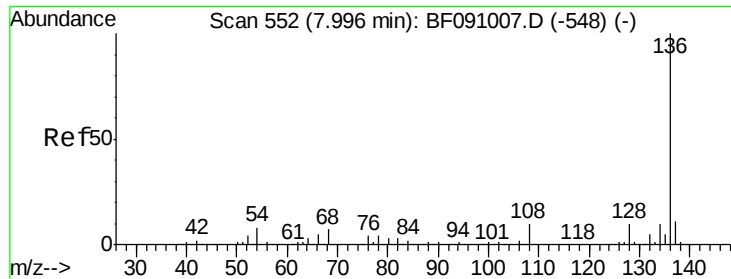




#21
Naphthalene-d8
Concen: 20.00 ng
RT: 7.95 min Scan# 548
Delta R.T. 0.00 min
Lab File: BF091108.D
Acq: 9 Nov 2016 4:10

Instrument :
BNA_F
ClientSampleId :
NORTH-SIDEWALL

Tot Ion:136	Resp:	746762
Ion Ratio	Lower	Upper
136	100	
137	10.7	8.9 13.3
54	6.8	6.2 9.2
68	6.0	5.5 8.3




Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF0
Ion 68.00 (67.70 to 68.70): BF0

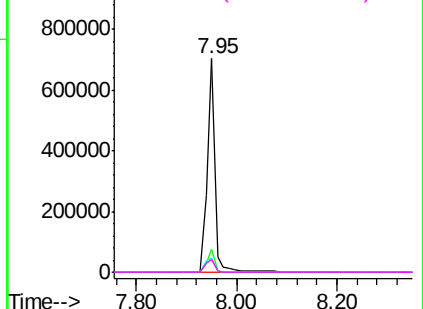




#23
Nitrobenzene-d5
Concen: 73.97 ng
RT: 7.23 min Scan# 485
Delta R.T. -0.01 min
Lab File: BF091108.D
Acq: 9 Nov 2016 4:10

Tgt Ion: 82	Resp:	1012586
Ion Ratio	Lower	Upper
82	100	
128	40.1	32.4 48.6
54	49.2	39.2 58.8



Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF0

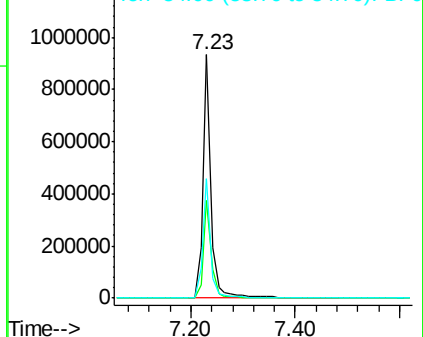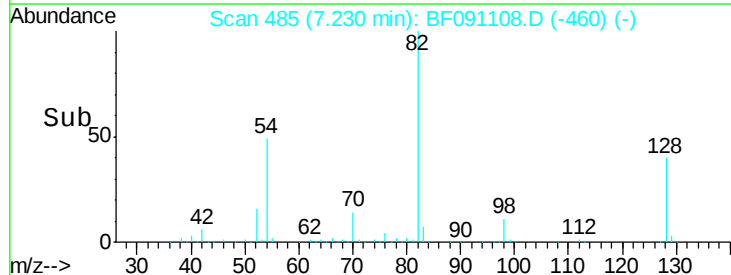







#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.70 min Scan# 701
 Delta R.T. 0.00 min
 Lab File: BF091108.D
 Acq: 9 Nov 2016 4:10

Instrument :
 BNA_F
 ClientSampleId :
 NORTH-SIDEWALL

Tot Ion:164 Resp: 370978
 Ion Ratio Lower Upper
 164 100
 162 102.9 83.6 125.4
 160 47.1 37.9 56.9




Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E


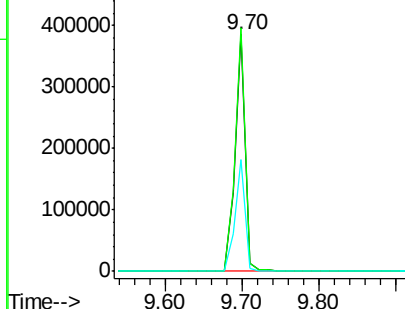



#41
 2,4,6-Tribromophenol
 Concen: 100.65 ng
 RT: 10.49 min Scan# 770
 Delta R.T. 0.00 min
 Lab File: BF091108.D
 Acq: 9 Nov 2016 4:10

Tgt Ion:330 Resp: 337552
 Ion Ratio Lower Upper
 330 100
 332 94.7 75.9 113.9
 141 40.6 36.1 54.1



Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

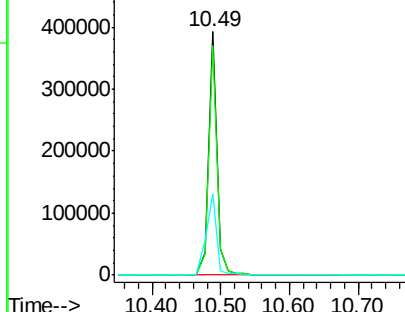







#44
2-Fluorobiphenyl
Concen: 65.92 ng
RT: 9.02 min Scan# 642
Delta R.T. -0.01 min
Lab File: BF091108.D
Acq: 9 Nov 2016 4:10

Instrument :
BNA_F
ClientSampleId :
NORTH-SIDEWALL

Tot Ion:172 Resp: 1420540
Ion Ratio Lower Upper
172 100
171 36.7 29.8 44.6
170 25.7 20.3 30.5




Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E


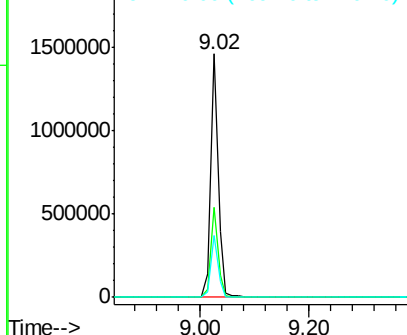



#49
Dimethylphthalate
Concen: 12.12 ng
RT: 9.42 min Scan# 677
Delta R.T. -0.01 min
Lab File: BF091108.D
Acq: 9 Nov 2016 4:10

Tgt Ion:163 Resp: 294880
Ion Ratio Lower Upper
163 100
194 3.0 2.6 4.0
164 10.3 8.7 13.1



Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

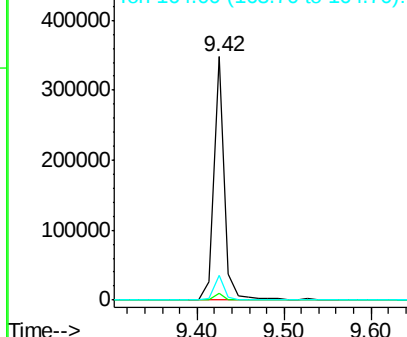







#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.17 min Scan# 830
Delta R.T. 0.00 min
Lab File: BF091108.D
Acq: 9 Nov 2016 4:10

Instrument :
BNA_F
ClientSampleId :
NORTH-SIDEWALL

Tot Ion:188 Resp: 524768
Ion Ratio Lower Upper
188 100
94 13.4 7.0 10.4#
80 14.9 7.5 11.3#

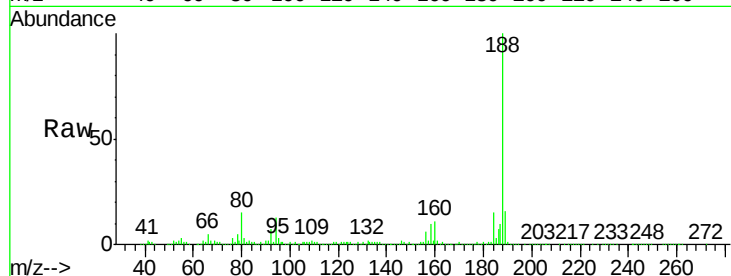


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0


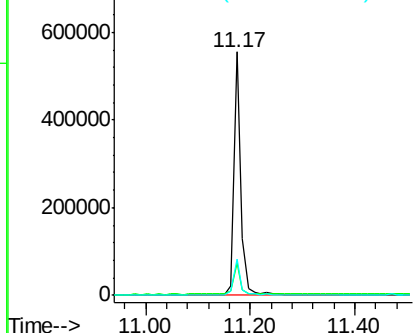



#75
Chrysene-d12
Concen: 20.00 ng
RT: 13.80 min Scan# 1060
Delta R.T. -0.01 min
Lab File: BF091108.D
Acq: 9 Nov 2016 4:10

Tgt Ion:240 Resp: 361094
Ion Ratio Lower Upper
240 100
120 18.2 12.9 19.3
236 27.3 21.9 32.9



Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

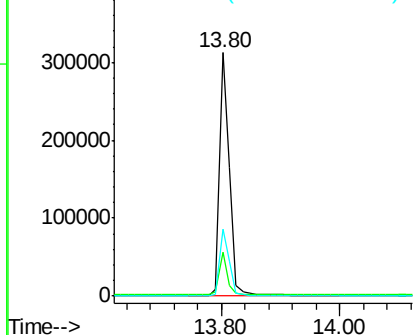



#78

Terphenyl-d14

Concen: 75.48 ng

RT: 12.76 min Scan# 969

Delta R.T. 0.00 min

Lab File: BF091108.D

Acq: 9 Nov 2016 4:10

Instrument :

BNA_F

ClientSampleId :

NORTH-SIDEWALL


Tot Ion:244 Resp: 1092224

Ion Ratio Lower Upper

244 100

212 7.6 6.4 9.6




122 12.1 12.3 18.5#



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

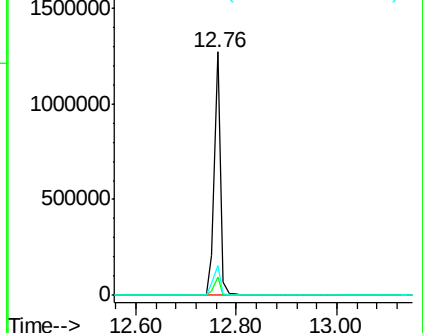

#86

Perylene-d12

Concen: 20.00 ng

RT: 15.19 min Scan# 1181

Delta R.T. 0.00 min

Lab File: BF091108.D

Acq: 9 Nov 2016 4:10


Tgt Ion:264 Resp: 346438

Ion Ratio Lower Upper

264 100

260 26.0 20.6 30.8

265 21.6 17.8 26.8



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

