

Data Path : Z:\HPCHEM1\BNA F\DATA\BF110816\
 Data File : BF091120.D
 Acq On : 9 Nov 2016 9:40
 Operator : UM/SJ
 Sample : H5547-07
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 WATER-QUALITYDRY-7

Quant Time: Nov 09 10:34:14 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110316.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 08 12:59:29 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.66	152	173654	20.00	ng	0.00
21) Naphthalene-d8	7.95	136	685333	20.00	ng	0.00
38) Acenaphthene-d10	9.70	164	322514	20.00	ng	0.00
63) Phenanthrene-d10	11.17	188	478183	20.00	ng	0.00
75) Chrysene-d12	13.80	240	331774	20.00	ng	-0.01
86) Perylene-d12	15.17	264	278987	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.25	112	502771	47.82	ng	0.01
7) Phenol-d6	6.30	99	390016	27.33	ng	-0.01
23) Nitrobenzene-d5	7.23	82	970216	77.23	ng	-0.01
41) 2,4,6-Tribromophenol	10.49	330	354537	121.59	ng	0.00
44) 2-Fluorobiphenyl	9.02	172	1607196	85.79	ng	-0.01
78) Terphenyl-d14	12.76	244	1329674	100.01	ng	0.00
Target Compounds						
49) Dimethylphthalate	9.42	163	82416	3.90	ng	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF110816\
Data File : BF091120.D
Acq On : 9 Nov 2016 9:40
Operator : UM/SJ
Sample : H5547-07
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WATER-QUALITYDRY-7

Quant Time: Nov 09 10:34:14 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 08 12:59:29 2016
Response via : Initial Calibration

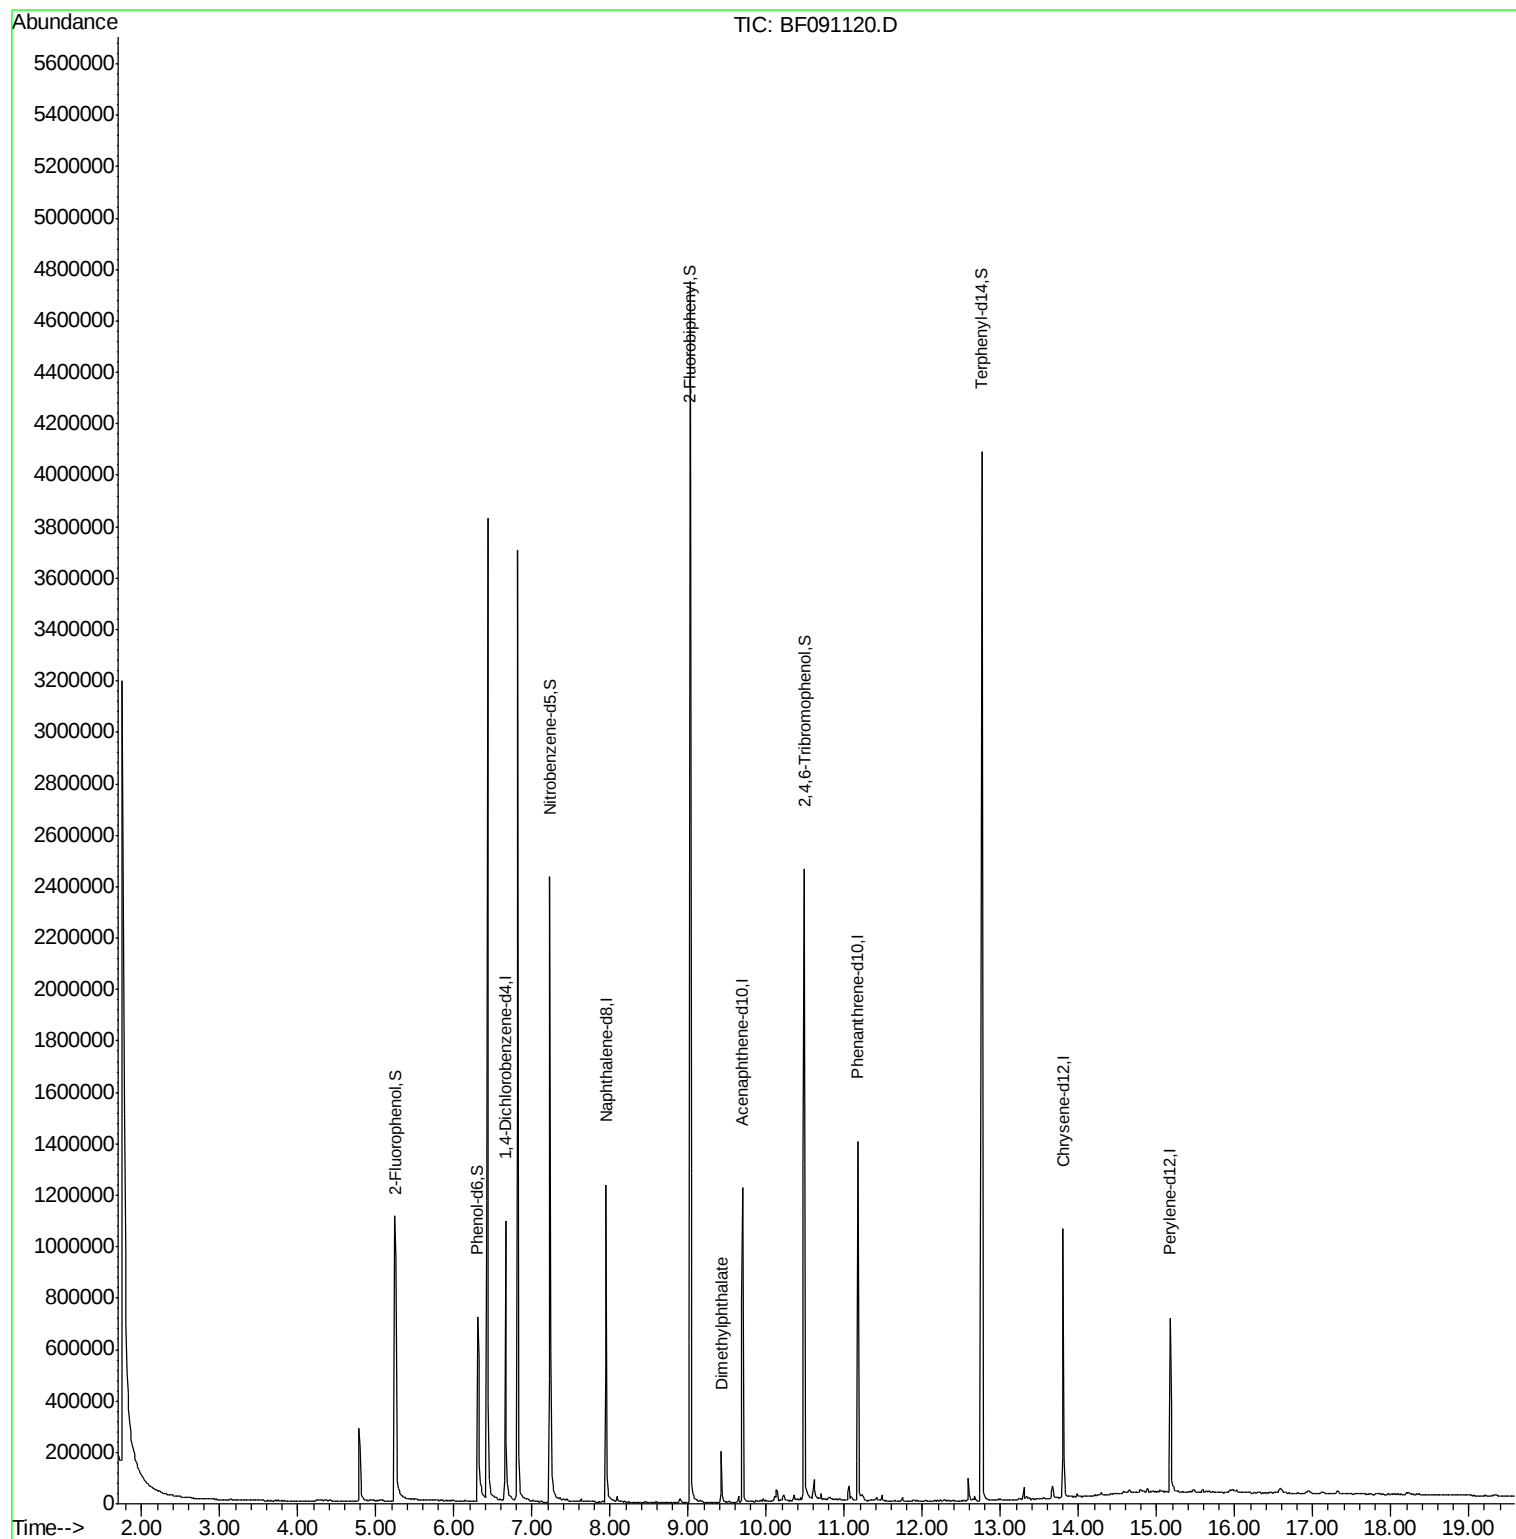

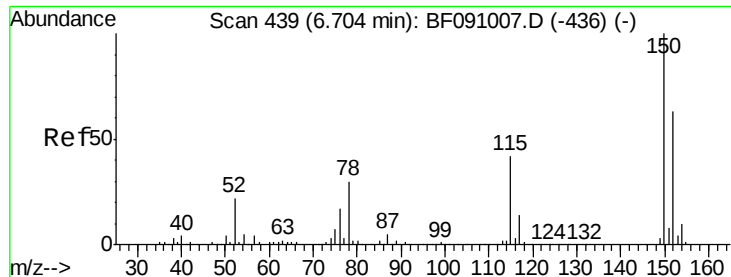

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.66 min Scan# 435

Delta R.T. 0.00 min

Lab File: BF091120.D

Acq: 9 Nov 2016 9:40

Instrument :

BNA_F

ClientSampleId :

WATER-QUALITYDRY-7


Tot Ion:152 Resp: 173654

Ion Ratio Lower Upper

152 100

150 156.3 126.8 190.2




115 66.1 53.3 79.9

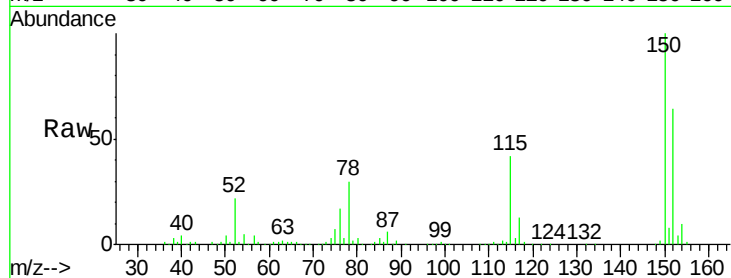

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

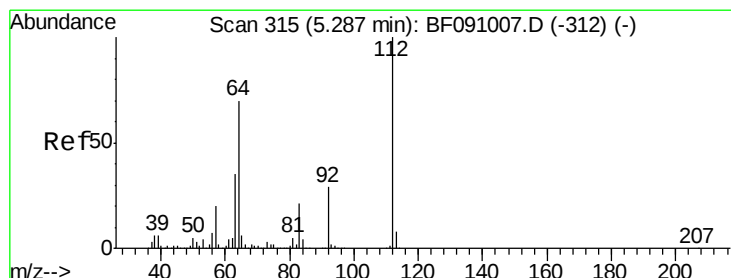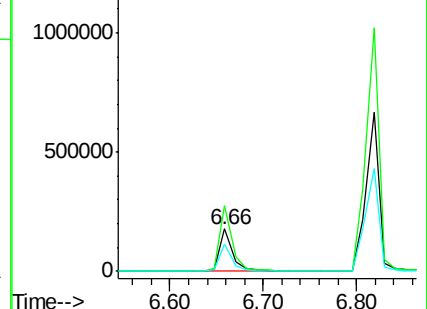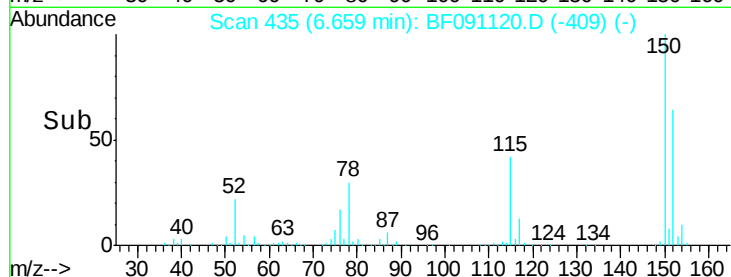

#5

2-Fluorophenol

Concen: 47.82 ng

RT: 5.25 min Scan# 312

Delta R.T. 0.01 min

Lab File: BF091120.D

Acq: 9 Nov 2016 9:40


Tgt Ion:112 Resp: 502771

Ion Ratio Lower Upper

112 100

64 54.5 55.8 83.6#



63 27.2 28.0 42.0#

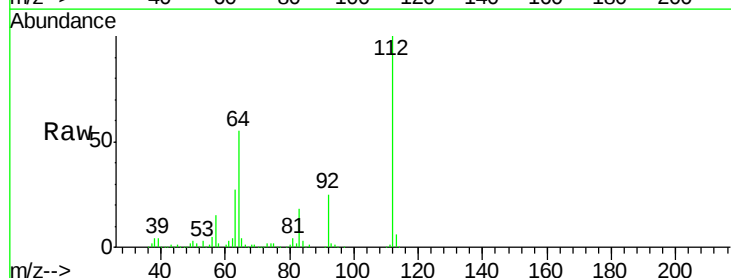


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

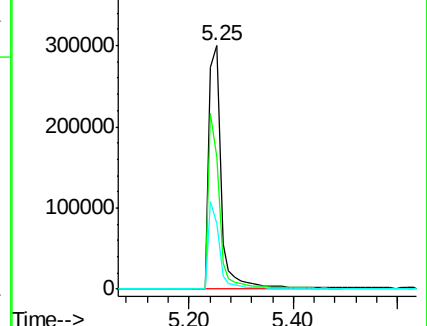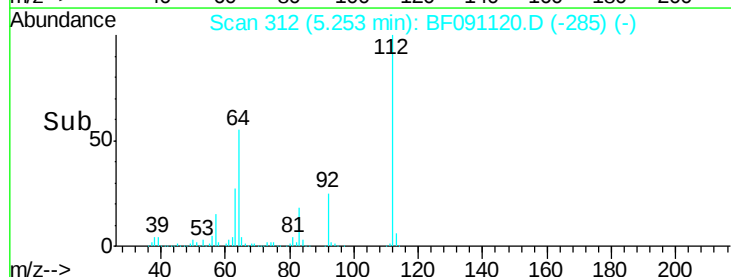

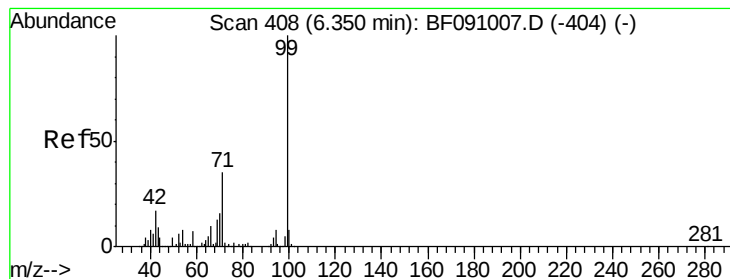

#7

Phenol-d6

Concen: 27.33 ng

RT: 6.30 min Scan# 404

Delta R.T. -0.01 min

Lab File: BF091120.D

Acq: 9 Nov 2016 9:40

Instrument :

BNA_F

ClientSampleId :

WATER-QUALITYDRY-7





Tot Ion: 99 Resp: 390016

Ion Ratio Lower Upper

99 100

42 21.2 13.9 20.9#

71 37.7 27.8 41.8

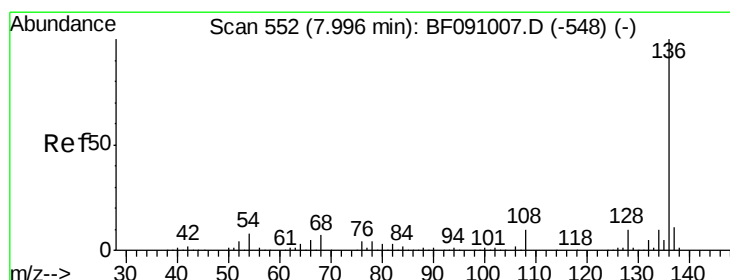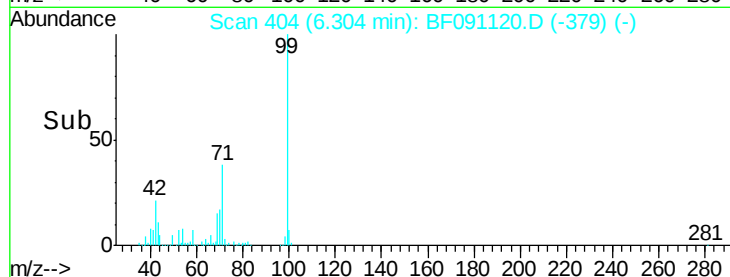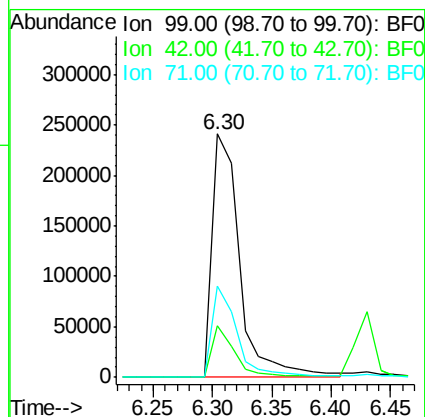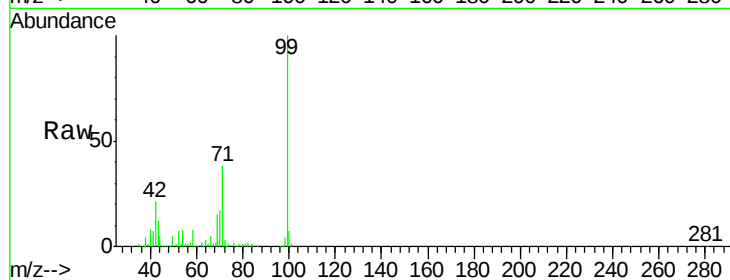

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.95 min Scan# 548

Delta R.T. 0.00 min

Lab File: BF091120.D

Acq: 9 Nov 2016 9:40

Tgt Ion: 136 Resp: 685333




Ion Ratio Lower Upper


136 100

137 10.9 8.9 13.3

54 6.3 6.2 9.2

68 5.9 5.5 8.3

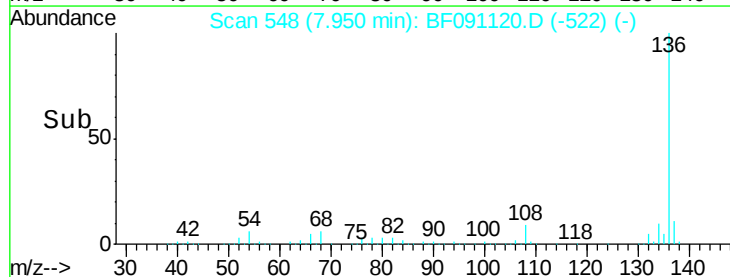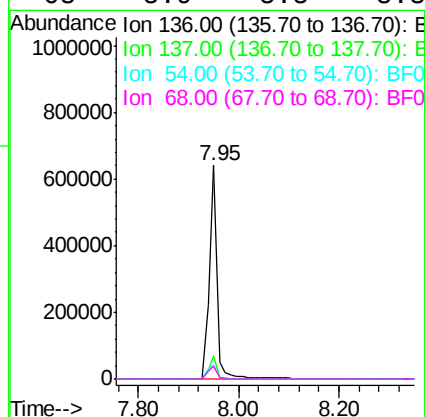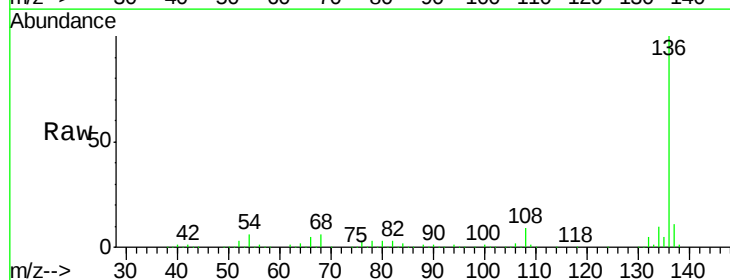


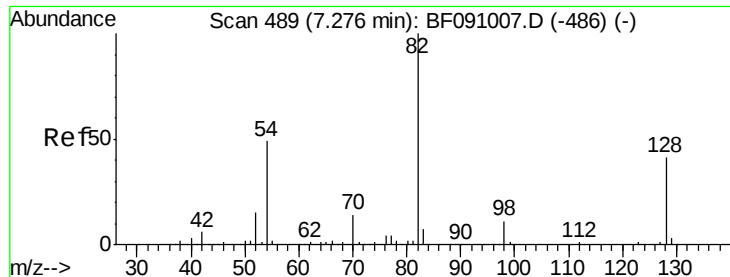




#23
Nitrobenzene-d5
Concen: 77.23 ng
RT: 7.23 min Scan# 485
Delta R.T. -0.01 min
Lab File: BF091120.D
Acq: 9 Nov 2016 9:40

Instrument :
BNA_F
ClientSampleId :
WATER-QUALITYDRY-7

Tot Ion: 82 Resp: 970216
Ion Ratio Lower Upper
82 100
128 42.9 32.4 48.6
54 47.4 39.2 58.8

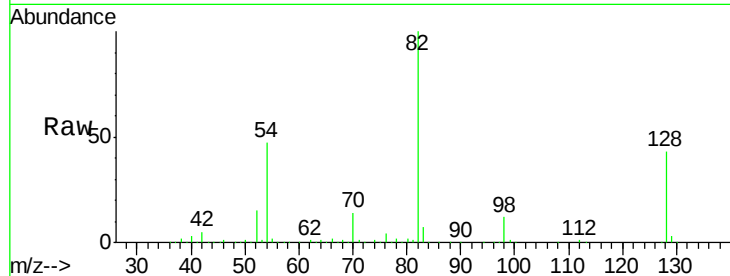


Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): B
Ion 54.00 (53.70 to 54.70): BF0

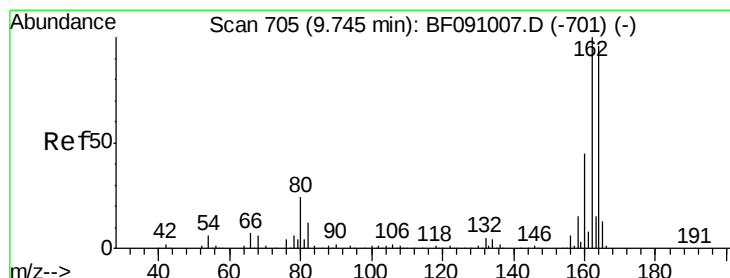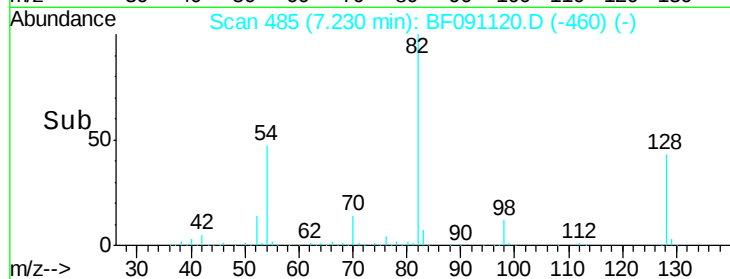
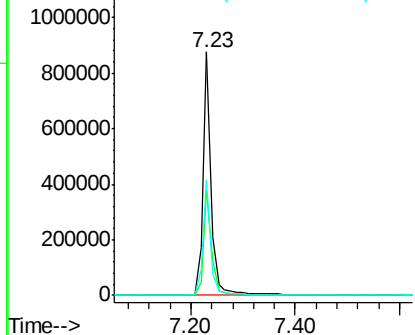



#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.70 min Scan# 701
Delta R.T. 0.00 min
Lab File: BF091120.D
Acq: 9 Nov 2016 9:40

Tgt Ion:164 Resp: 322514
Ion Ratio Lower Upper
164 100
162 103.9 83.6 125.4
160 47.8 37.9 56.9

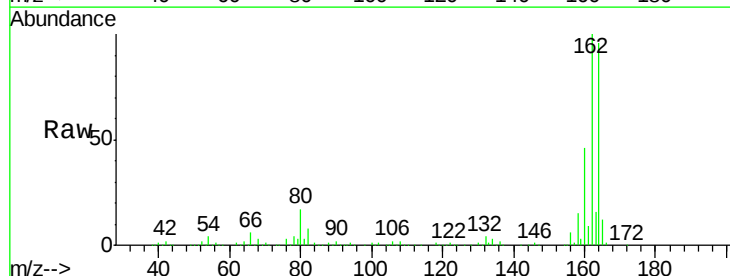

Abundance Ion 164.00 (163.70 to 164.70): B
Ion 162.00 (161.70 to 162.70): B
Ion 160.00 (159.70 to 160.70): B

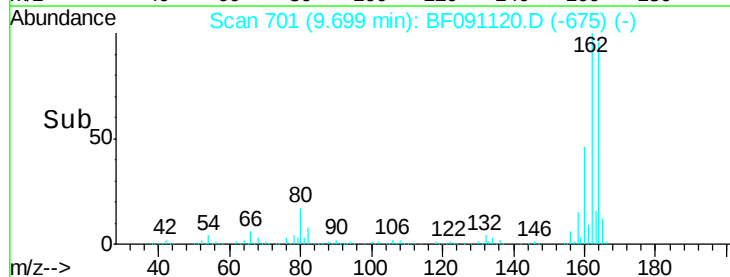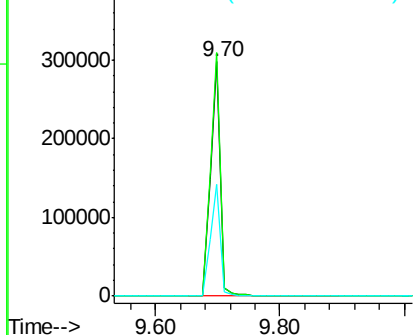


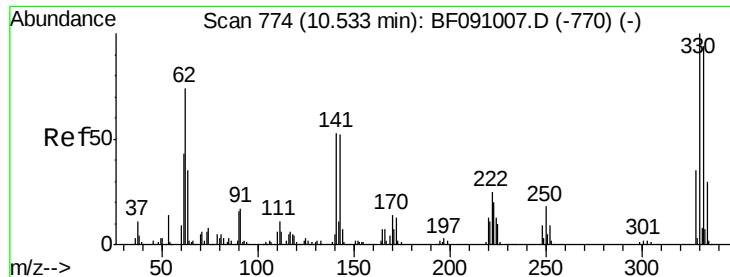




#41
 2,4,6-Tribromophenol
 Concen: 121.59 ng
 RT: 10.49 min Scan# 770
 Delta R.T. 0.00 min
 Lab File: BF091120.D
 Acq: 9 Nov 2016 9:40

Instrument :
 BNA_F
 ClientSampleId :
 WATER-QUALITYDRY-7

Tot Ion:330 Resp: 354537
 Ion Ratio Lower Upper
 330 100
 332 95.6 75.9 113.9
 141 36.7 36.1 54.1

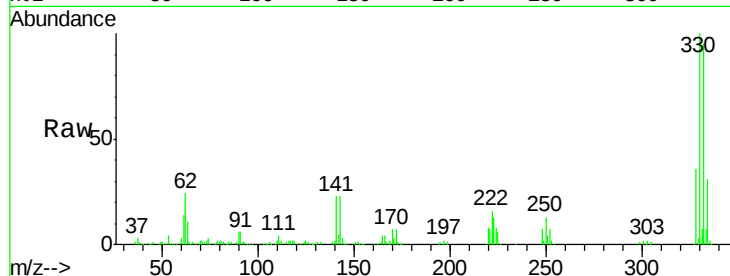


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

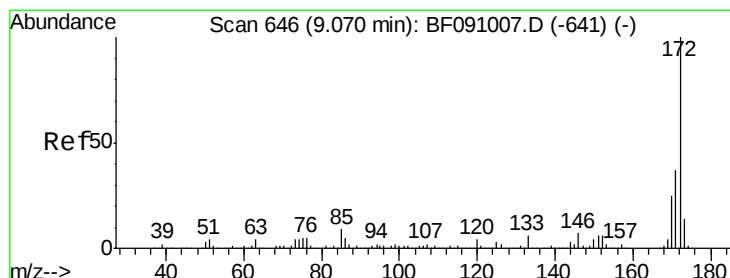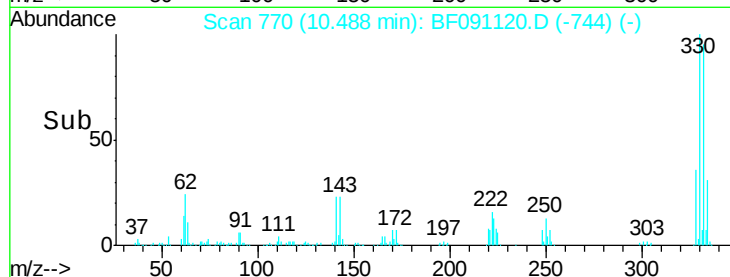
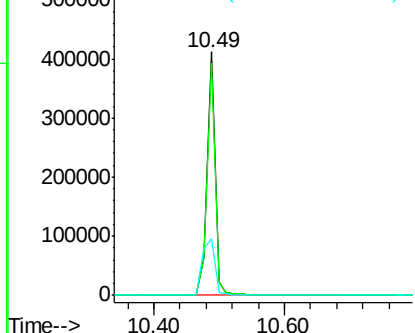



#44
 2-Fluorobiphenyl
 Concen: 85.79 ng
 RT: 9.02 min Scan# 642
 Delta R.T. -0.01 min
 Lab File: BF091120.D
 Acq: 9 Nov 2016 9:40

Tgt Ion:172 Resp: 1607196
 Ion Ratio Lower Upper
 172 100
 171 37.2 29.8 44.6
 170 25.1 20.3 30.5

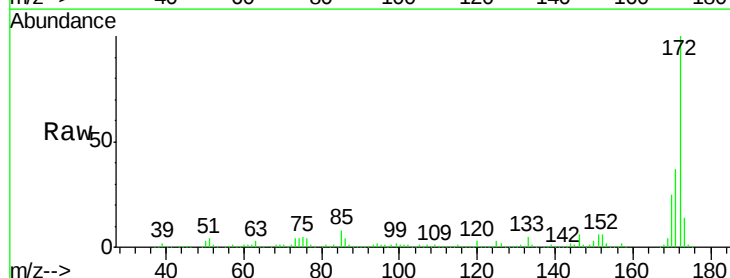

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

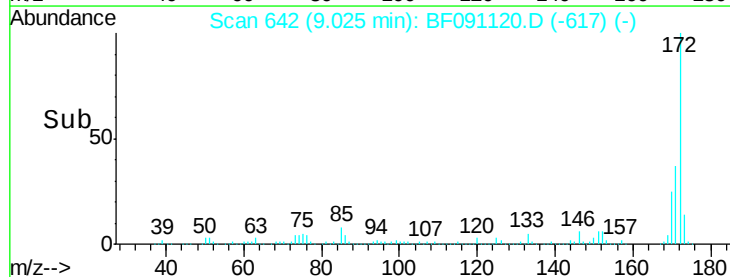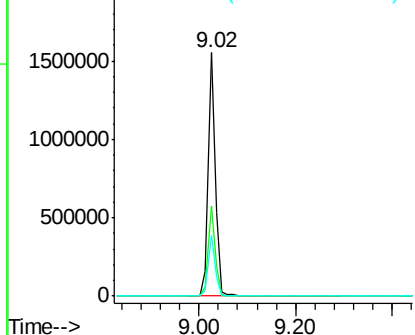


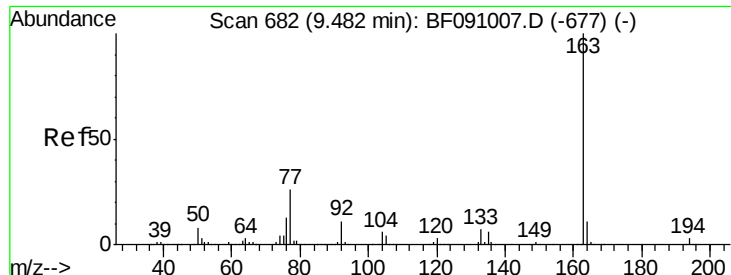




#49
Dimethylphthalate
Concen: 3.90 ng
RT: 9.42 min Scan# 677
Delta R.T. -0.01 min
Lab File: BF091120.D
Acq: 9 Nov 2016 9:40

Instrument :
BNA_F
ClientSampleId :
WATER-QUALITYDRY-7

Tot Ion:163 Resp: 82416
Ion Ratio Lower Upper
163 100
194 3.2 2.6 4.0
164 10.0 8.7 13.1

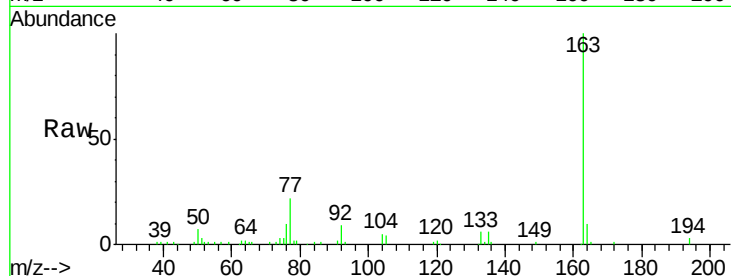


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

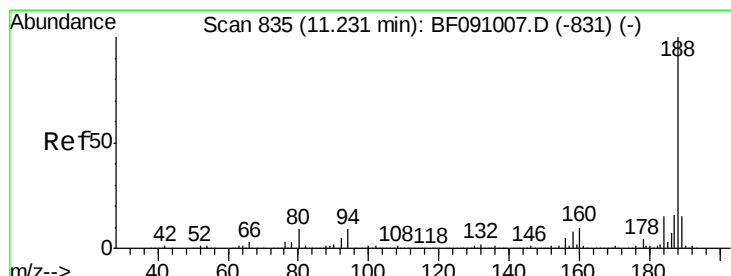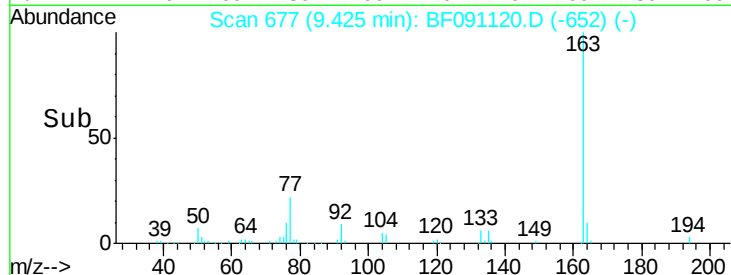
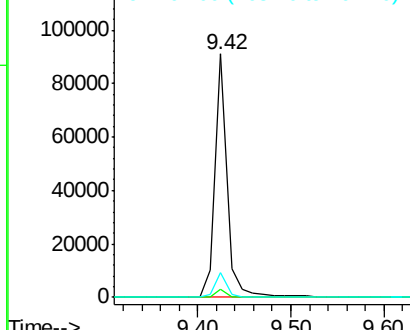



#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.17 min Scan# 830
Delta R.T. 0.00 min
Lab File: BF091120.D
Acq: 9 Nov 2016 9:40

Tgt Ion:188 Resp: 478183
Ion Ratio Lower Upper
188 100
94 11.8 7.0 10.4#
80 13.0 7.5 11.3#

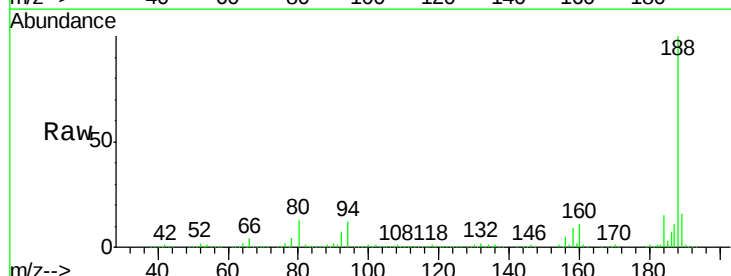

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

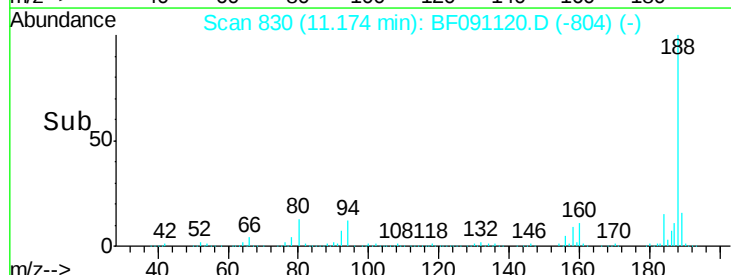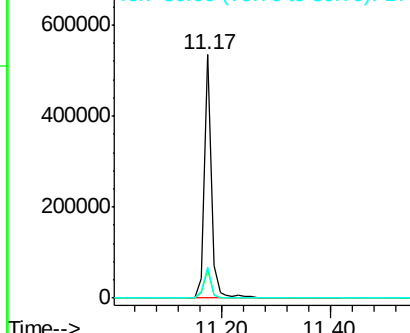

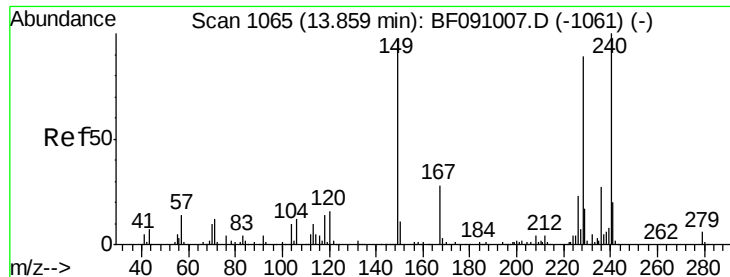

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.80 min Scan# 1060

Delta R.T. -0.01 min

Lab File: BF091120.D

Acq: 9 Nov 2016 9:40

Instrument :

BNA_F

ClientSampleId :

WATER-QUALITYDRY-7


Tot Ion:240 Resp: 331774

Ion Ratio Lower Upper




240 100

120 14.2 12.9 19.3

236 27.9 21.9 32.9

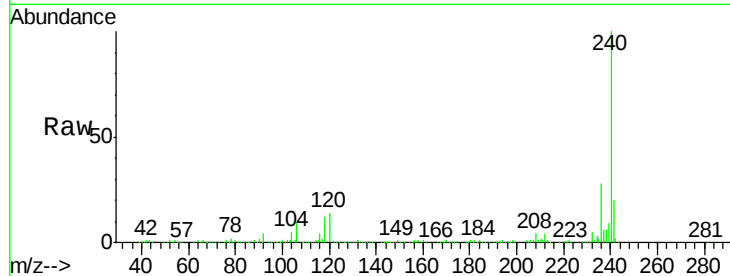

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

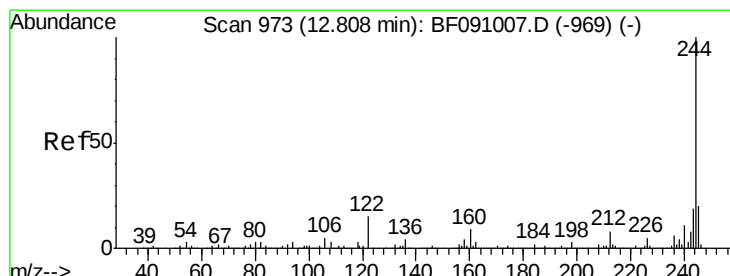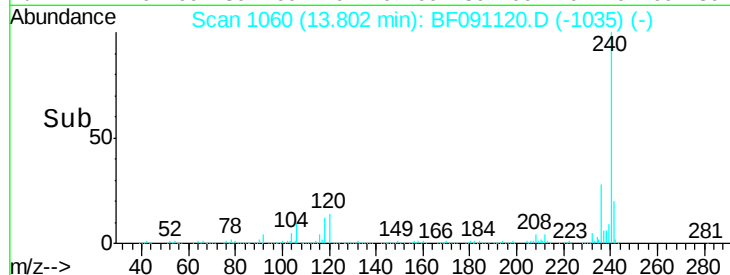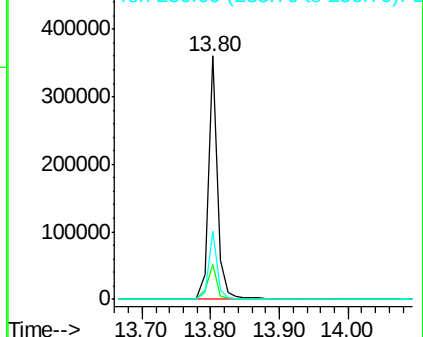

#78

Terphenyl-d14

Concen: 100.01 ng

RT: 12.76 min Scan# 969

Delta R.T. 0.00 min

Lab File: BF091120.D

Acq: 9 Nov 2016 9:40


Tgt Ion:244 Resp: 1329674

Ion Ratio Lower Upper



244 100


212 7.5 6.4 9.6

122 10.8 12.3 18.5#

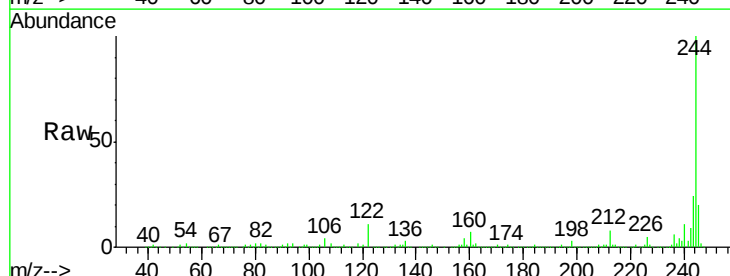

Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

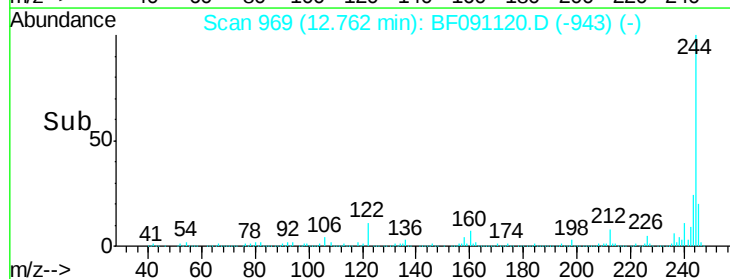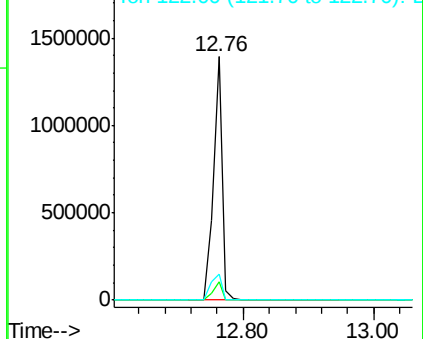

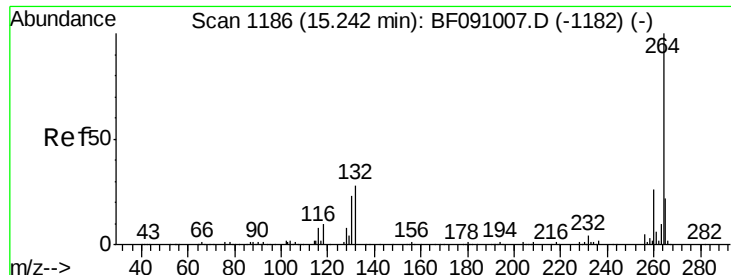

#86
Pervlene-d12
Concen: 20.00 ng
RT: 15.17 min Scan# 1180
Delta R.T. -0.01 min
Lab File: BF091120.D
Acq: 9 Nov 2016 9:40

Instrument :
BNA_F
ClientSampleId :
WATER-QUALITYDRY-7

Tot Ion:	264	Resp:	278987
Ion	Ratio	Lower	Upper
264	100		
260	25.7	20.6	30.8
265	22.3	17.8	26.8

