
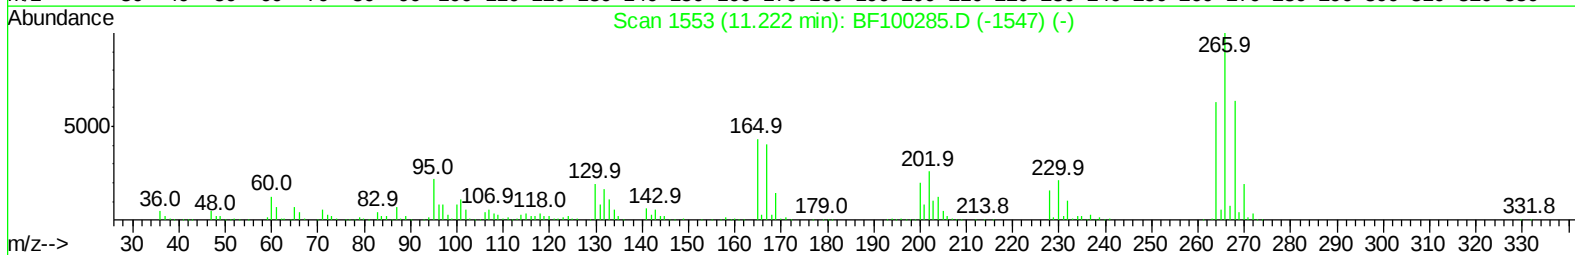
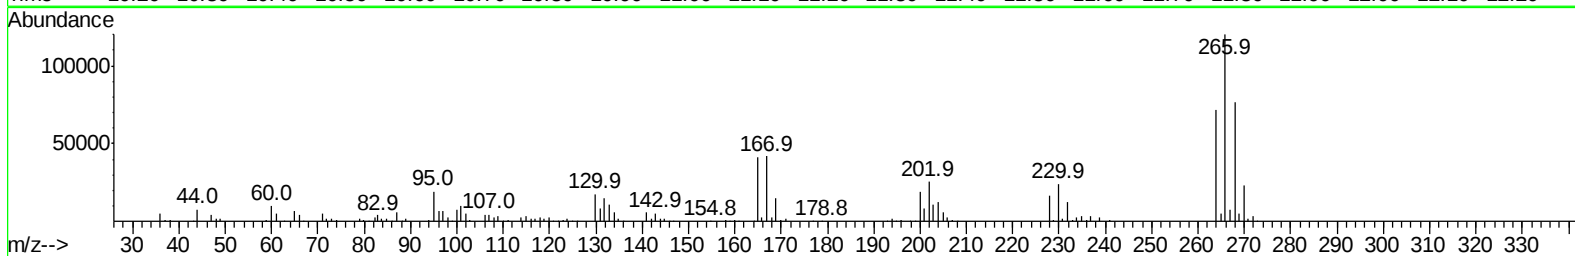


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA F\Data\BF110817\
Data File : BF100281.D
Acq On : 8 Nov 2017 10:06
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 10 08:41:56 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 09 16:04:38 2017
Response via : Initial Calibration

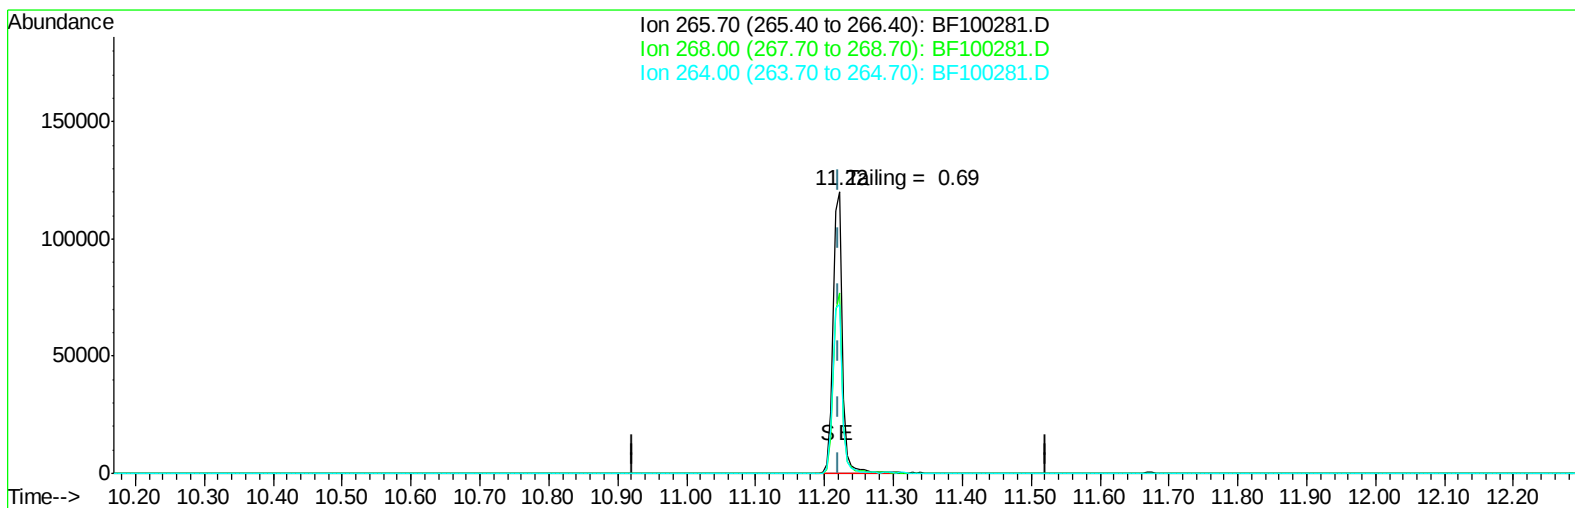

TIC: BF100281.D

(69) Pentachlorophenol (C)




11.222min (+0.000) 32289.05ng

response 111362

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.95
264.00	61.90	60.01
0.00	0.00	0.00

Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA F\Data\BF110817\
Data File : BF100281.D
Acq On : 8 Nov 2017 10:06
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 10 08:41:56 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 09 16:04:38 2017
Response via : Initial Calibration

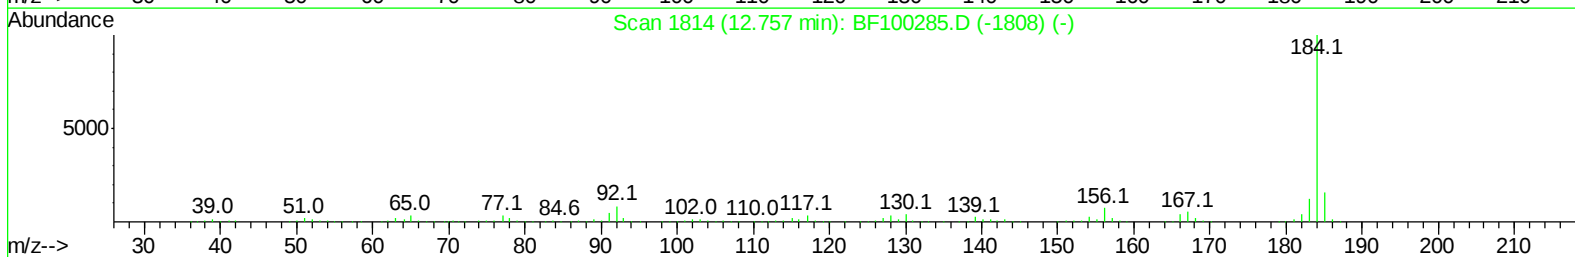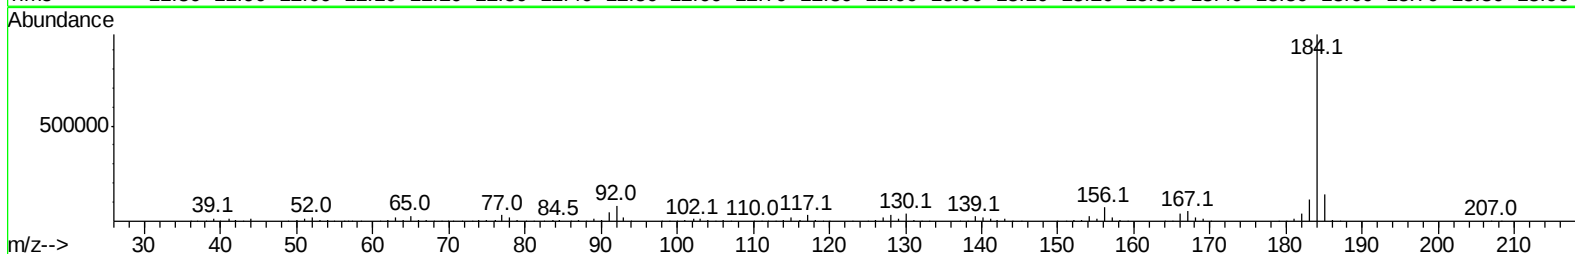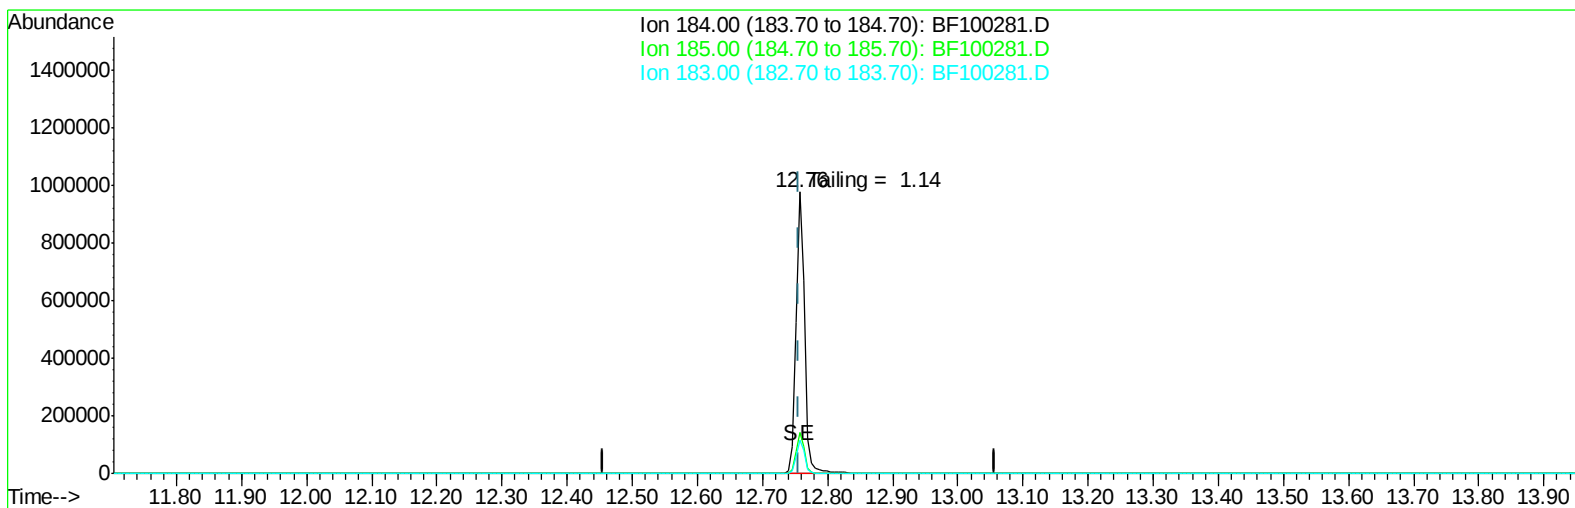

TIC: BF100281.D

(76) Benzidine

12.757min (+0.000) 0.00ng

response 891475

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.47
183.00	11.60	11.82
0.00	0.00	0.00