
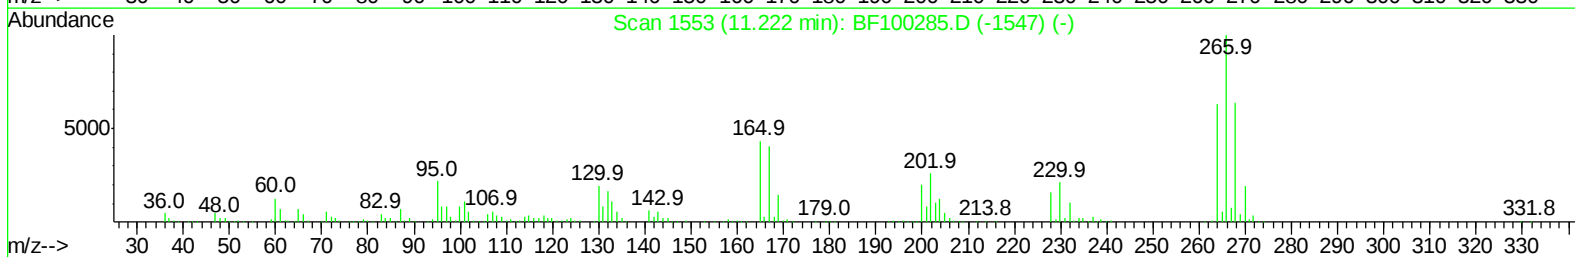
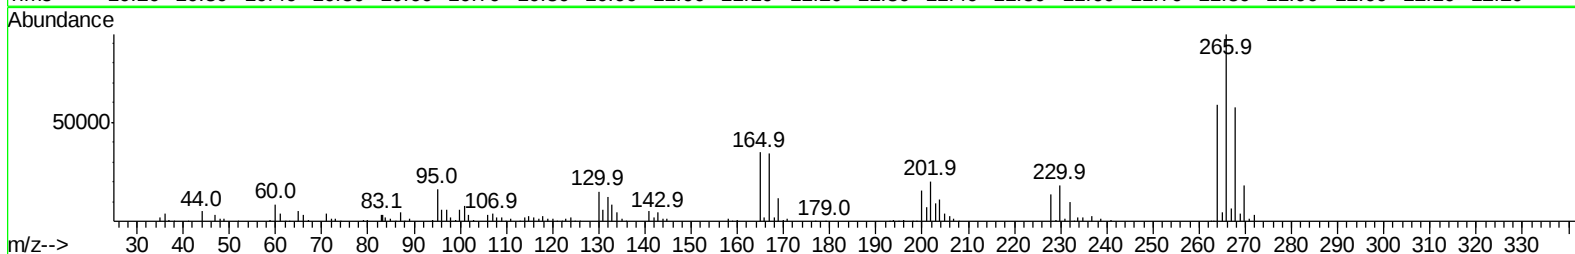


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA F\Data\BF110817\
Data File : BF100316.D
Acq On : 9 Nov 2017 2:47
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 10 08:46:08 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 09 16:04:38 2017
Response via : Initial Calibration

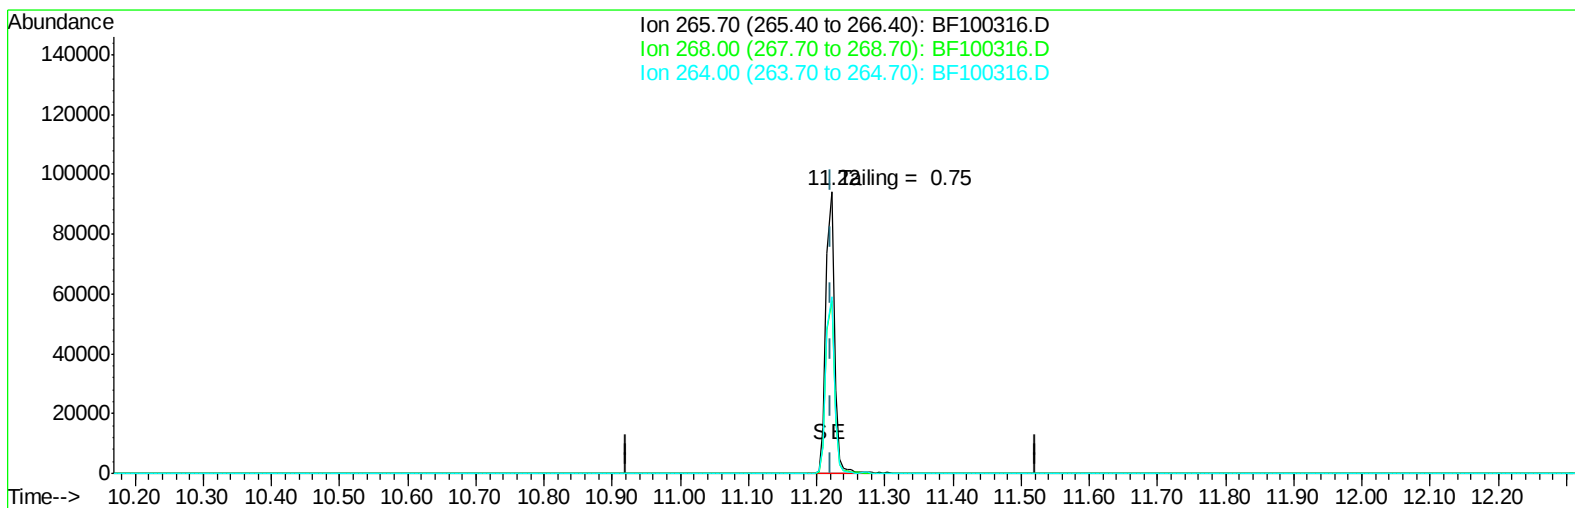

TIC: BF100316.D

(69) Pentachlorophenol (C)




11.221min (0.000) 16635.68ng

response 79041

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	61.42
264.00	61.90	62.76
0.00	0.00	0.00

Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA F\Data\BF110817\
Data File : BF100316.D
Acq On : 9 Nov 2017 2:47
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 10 08:46:08 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 09 16:04:38 2017
Response via : Initial Calibration

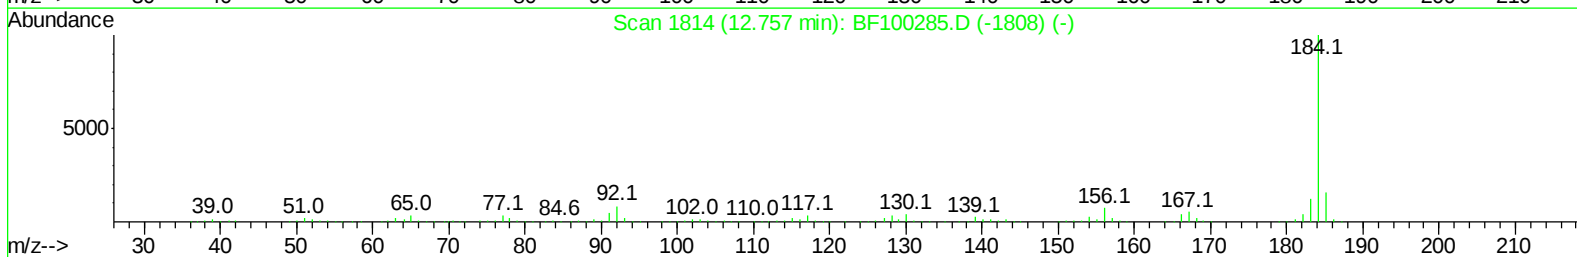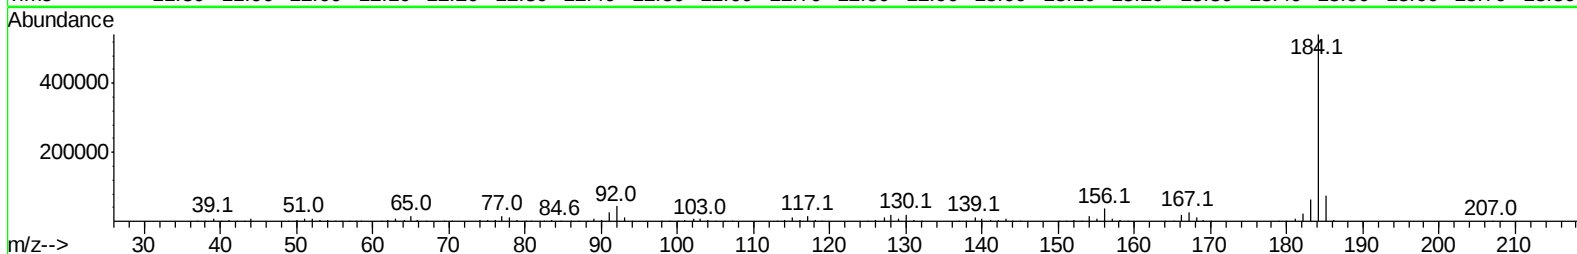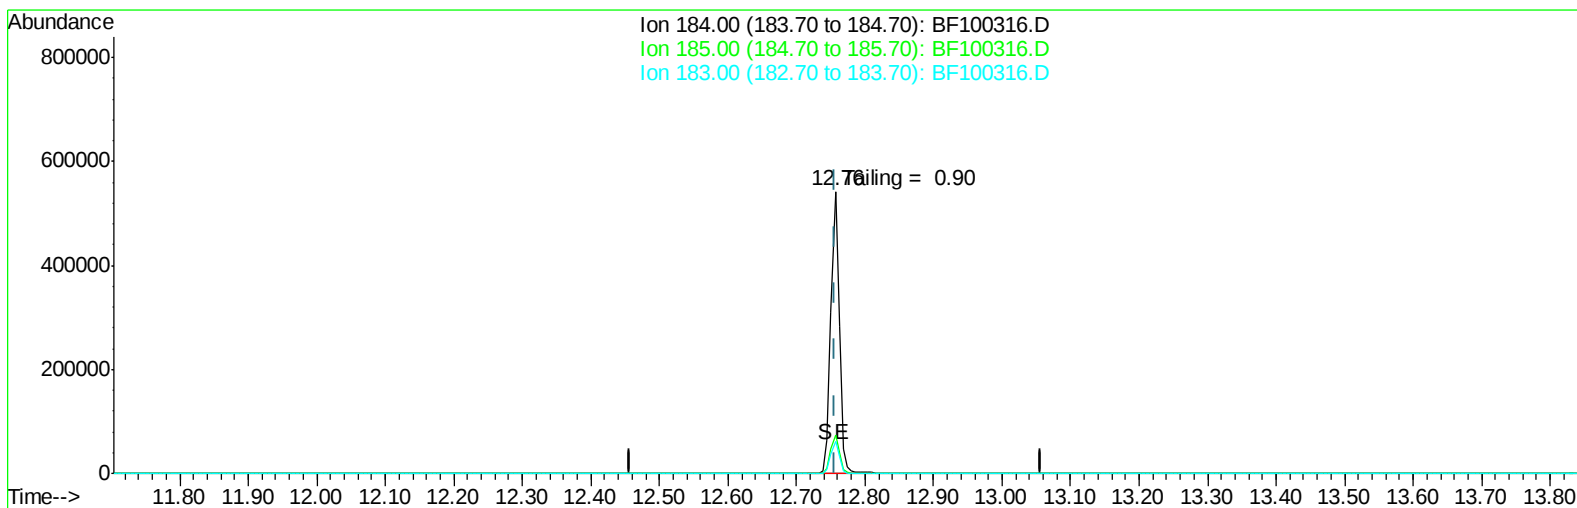

TIC: BF100316.D

(76) Benzidine

12.757min (0.000) 55651.88ng

response 454662

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	13.83
183.00	11.60	11.44
0.00	0.00	0.00