

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF110817\
 Data File : BF100309.D
 Acq On : 8 Nov 2017 23:13
 Operator : SJ/JU
 Sample : I6354-04 10X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 POOL-5001-0001-02

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.110	511	514	521	rBV	86741	83092	6.01%	0.807%
2	5.504	577	581	584	rBV	577361	488021	35.28%	4.738%
3	6.504	748	751	756	rBV	535790	495692	35.84%	4.812%
4	6.663	774	778	781	rBV	597807	509556	36.84%	4.947%
5	6.898	814	818	822	rVB	1282284	1088132	78.67%	10.564%
6	7.057	841	845	848	rVB	437277	396701	28.68%	3.851%
7	7.457	909	913	916	rBV	321044	272476	19.70%	2.645%
8	8.180	1032	1036	1040	rBV	1720900	1383100	100.00%	13.428%
9	9.251	1215	1218	1222	rVB	680939	544378	39.36%	5.285%
10	9.933	1330	1334	1338	rBV	1424331	1334392	96.48%	12.955%
11	10.645	1452	1455	1458	rVB	50590	37579	2.72%	0.365%
12	10.716	1464	1467	1471	rBV	267675	218522	15.80%	2.121%
13	11.421	1583	1587	1590	rBV	1383010	1099131	79.47%	10.671%
14	13.004	1852	1856	1859	rBV	401158	342432	24.76%	3.324%
15	14.057	2031	2035	2039	rVB	1158135	1013285	73.26%	9.837%
16	15.539	2282	2287	2298	rVB	783804	993943	71.86%	9.650%


Sum of corrected areas: 10300432

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF110817\
Data File : BF100309.D
Acq On : 8 Nov 2017 23:13
Operator : SJ/JU
Sample : I6354-04 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
POOL-5001-0001-02

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

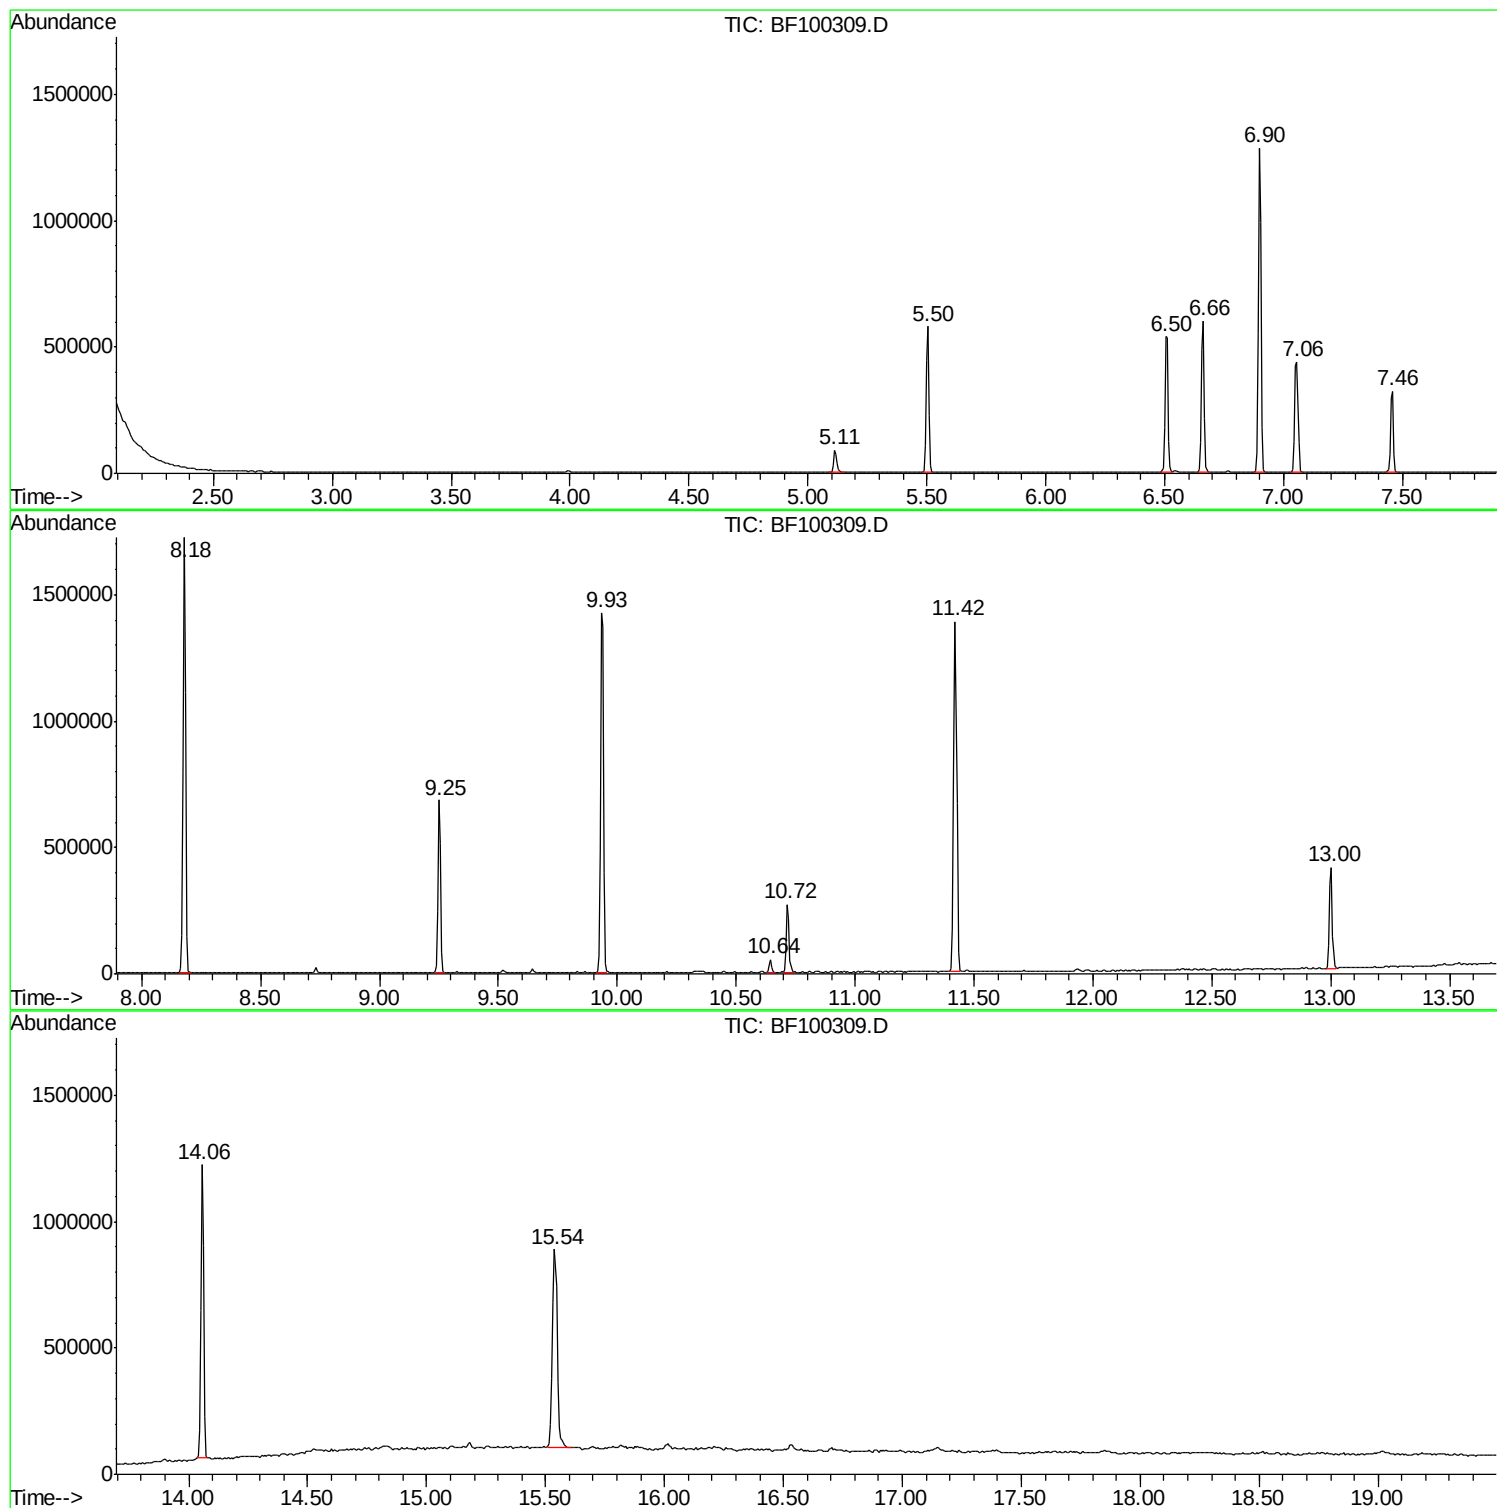

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA F\DATA\BF110817\
Data File : BF100309.D
Acq On : 8 Nov 2017 23:13
Operator : SJ/JU
Sample : I6354-04 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
POOL-5001-0001-02










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.66 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.66	9.37 ng	509556	1,4-Dichlorobenzene-d4	6.90

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	12
3		Amphetaminil	250	C17H18N2	017590-01-1	10
4		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
5		2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9

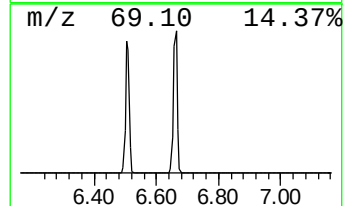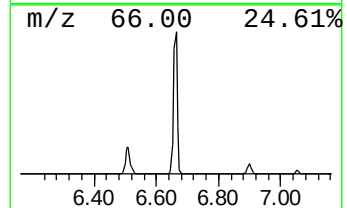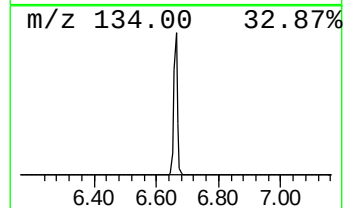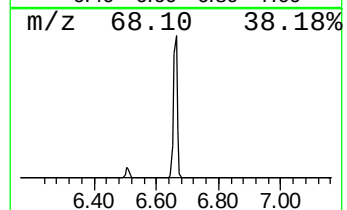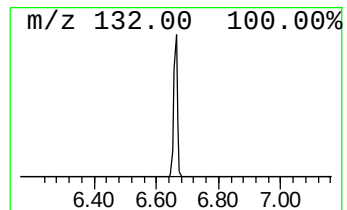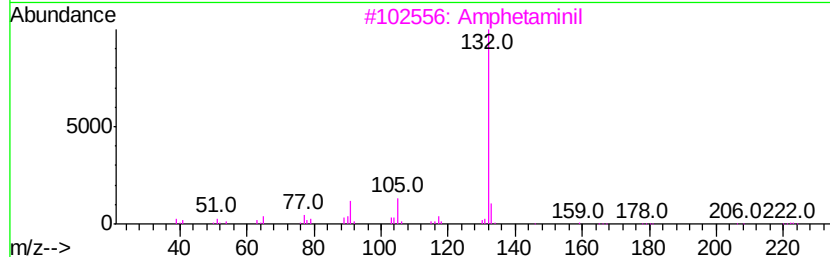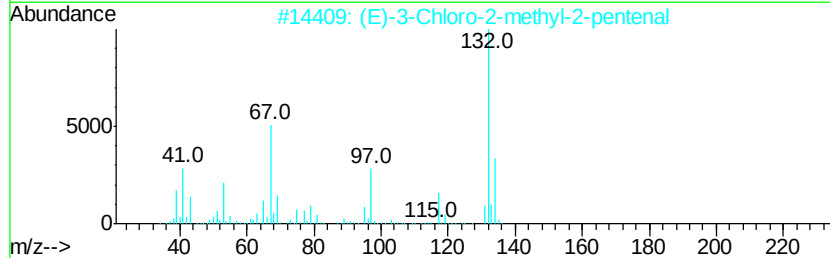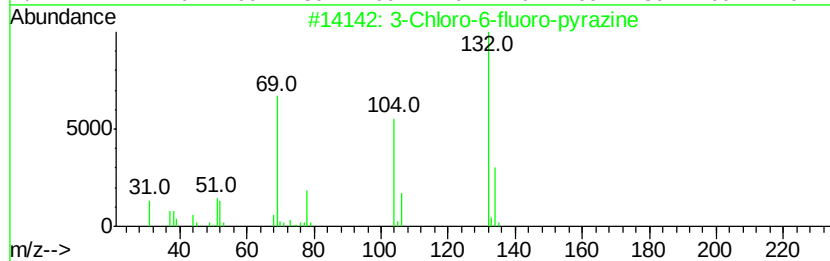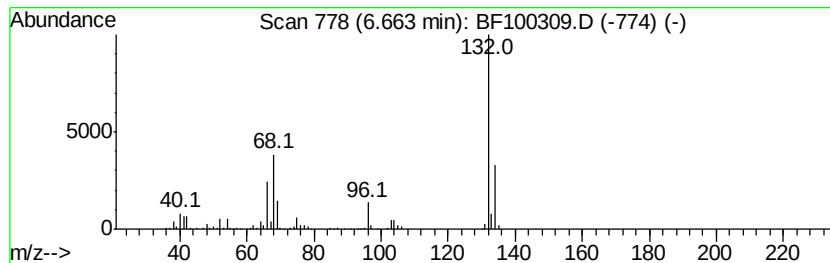

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF110817\
Data File : BF100309.D
Acq On : 8 Nov 2017 23:13
Operator : SJ/JU
Sample : I6354-04 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
POOL-5001-0001-02

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.66	6.66	9.4	ng	509556	1	6.90	1088130	20.0