


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA F\Data\BF110817\
 Data File : BF100316.D
 Acq On : 9 Nov 2017 2:47
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 08 14:33:31 2017

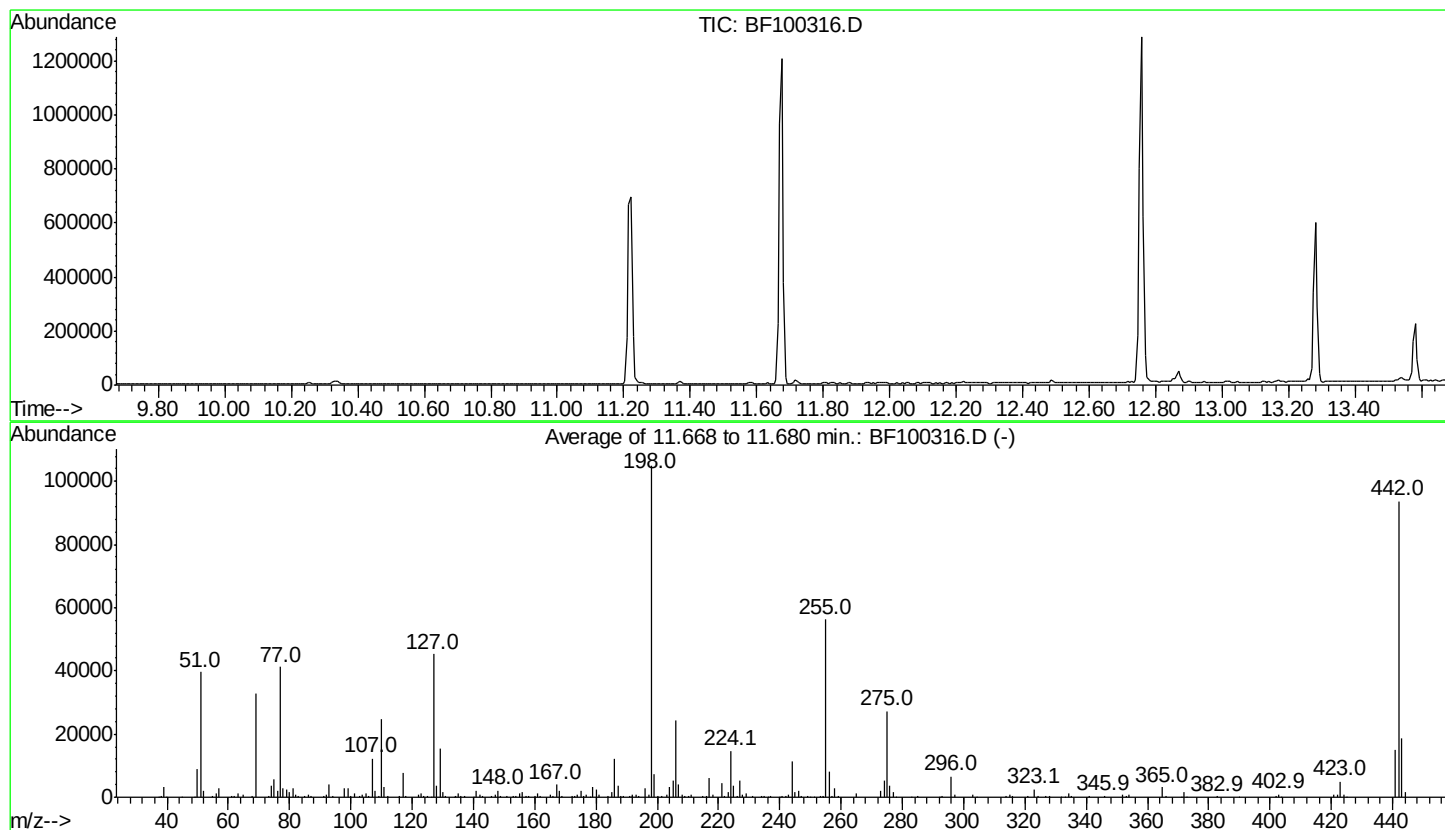

AutoFind: Scans 1629, 1630, 1631; Background Corrected with Scan 1624

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.7	39619	PASS
68	69	0.00	2	1.5	496	PASS
69	198	0.00	100	31.4	32950	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.2	45365	PASS
197	198	0.00	2	1.0	1017	PASS
198	198	100	100	100.0	104984	PASS
199	198	5	9	6.8	7132	PASS
275	198	10	60	25.9	27225	PASS
365	198	1	100	3.0	3121	PASS
441	443	0.01	100	82.3	15210	PASS
442	198	50	100	89.3	93749	PASS
443	442	15	24	19.7	18488	PASS