
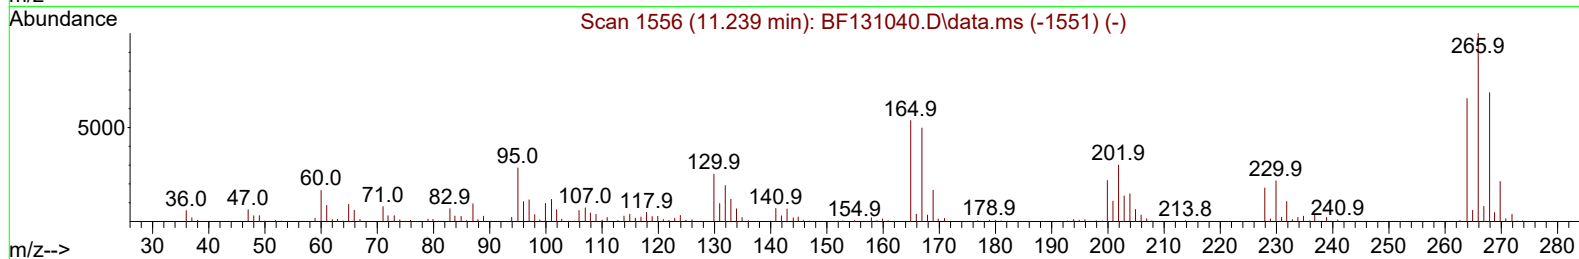
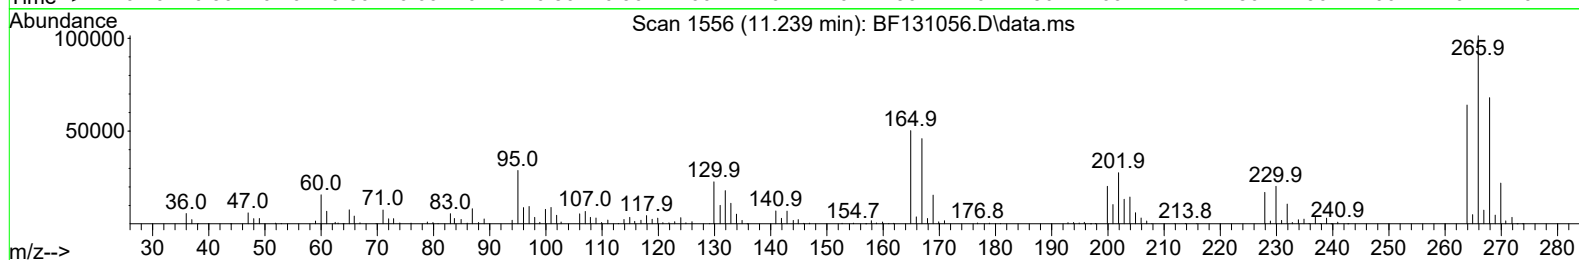


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110822\
Data File : BF131056.D
Acq On : 08 Nov 2022 09:13
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 09 07:01:53 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 08 01:40:43 2022
Response via : Initial Calibration

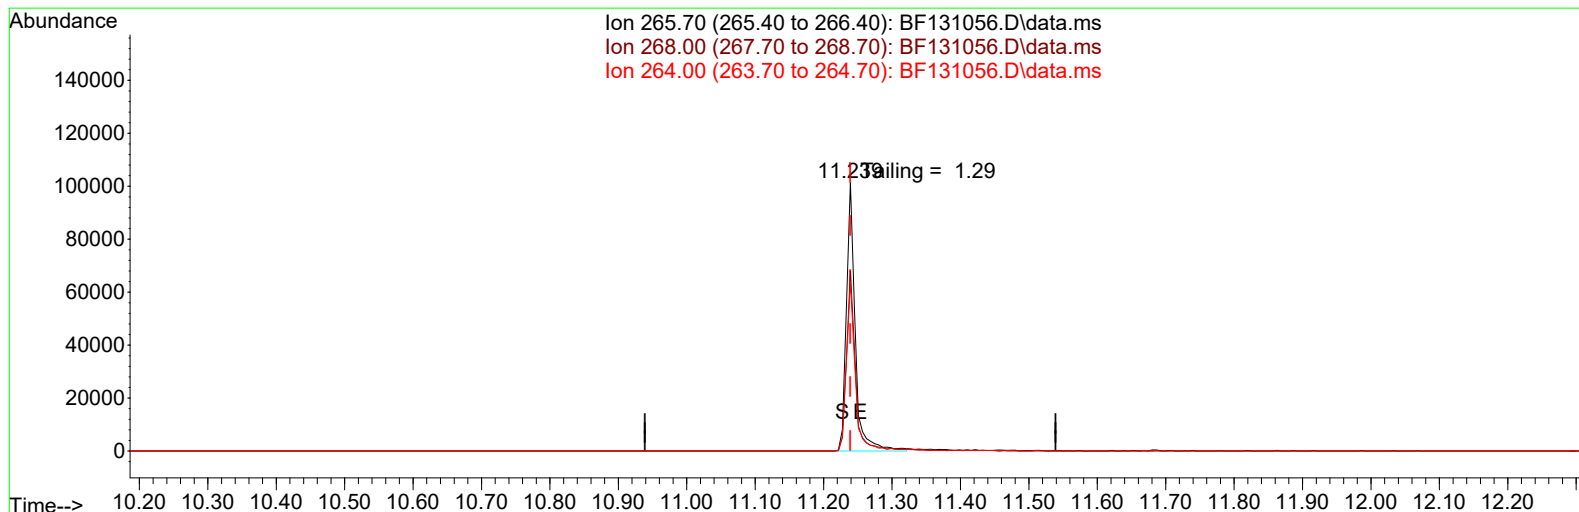

TIC: BF131056.D\data.ms

(70) Pentachlorophenol (C)




11.239min (+ 0.000) 36988.16 ng

response 90768

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	68.50	67.11
264.00	65.40	63.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110822\
Data File : BF131056.D
Acq On : 08 Nov 2022 09:13
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 09 07:01:53 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 08 01:40:43 2022
Response via : Initial Calibration

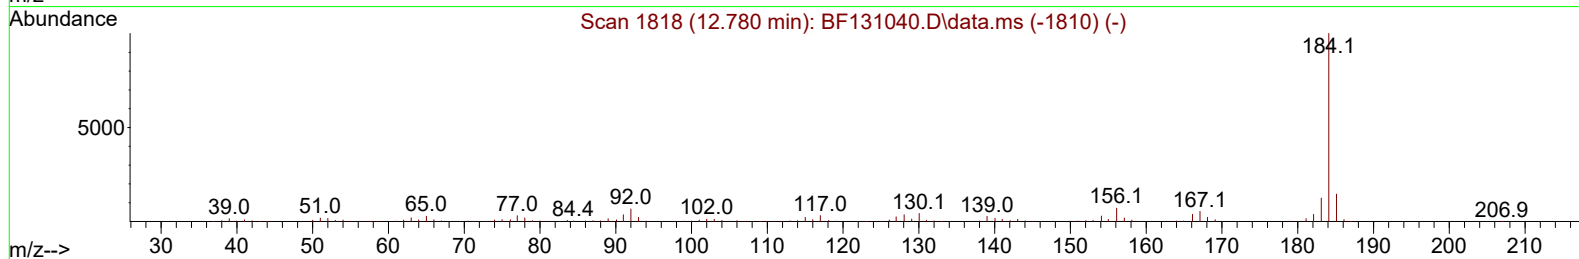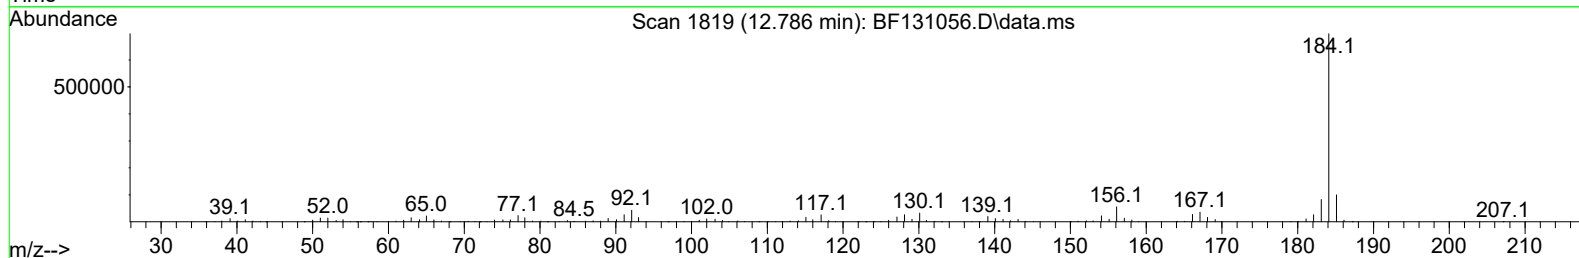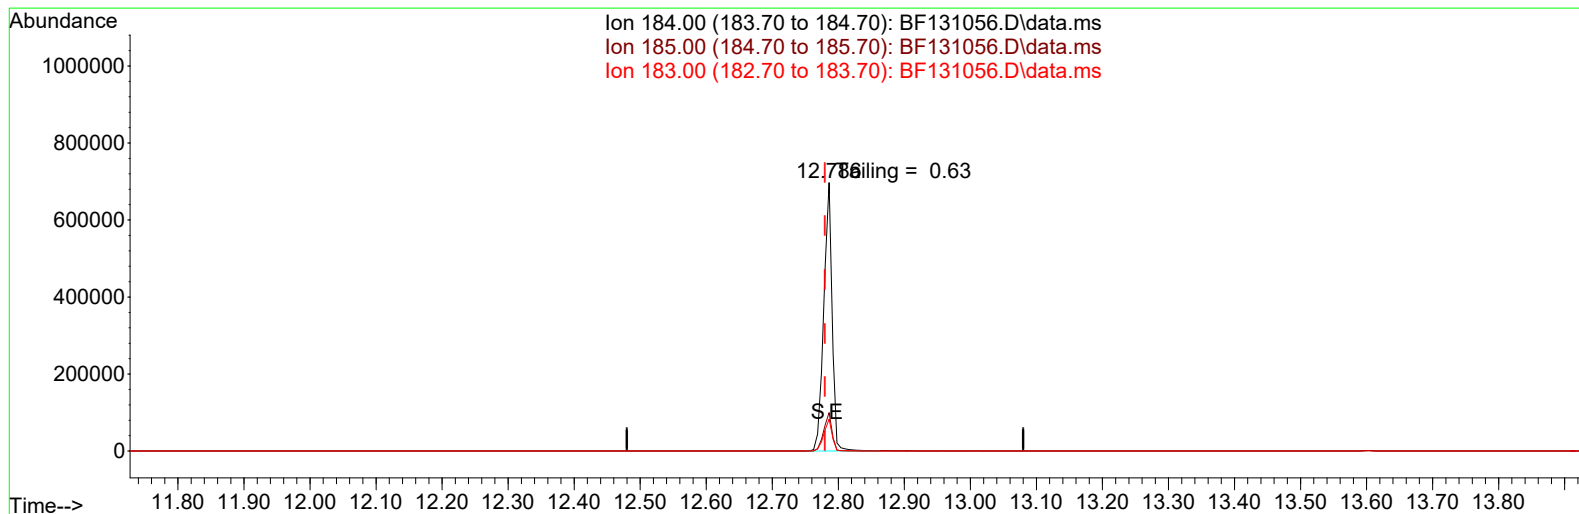

TIC: BF131056.D\data.ms

(77) Benzidine

12.786min (+ 0.006) 0.00 ng

response 615833

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.34
183.00	12.50	11.86
0.00	0.00	0.00