

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110822\
 Data File : BF131068.D
 Acq On : 08 Nov 2022 15:48
 Operator : CG\JU
 Sample : N5479-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TUL-ROS-1104

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF131068.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.357	18	46	48	rVB	5110420	41937299	100.00%	82.109%
2	4.516	408	413	420	rBV	586681	672823	1.60%	1.317%
3	5.134	513	518	524	rBV2	391601	554146	1.32%	1.085%
4	5.528	580	585	588	rBV	1777927	1507472	3.59%	2.951%
5	6.528	750	755	768	rBV	1573768	1451849	3.46%	2.843%
6	7.463	909	914	917	rBV	1253641	1114514	2.66%	2.182%
7	9.263	1215	1220	1223	rBV	1660421	1512698	3.61%	2.962%
8	10.733	1466	1470	1474	rBV	1005148	884677	2.11%	1.732%
9	13.027	1856	1860	1863	rBV	1712787	1439404	3.43%	2.818%




Sum of corrected areas: 51074882

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110822\
Data File : BF131068.D
Acq On : 08 Nov 2022 15:48
Operator : CG\JU
Sample : N5479-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TUL-ROS-1104

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

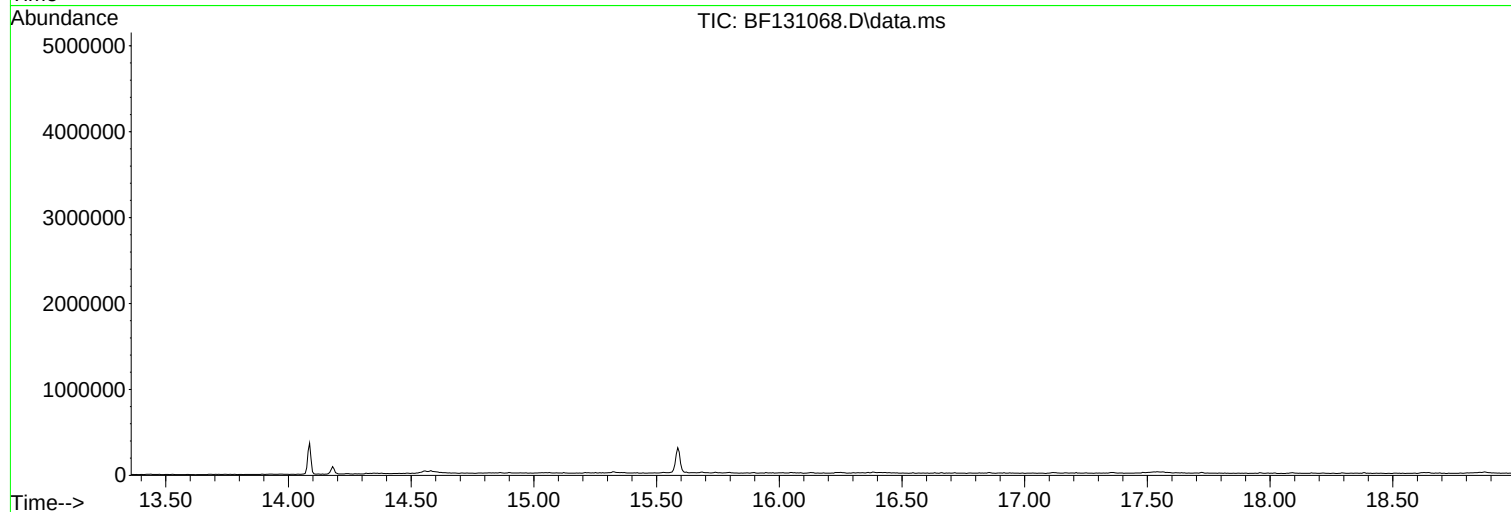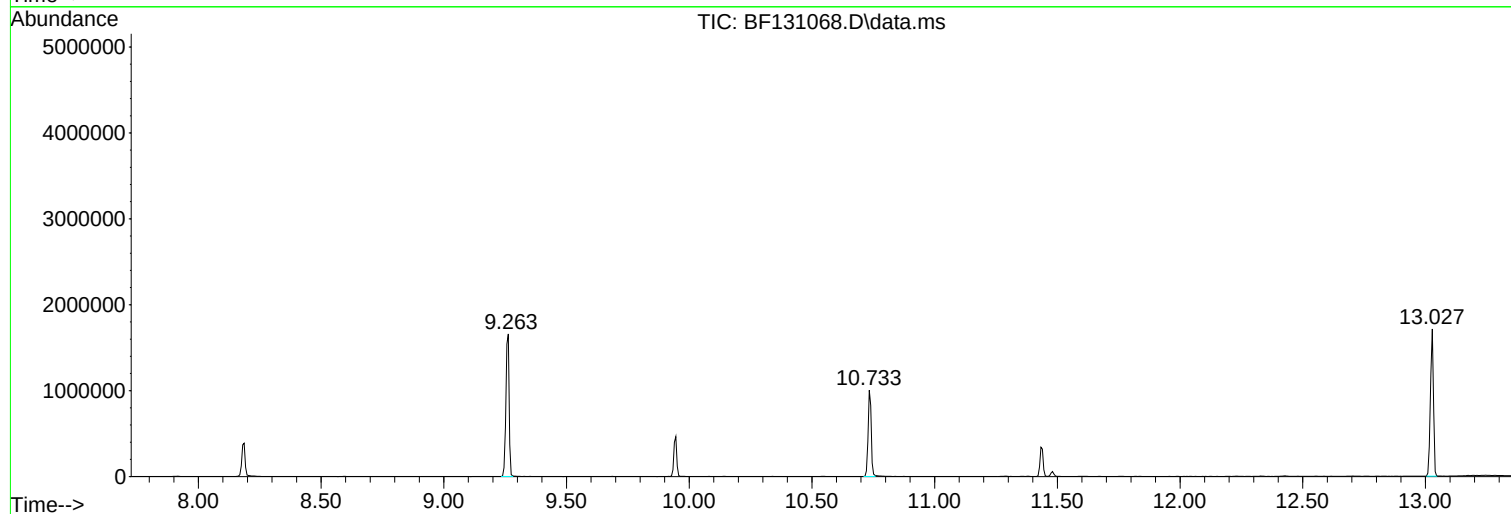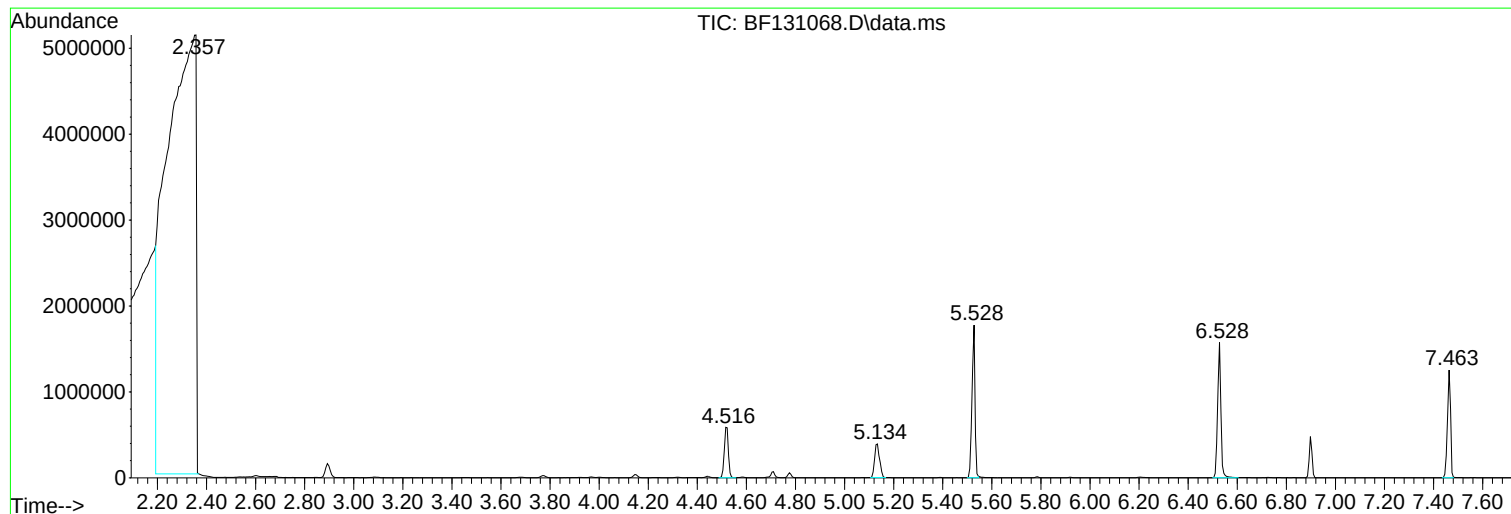

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110822\
Data File : BF131068.D
Acq On : 08 Nov 2022 15:48
Operator : CG\JU
Sample : N5479-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TUL-ROS-1104

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110822\
Data File : BF131068.D
Acq On : 08 Nov 2022 15:48
Operator : CG\JU
Sample : N5479-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TUL-ROS-1104

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------