
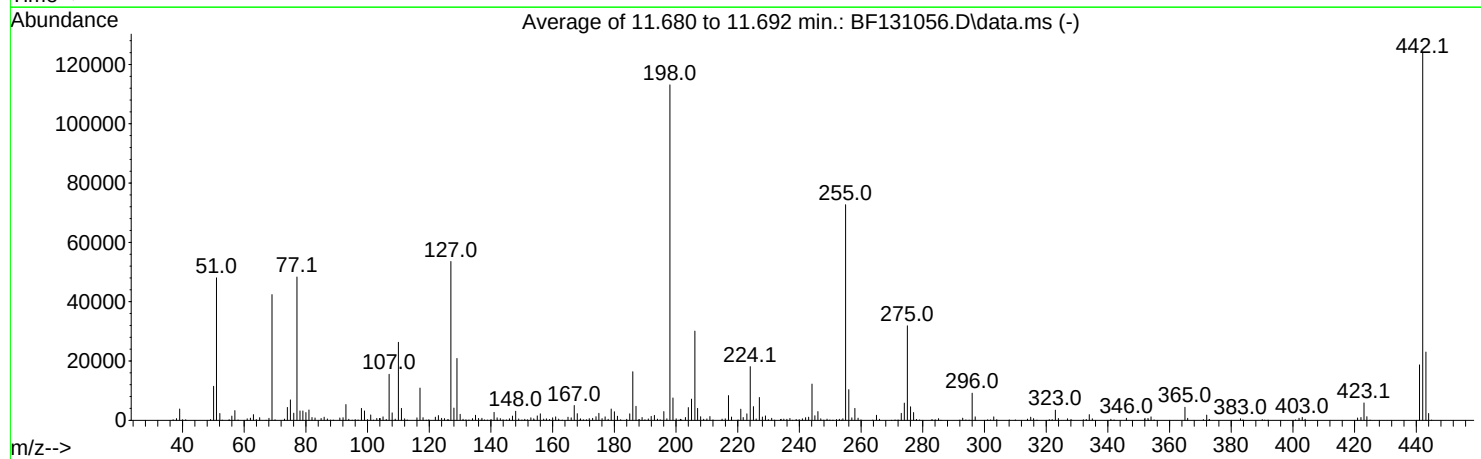


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110822\
 Data File : BF131056.D
 Acq On : 08 Nov 2022 09:13
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 08 01:40:43 2022

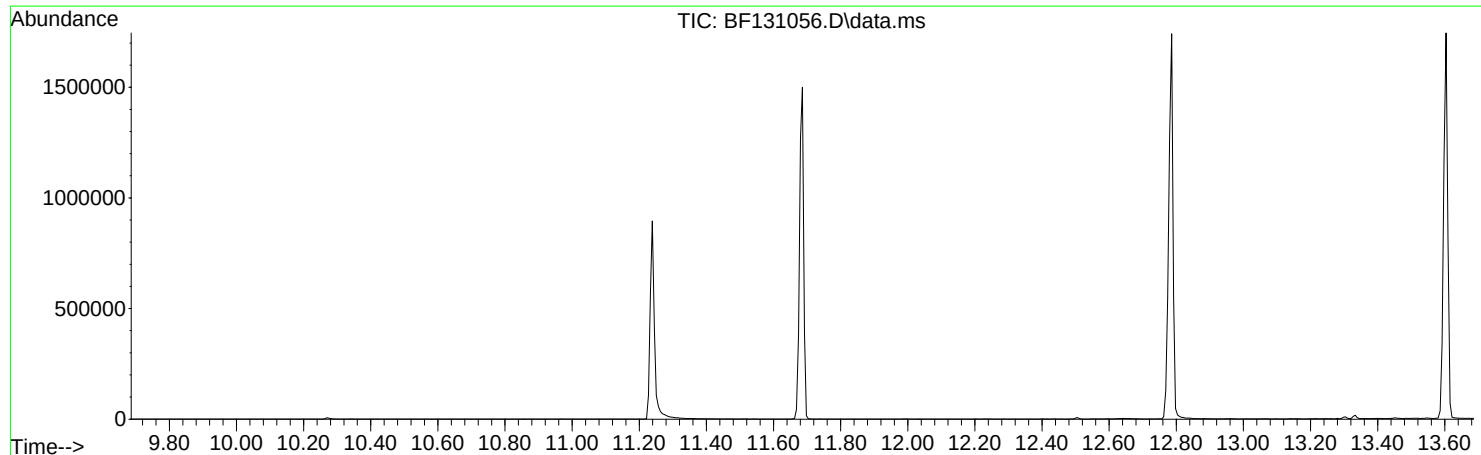




AutoFind: Scans 1631, 1632, 1633; Background Corrected with Scan 1625

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.5	48076	PASS
68	69	0.00	2	1.6	684	PASS
69	198	0.00	100	37.5	42380	PASS
70	69	0.00	2	0.4	183	PASS
127	198	10	80	47.4	53586	PASS
197	198	0.00	2	0.5	538	PASS
198	198	100	100	100.0	113149	PASS
199	198	5	9	6.7	7553	PASS
275	198	10	60	28.2	31882	PASS
365	198	1	100	3.9	4391	PASS
441	198	0.01	100	16.5	18701	PASS
442	442	50	100	100.0	124059	PASS
443	442	15	24	18.5	22997	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110822\
Data File : BF131056.D
Acq On : 08 Nov 2022 09:13
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 09 07:01:53 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 08 01:40:43 2022
Response via : Initial Calibration

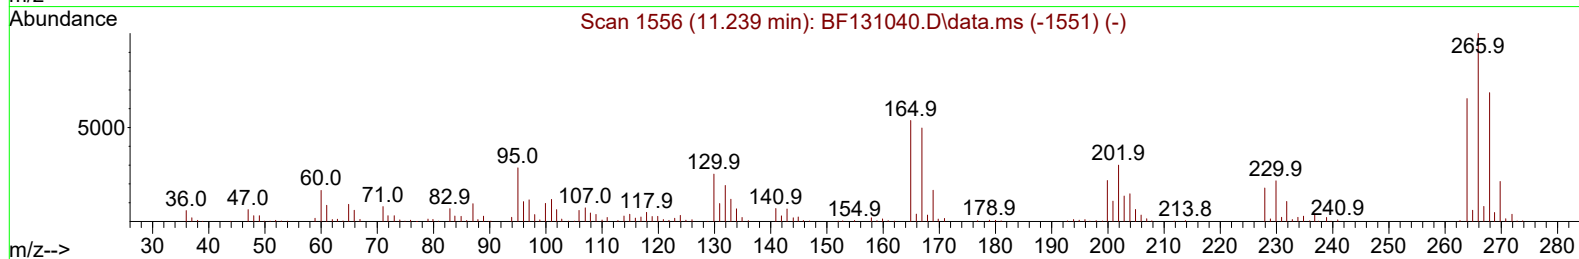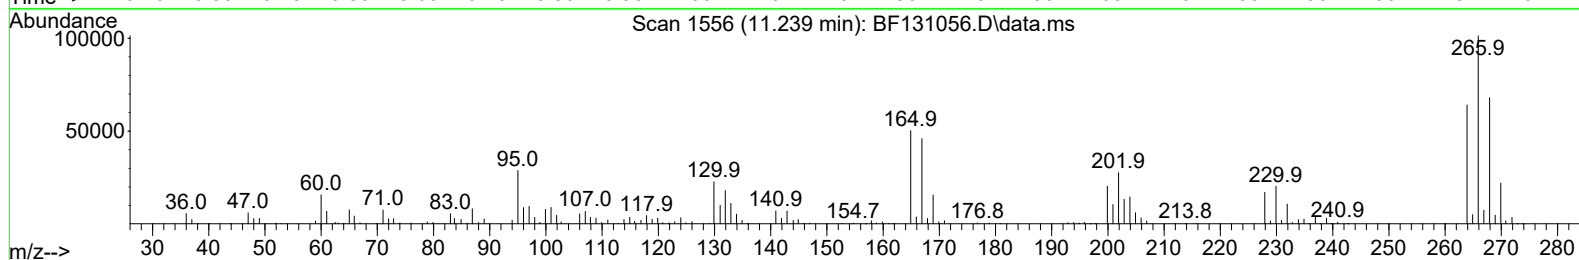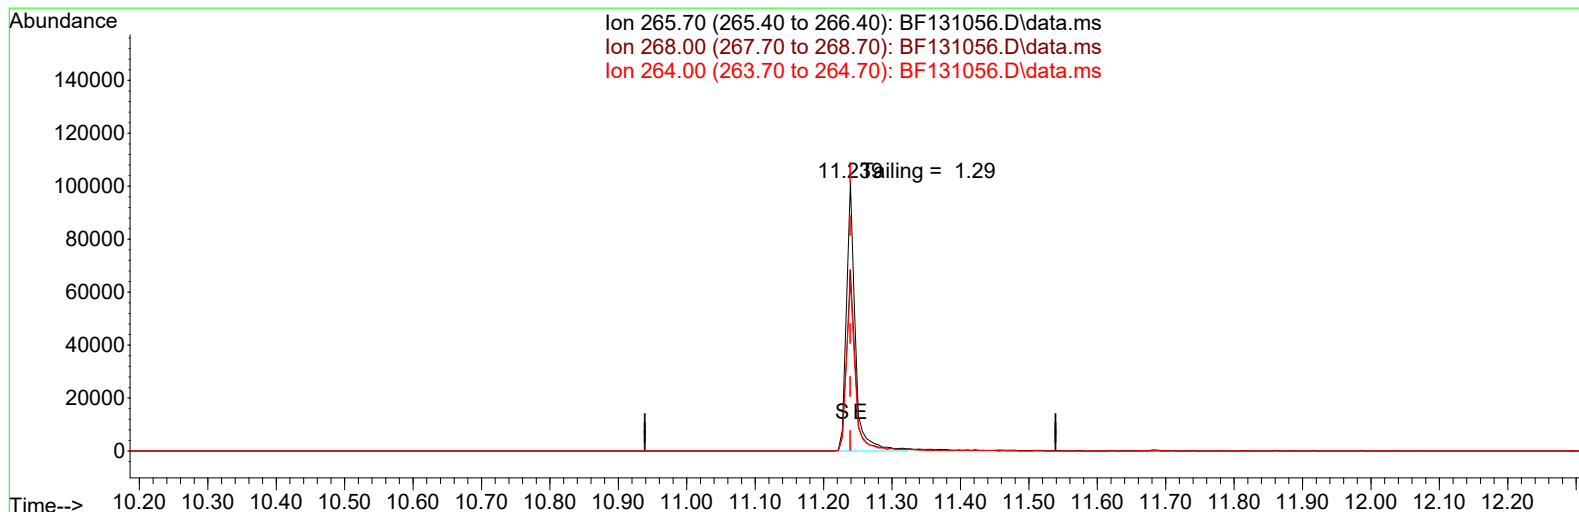

TIC: BF131056.D\data.ms

(70) Pentachlorophenol (C)

11.239min (+ 0.000) 36988.16 ng




response 90768

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	68.50	67.11
264.00	65.40	63.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110822\
Data File : BF131056.D
Acq On : 08 Nov 2022 09:13
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 09 07:01:53 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 08 01:40:43 2022
Response via : Initial Calibration

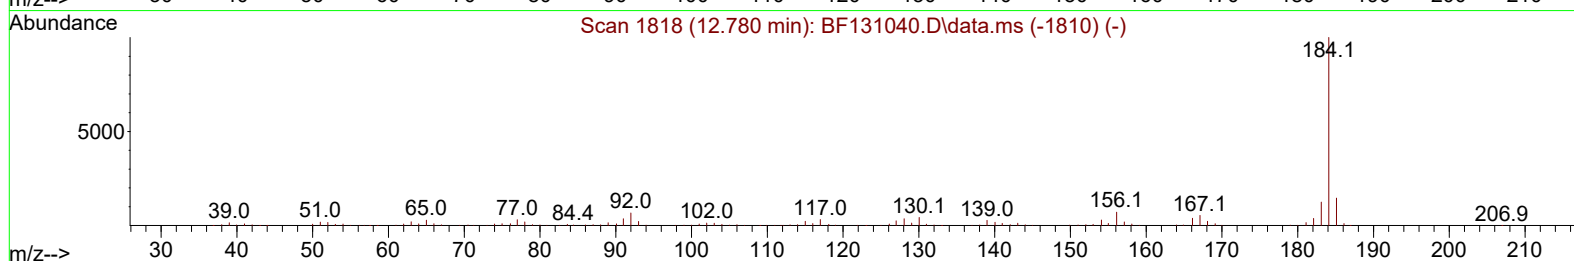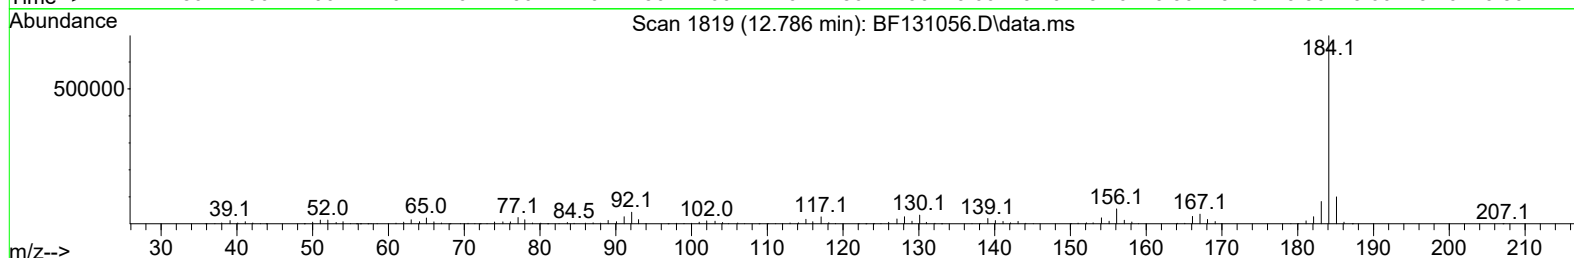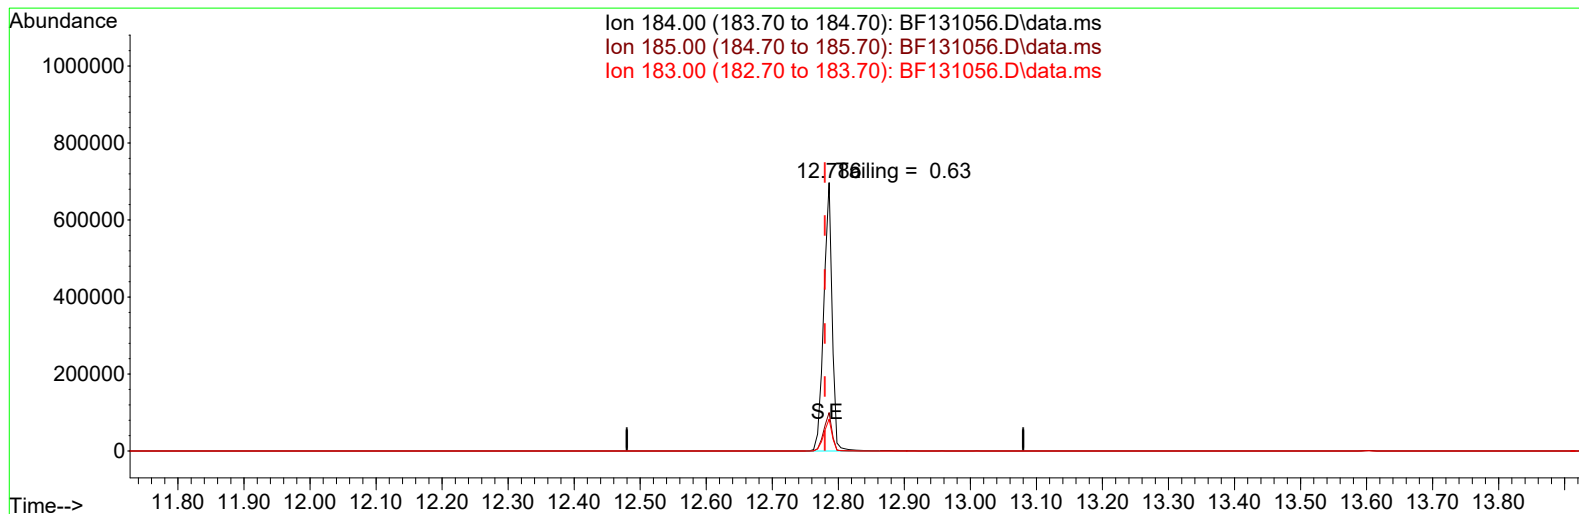

TIC: BF131056.D\data.ms

(77) Benzidine

12.786min (+ 0.006) 0.00 ng

response 615833

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.34
183.00	12.50	11.86
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/8/2022	BNA_F	<u>BF131056.D</u>
Compound Name	Response	Retention Time
DDT	283532	13.604
DDD	5154	13.333
DDE	487	12.963
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5641	289173	1.95

Instrument :
BNA_F
ClientSampleId :
DFTPP