

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110824\
 Data File : BF140287.D
 Acq On : 08 Nov 2024 10:02
 Operator : RC/JU
 Sample : PB164765BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB164765BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110524.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF140287.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.263	21	29	41	rVB	109015	201310	2.03%	0.412%
2	5.510	574	581	586	rBV	4024868	5949868	60.03%	12.188%
3	6.504	742	750	756	rBV	3680101	6003232	60.57%	12.297%
4	6.875	808	813	818	rBV	903899	1097371	11.07%	2.248%
5	7.439	901	909	914	rBV	2750403	4151444	41.89%	8.504%
6	8.157	1024	1031	1036	rBV	1091792	1444499	14.57%	2.959%
7	9.233	1206	1214	1219	rBV	5251893	7685364	77.54%	15.743%
8	9.916	1322	1330	1335	rBV	1342582	1786593	18.03%	3.660%
9	10.710	1456	1465	1470	rBV	3928255	5487642	55.37%	11.241%
10	11.404	1576	1583	1592	rBV	1611620	2050652	20.69%	4.201%
11	13.004	1847	1855	1860	rBV	6583600	9910971	100.00%	20.302%
12	14.051	2027	2033	2045	rBV	1345218	1768286	17.84%	3.622%
13	15.545	2281	2287	2300	rVB	765620	1281445	12.93%	2.625%




Sum of corrected areas: 48818677

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110824\
Data File : BF140287.D
Acq On : 08 Nov 2024 10:02
Operator : RC/JU
Sample : PB164765BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB164765BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

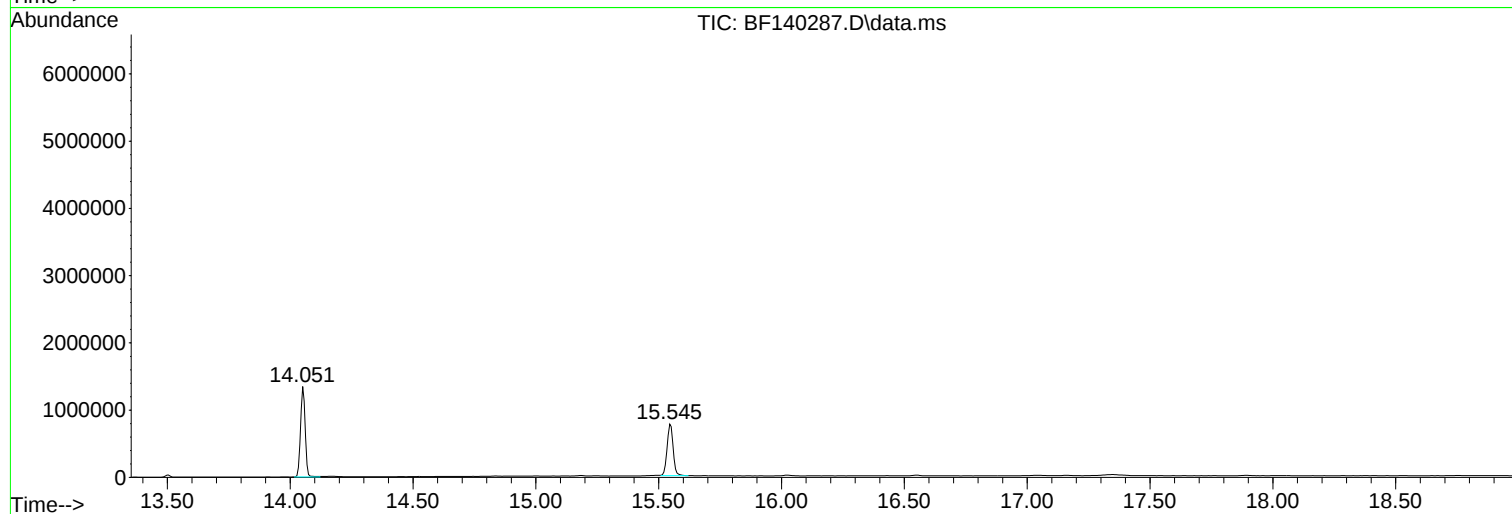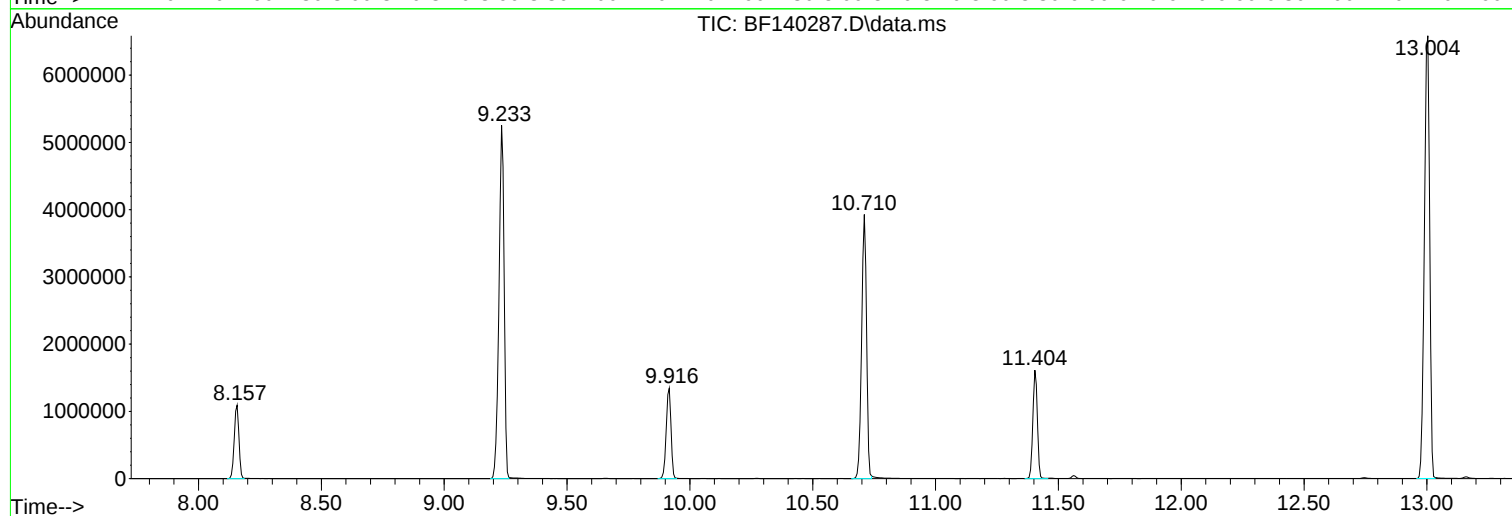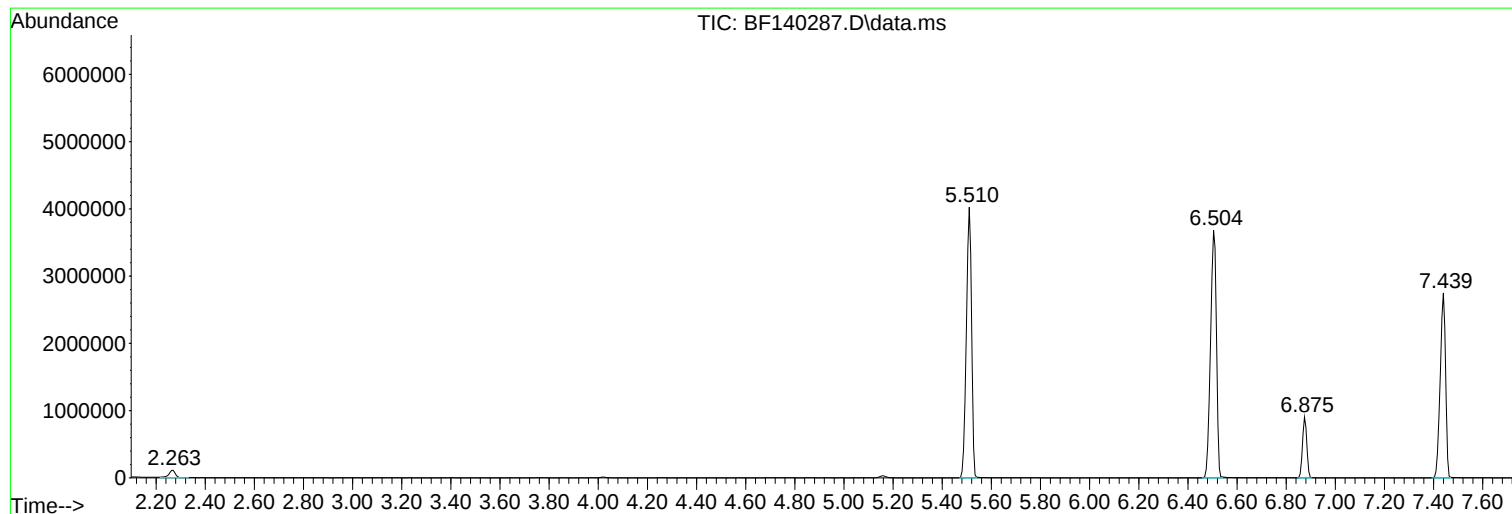

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110824\
Data File : BF140287.D
Acq On : 08 Nov 2024 10:02
Operator : RC/JU
Sample : PB164765BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB164765BL









Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.263	3.67 ng	201310	1,4-Dichlorobenzene-d4	6.875

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	39
3			2-Methyl-5-hexen-3-ol	114	C7H14O	032815-70-6	25
4			Octanal, 7-methoxy-3,7-dimethyl-	186	C11H22O2	003613-30-7	17
5			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	12

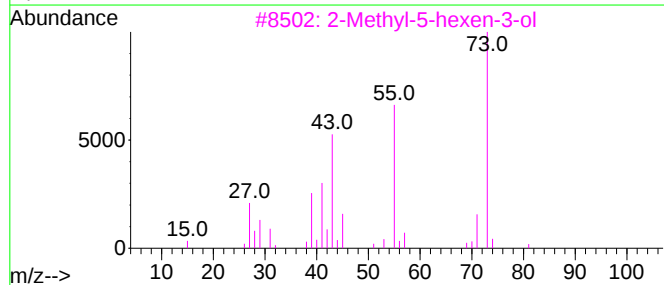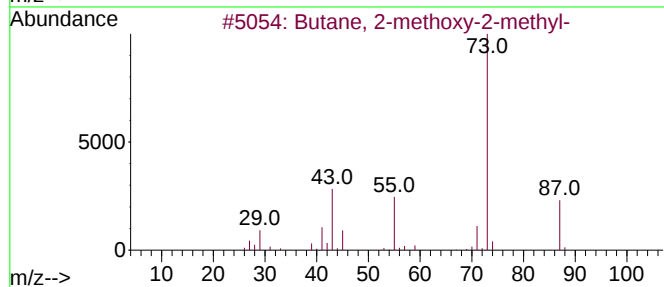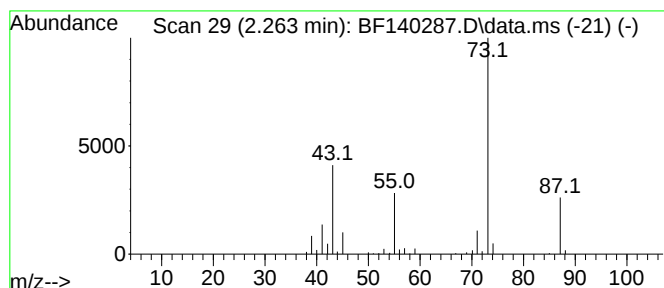

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110824\
Data File : BF140287.D
Acq On : 08 Nov 2024 10:02
Operator : RC/JU
Sample : PB164765BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB164765BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.263	3.7	ng	201310	1	6.875	1097370	20.0