
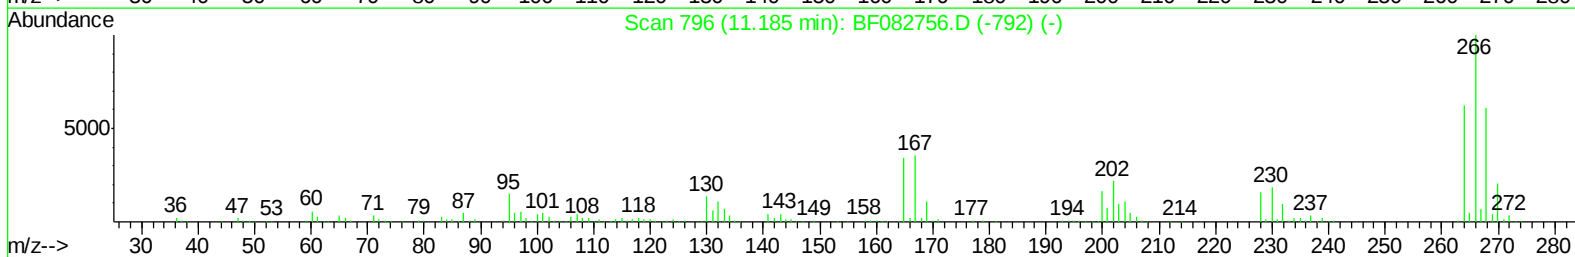
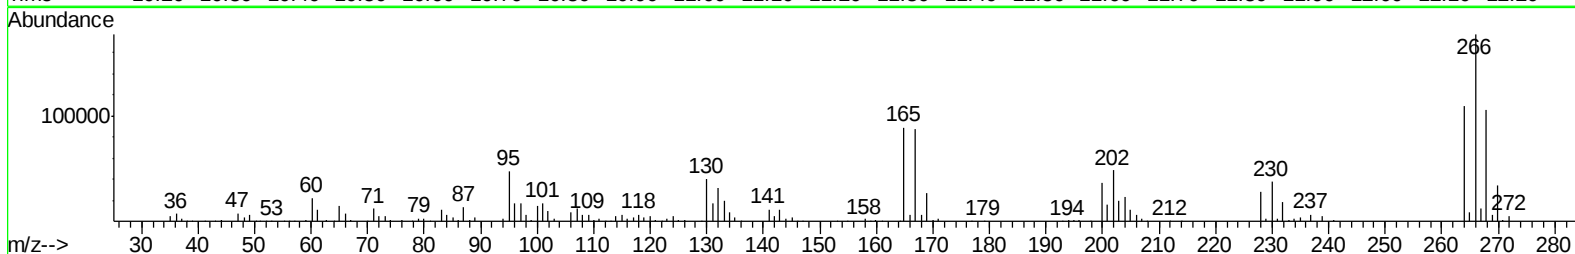


Data Path : Z:\HPCHEM1\BNA F\DATA\BF110915\
Data File : BF082830.D
Acq On : 9 Nov 2015 11:36
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 10 06:59:26 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 07 02:32:49 2015
Response via : Initial Calibration

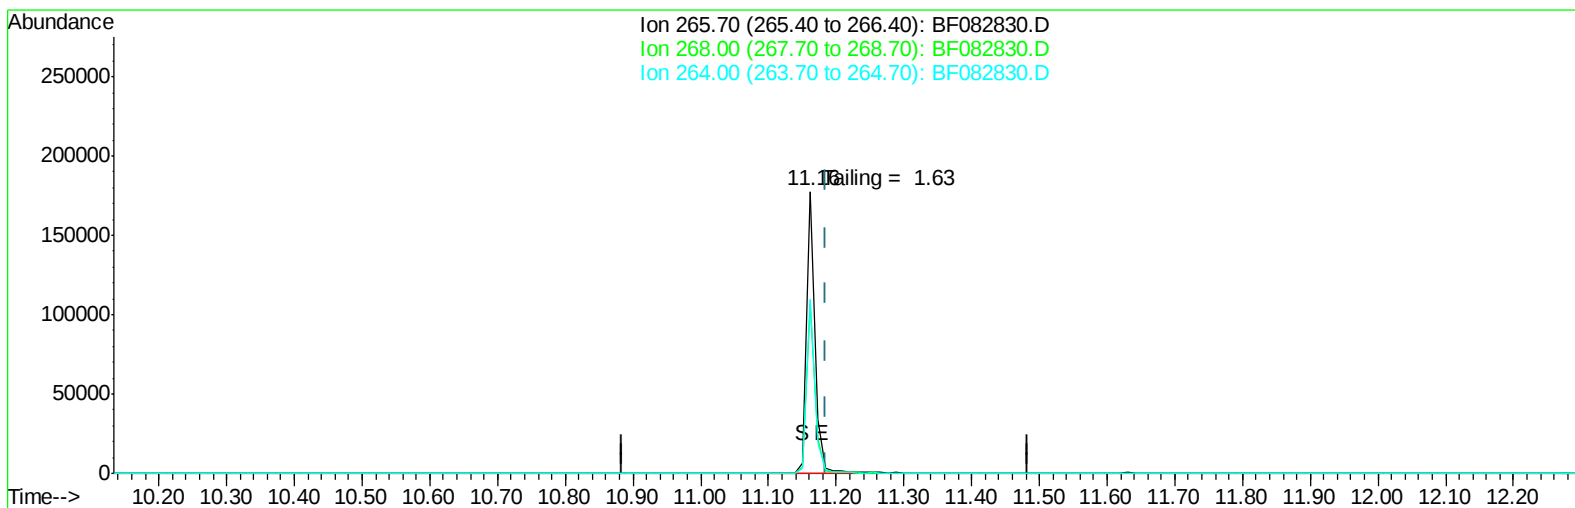

TIC: BF082830.D

(69) Pentachlorophenol (C)




11.162min (-0.023) 45035.82ng m

response 154431

Ion	Exp%	Act%
265.70	100	100
268.00	63.80	59.89
264.00	63.20	61.63
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF110915\
 Data File : BF082830.D
 Acq On : 9 Nov 2015 11:36
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 10 06:59:26 2015
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Nov 07 02:32:49 2015
 Response via : Initial Calibration

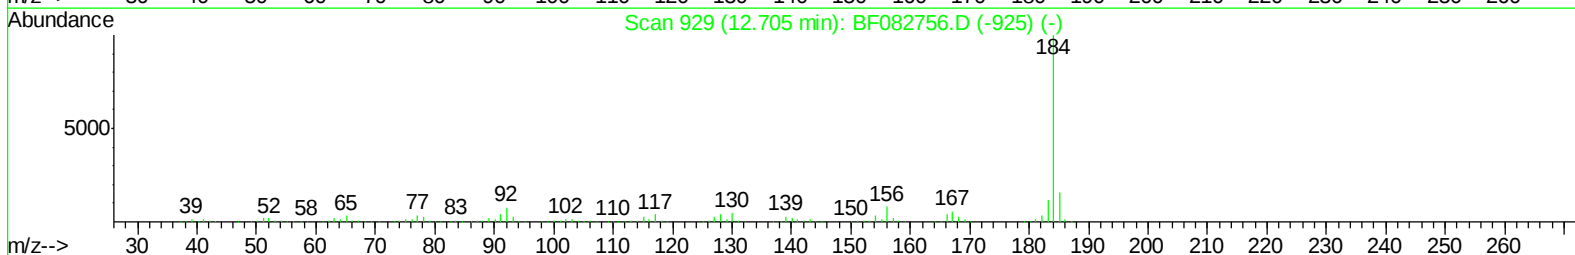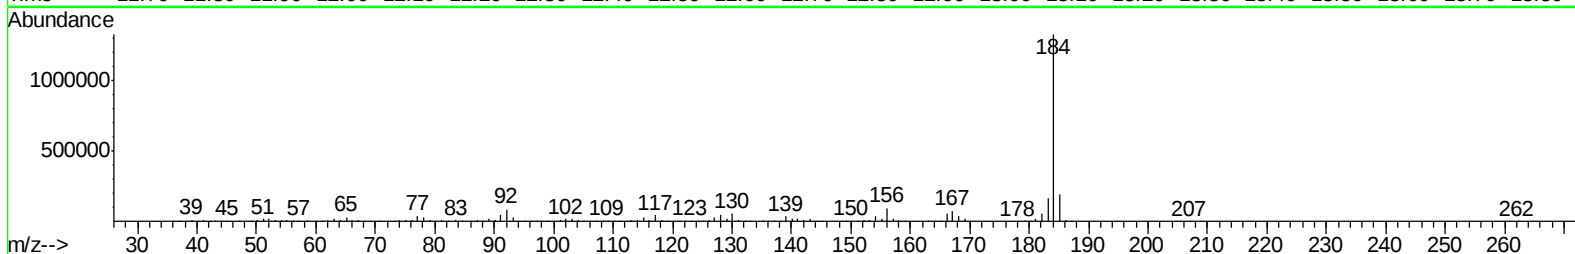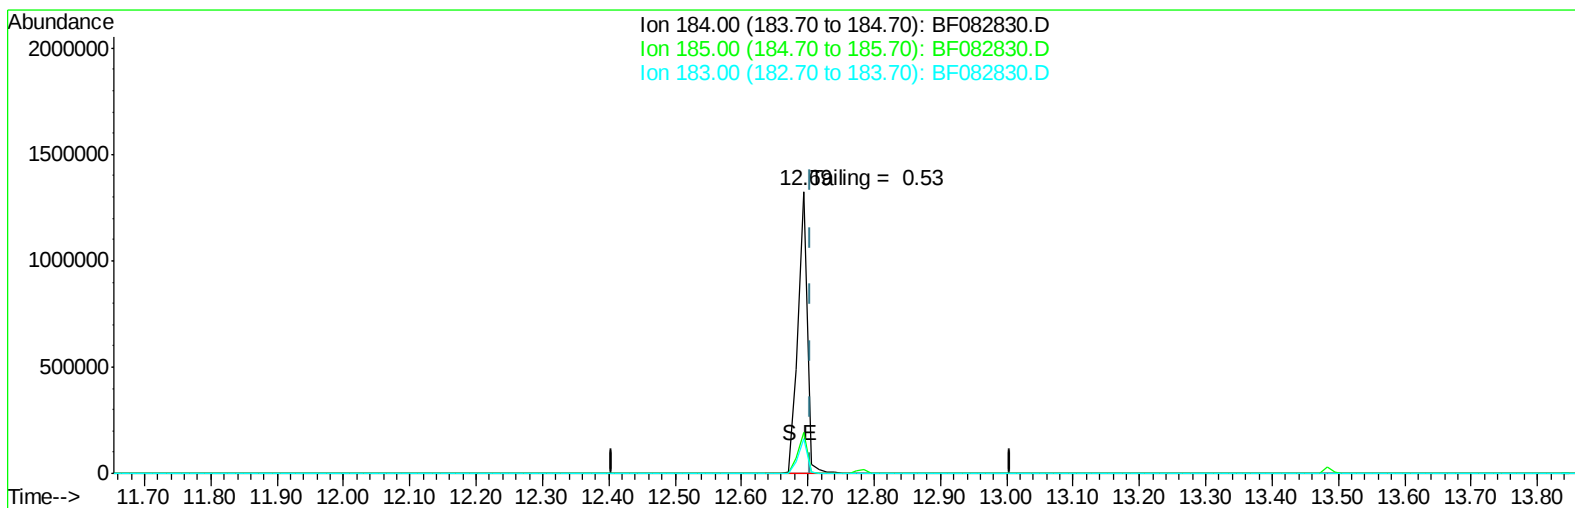

TIC: BF082830.D

(76) Benzidine

12.694min (-0.011) 44607.34ng

response 1308102

Ion	Exp%	Act%
184.00	100	100
185.00	15.00	14.44
183.00	12.00	12.08
0.00	0.00	0.00