
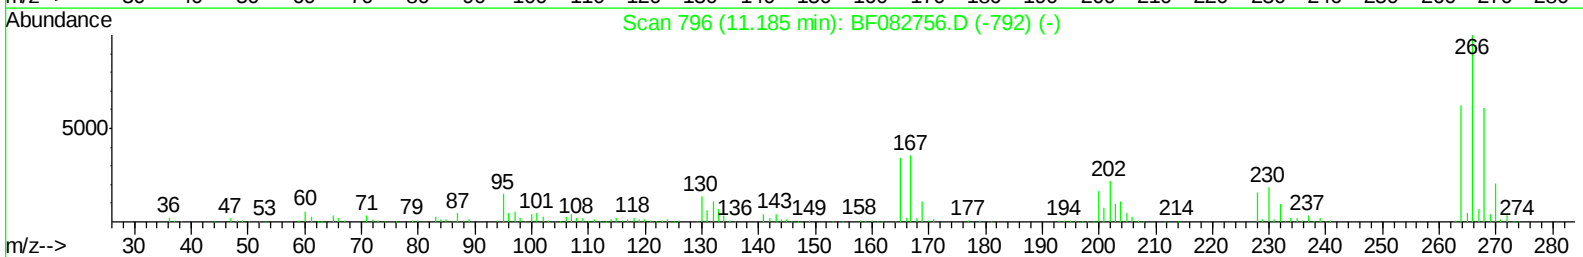
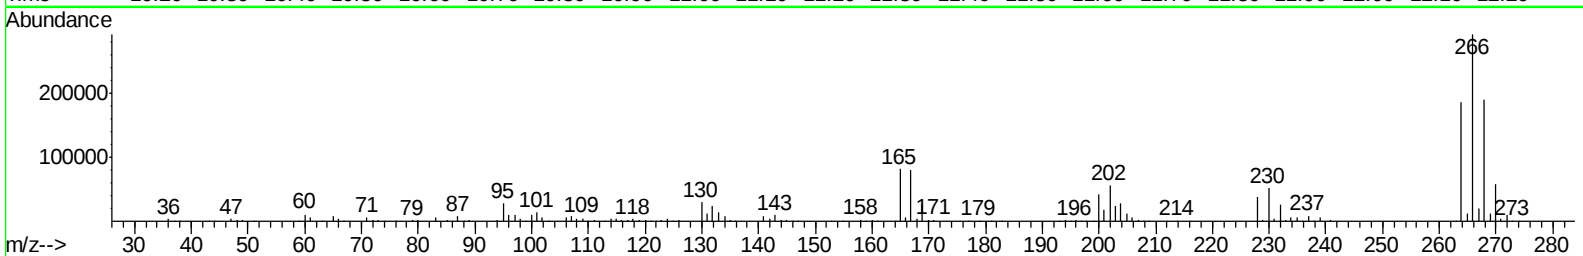


Data Path : Z:\HPCHEM1\BNA F\DATA\BF110915\
Data File : BF082847.D
Acq On : 10 Nov 2015 1:45
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 10 07:00:33 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 07 02:32:49 2015
Response via : Initial Calibration

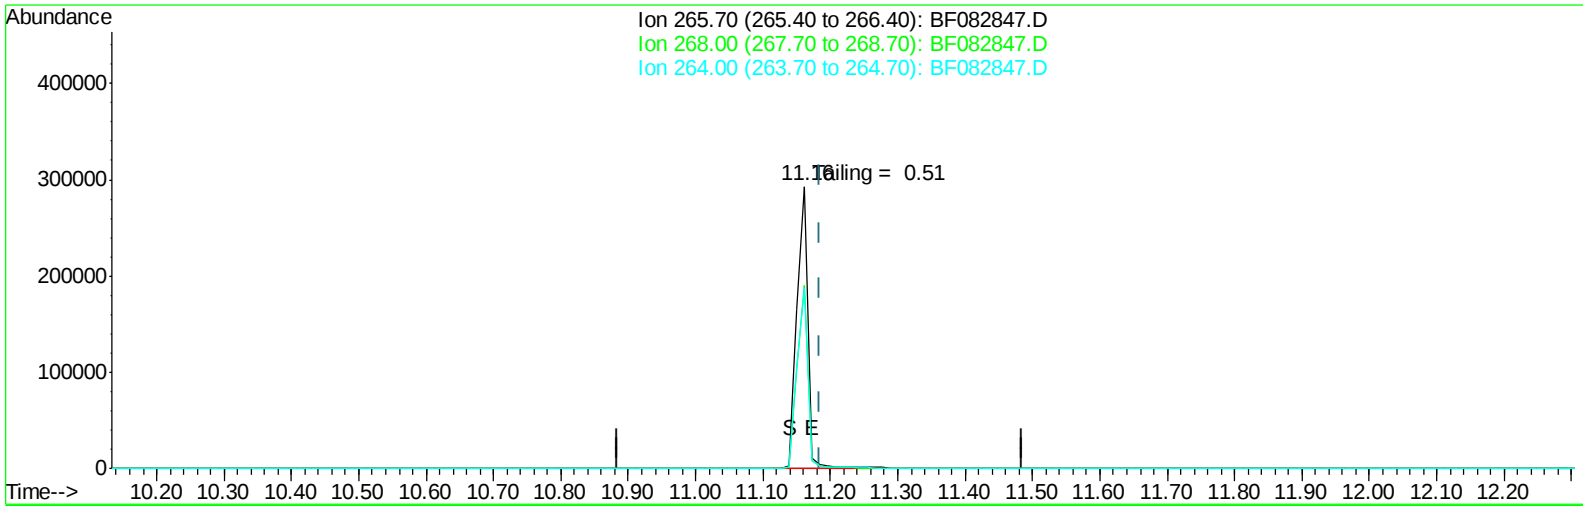

TIC: BF082847.D

(69) Pentachlorophenol (C)




11.162min (-0.023) 28140.92ng

response 329469

Ion	Exp%	Act%
265.70	100	100
268.00	63.80	64.86
264.00	63.20	63.92
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF110915\
Data File : BF082847.D
Acq On : 10 Nov 2015 1:45
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 10 07:00:33 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 07 02:32:49 2015
Response via : Initial Calibration

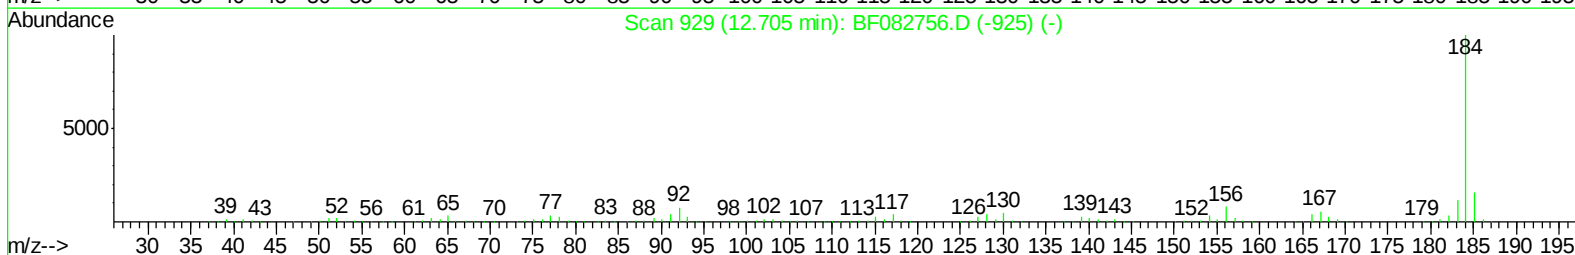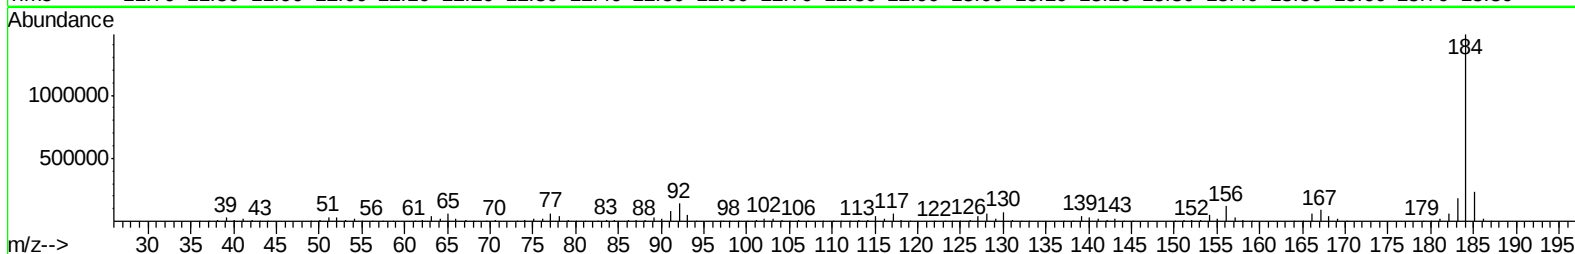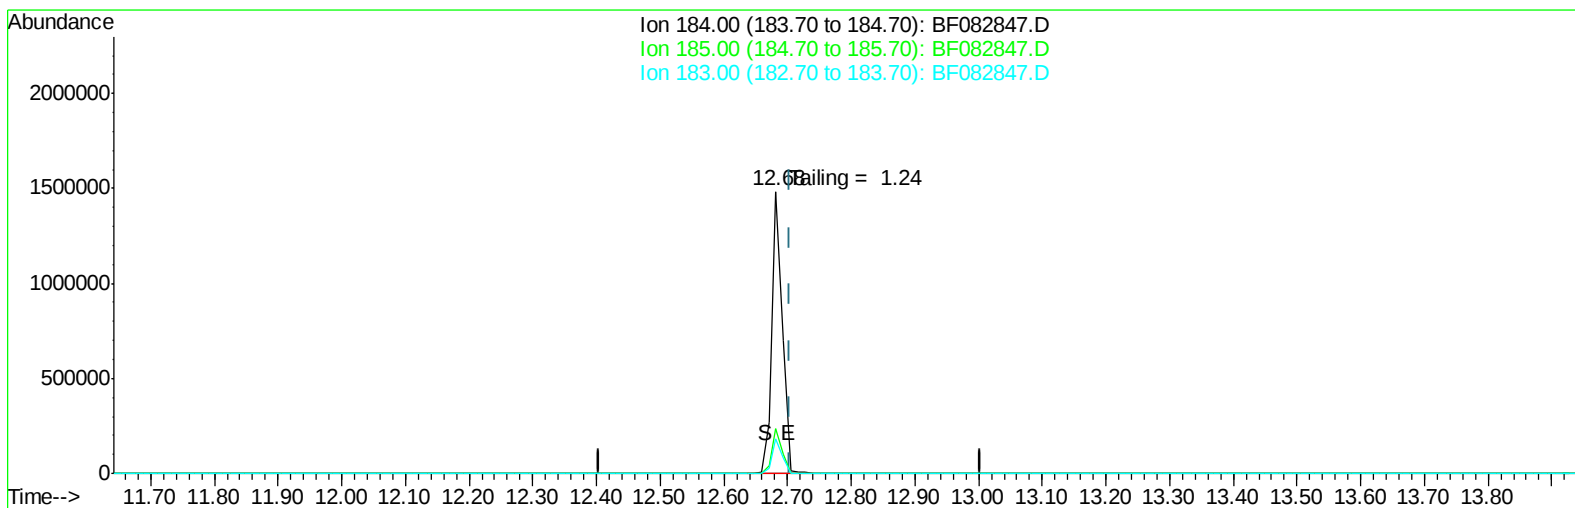

TIC: BF082847.D

(76) Benzidine

12.682min (-0.023) 0.00ng

response 1717276

Ion	Exp%	Act%
184.00	100	100
185.00	15.00	15.79
183.00	12.00	12.34
0.00	0.00	0.00