

Data Path : Z:\HPCHEM1\BNA F\DATA\BF110915\
 Data File : BF082839.D
 Acq On : 9 Nov 2015 19:55
 Operator : UM/IZ
 Sample : G4306-14
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 D2

Quant Time: Nov 10 03:40:47 2015
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Nov 07 02:32:49 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.83	152	243665	20.00	ng	-0.02
21) Naphthalene-d8	8.11	136	839758	20.00	ng	-0.03
38) Acenaphthene-d10	9.87	164	443601	20.00	ng	-0.02
63) Phenanthrene-d10	11.34	188	782736	20.00	ng	-0.03
75) Chrysene-d12	13.99	240	765789	20.00	ng	-0.03
86) Perylene-d12	15.41	264	672762	20.00	ng	-0.05
System Monitoring Compounds						
5) 2-Fluorophenol	5.45	112	2128876	135.94	ng	0.00
7) Phenol-d6	6.48	99	2931039	140.78	ng	0.00
23) Nitrobenzene-d5	7.39	82	1635635	84.75	ng	-0.02
41) 2,4,6-Tribromophenol	10.66	330	667205	131.18	ng	-0.02
44) 2-Fluorobiphenyl	9.20	172	2522498	81.50	ng	-0.02
78) Terphenyl-d14	12.94	244	2610309	80.85	ng	-0.02
Target Compounds						
49) Dimethylphthalate	9.58	163	641100	17.64	ng	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF110915\
Data File : BF082839.D
Acq On : 9 Nov 2015 19:55
Operator : UM/IZ
Sample : G4306-14
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
D2

Quant Time: Nov 10 03:40:47 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 07 02:32:49 2015
Response via : Initial Calibration

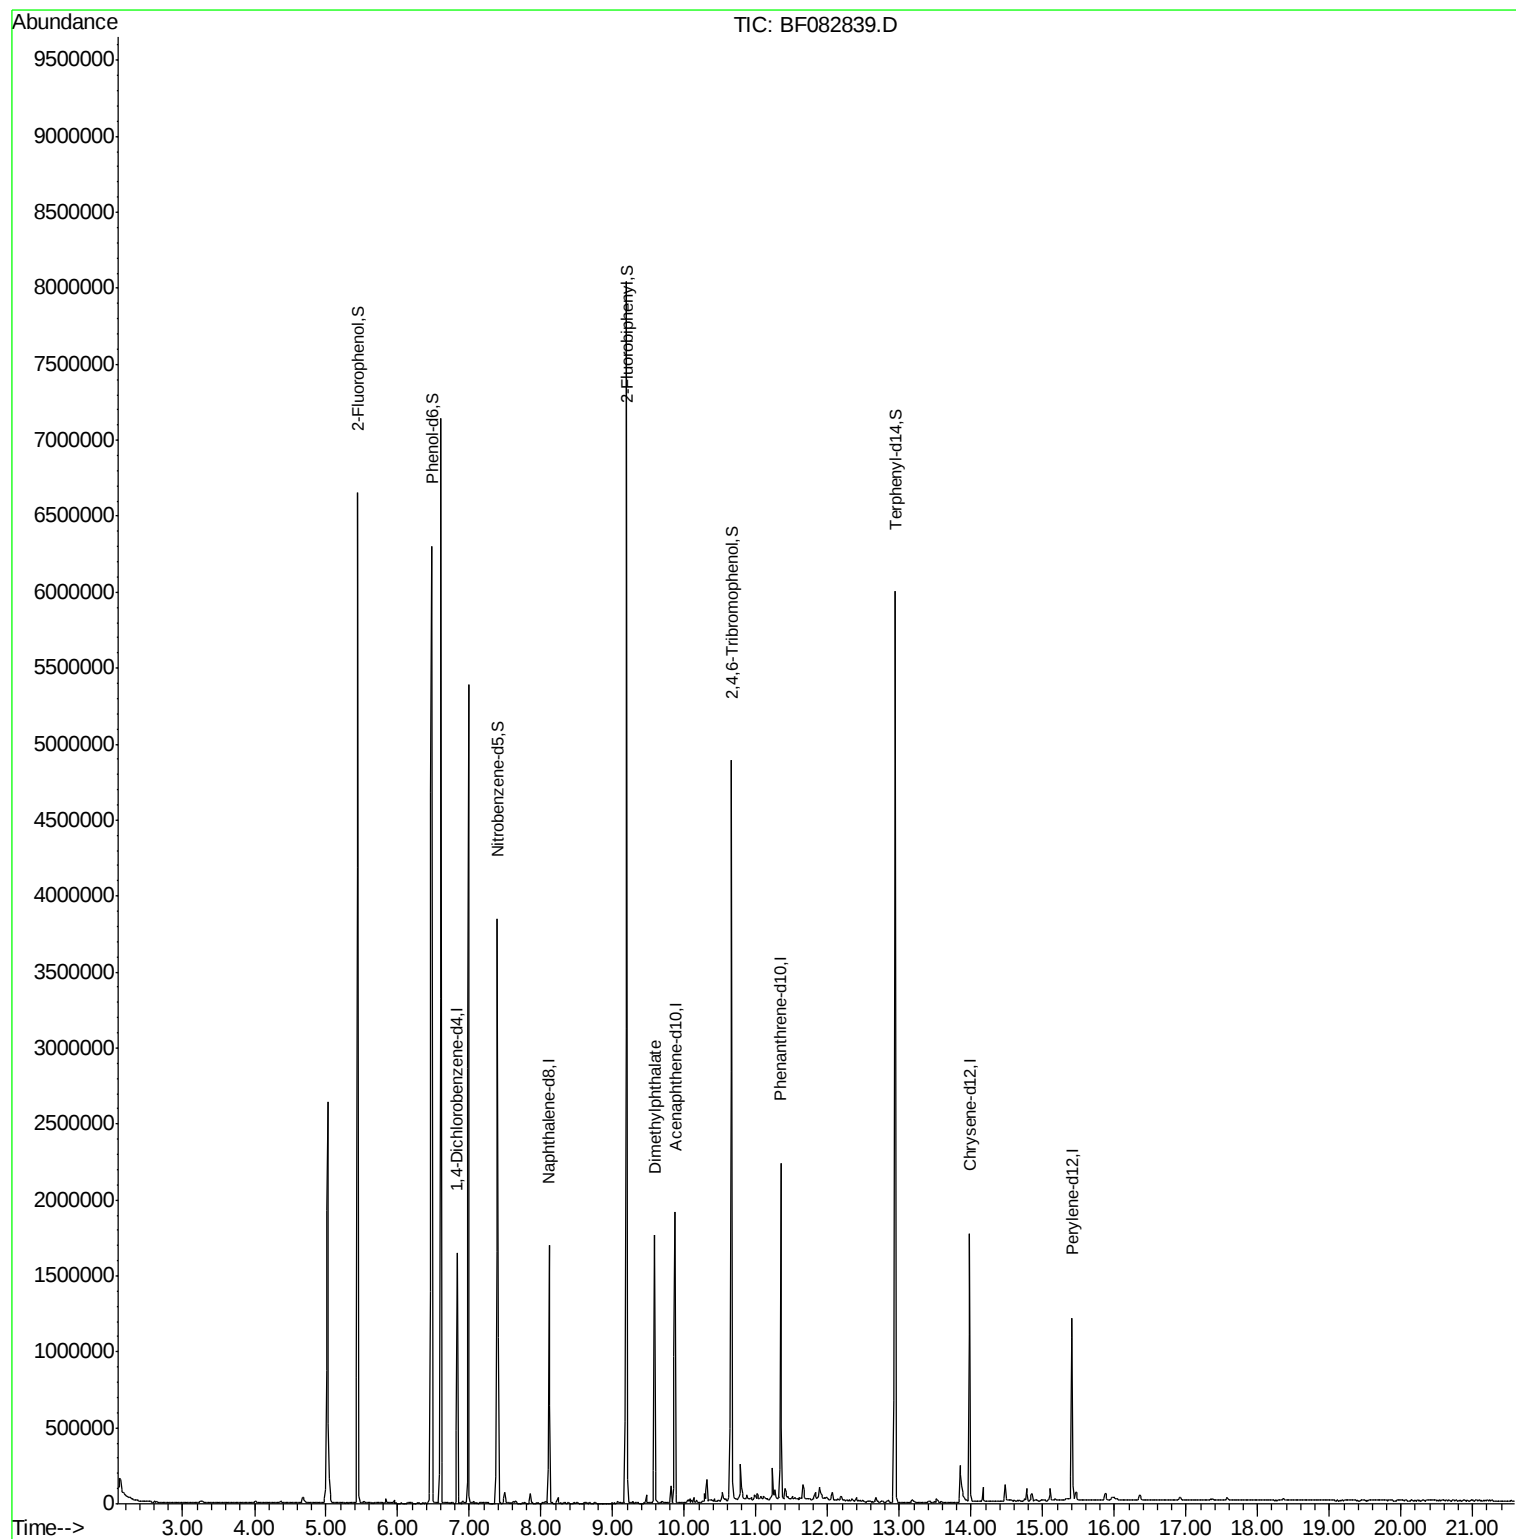

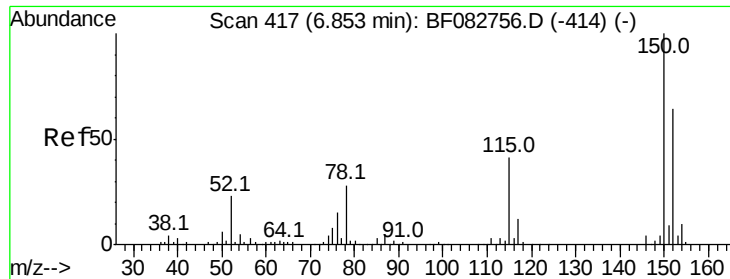

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.83 min Scan# 415

Delta R.T. -0.02 min

Lab File: BF082839.D

Acq: 9 Nov 2015 19:55

Instrument :

BNA_F

ClientSampled :

D2


Tot Ion:152 Resp: 243665

Ion Ratio Lower Upper

152 100

150 152.9 127.0 190.4




115 61.2 47.0 70.6

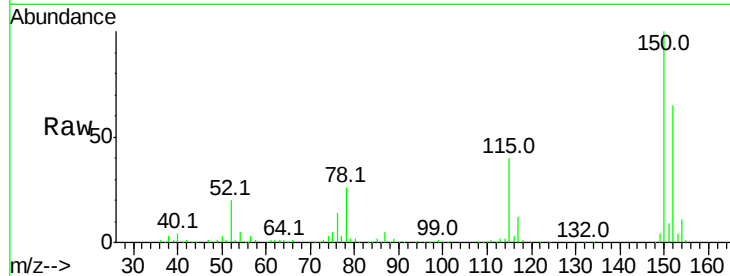

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

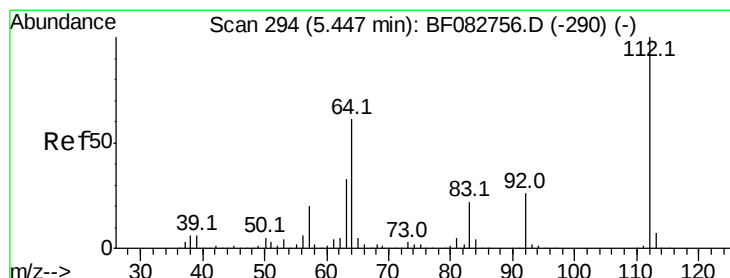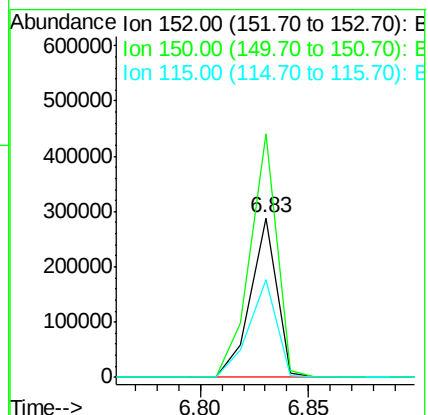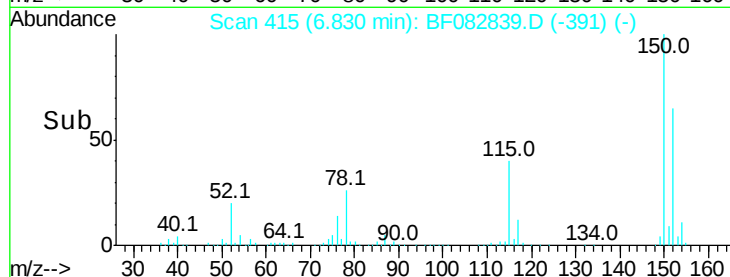

#5

2-Fluorophenol

Concen: 135.94 ng

RT: 5.45 min Scan# 294

Delta R.T. 0.00 min

Lab File: BF082839.D

Acq: 9 Nov 2015 19:55


Tgt Ion:112 Resp: 2128876

Ion Ratio Lower Upper

112 100

64 63.2 48.9 73.3



63 33.4 28.1 42.1

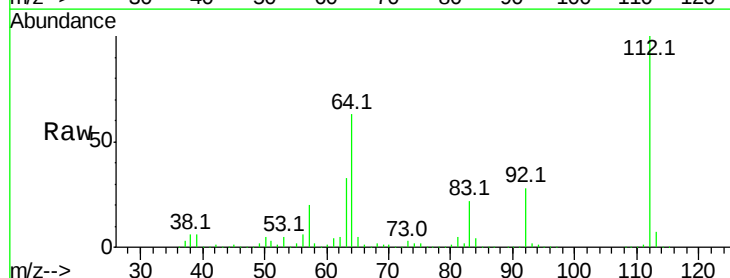


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

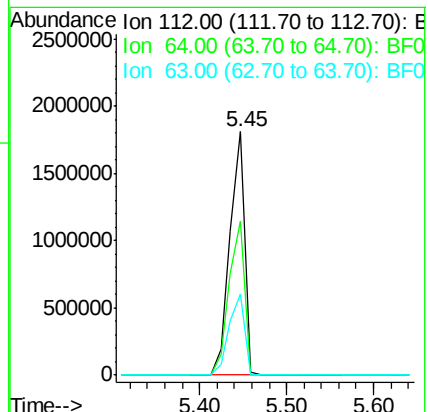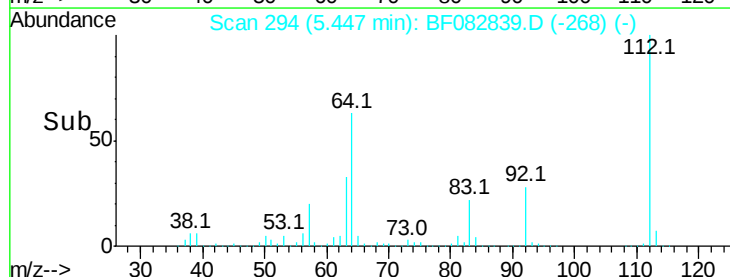



#7

Phenol-d6

Concen: 140.78 ng

RT: 6.48 min Scan# 384

Delta R.T. 0.00 min

Lab File: BF082839.D

Acq: 9 Nov 2015 19:55

Instrument :





BNA_F

ClientSampled :

D2

Tot Ion: 99 Resp: 2931039

Ion	Ratio	Lower	Upper
99	100		
42	18.6	19.2	28.8#
71	37.1	35.0	52.4

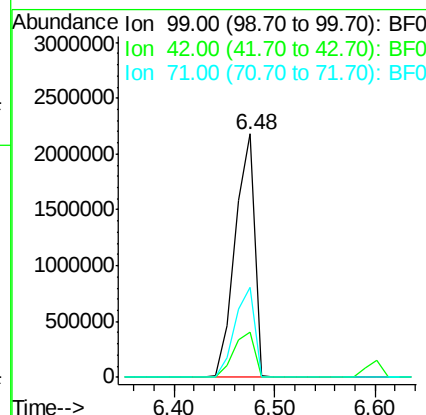

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.11 min Scan# 527




Delta R.T. -0.03 min


Lab File: BF082839.D

Acq: 9 Nov 2015 19:55

Tgt Ion: 136 Resp: 839758

Ion	Ratio	Lower	Upper
136	100		
137	11.0	9.1	13.7
54	10.5	9.1	13.7
68	7.2	4.8	7.2

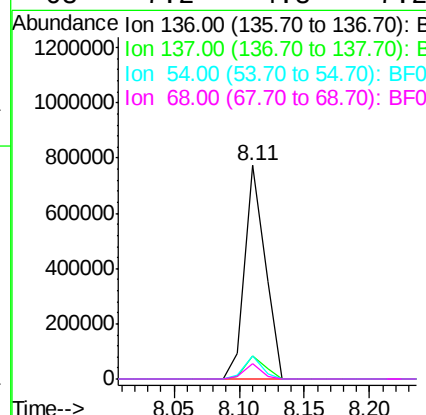







#23
 Nitrobenzene-d5
 Concen: 84.75 ng
 RT: 7.39 min Scan# 464
 Delta R.T. -0.02 min
 Lab File: BF082839.D
 Acq: 9 Nov 2015 19:55

Instrument :
 BNA_F
 ClientSampleId :
 D2

Tot Ion: 82 Resp: 1635635




Ion	Ratio	Lower	Upper
82	100		
128	38.0	26.8	40.2
54	53.3	45.7	68.5

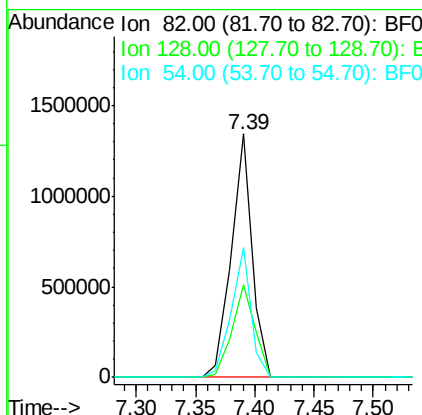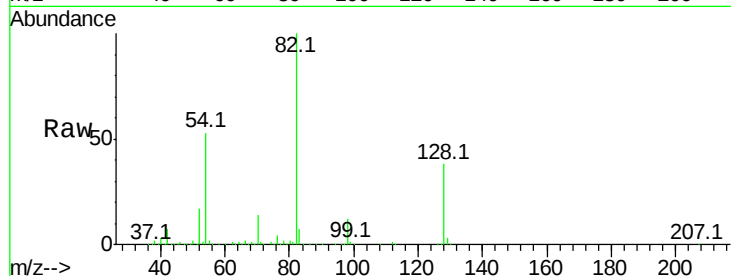


#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.87 min Scan# 681
 Delta R.T. -0.02 min
 Lab File: BF082839.D
 Acq: 9 Nov 2015 19:55

Tgt Ion: 164 Resp: 443601

Ion	Ratio	Lower	Upper
164	100		
162	103.6	84.9	127.3
160	45.3	37.5	56.3

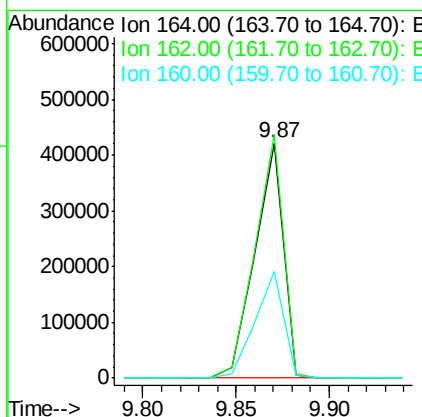







#41
 2,4,6-Tribromophenol
 Concen: 131.18 ng
 RT: 10.66 min Scan# 750
 Delta R.T. -0.02 min
 Lab File: BF082839.D
 Acq: 9 Nov 2015 19:55

Instrument :
 BNA_F
 ClientSampleID :
 D2

Tot Ion:330 Resp: 667205
 Ion Ratio Lower Upper
 330 100
 332 93.7 76.6 114.8
 141 39.8 41.2 61.8#

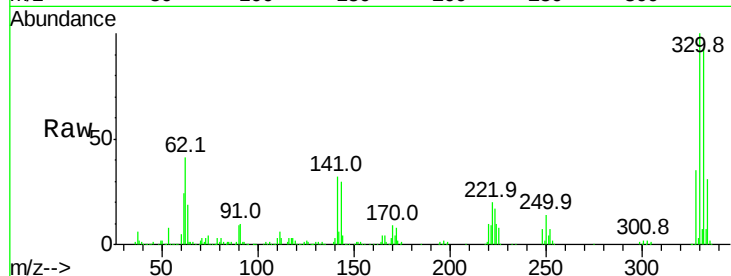


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E


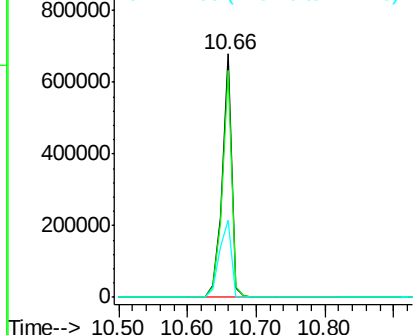



#44
 2-Fluorobiphenyl
 Concen: 81.50 ng
 RT: 9.20 min Scan# 622
 Delta R.T. -0.02 min
 Lab File: BF082839.D
 Acq: 9 Nov 2015 19:55

Tgt Ion:172 Resp: 2522498
 Ion Ratio Lower Upper
 172 100
 171 38.9 30.8 46.2
 170 27.0 21.2 31.8



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

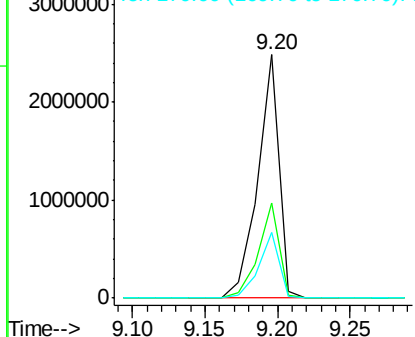

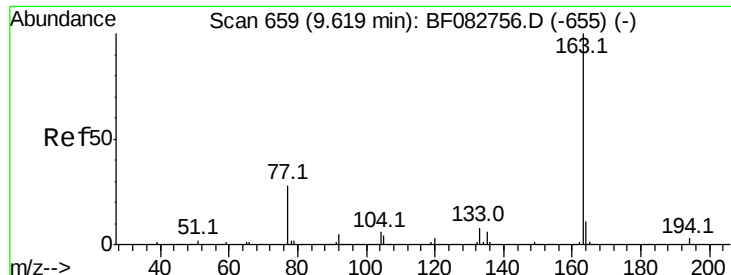

#49

Dimethylphthalate

Concen: 17.64 ng

RT: 9.58 min Scan# 656

Delta R.T. -0.03 min

Lab File: BF082839.D

Acq: 9 Nov 2015 19:55

Instrument :

BNA_F

ClientSampleId :

D2


Tot Ion:163 Resp: 641100

Ion Ratio Lower Upper

163 100

194 3.3 2.6 4.0




164 10.8 8.7 13.1



Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

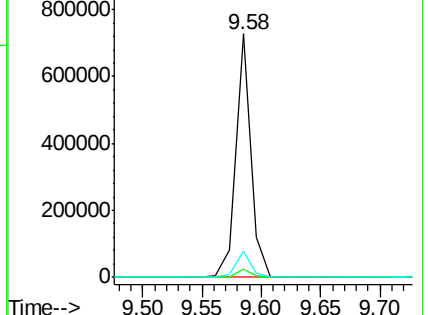

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.34 min Scan# 810

Delta R.T. -0.03 min

Lab File: BF082839.D

Acq: 9 Nov 2015 19:55


Tgt Ion:188 Resp: 782736

Ion Ratio Lower Upper

188 100

94 11.5 6.1 9.1#



80 12.7 7.0 10.6#




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

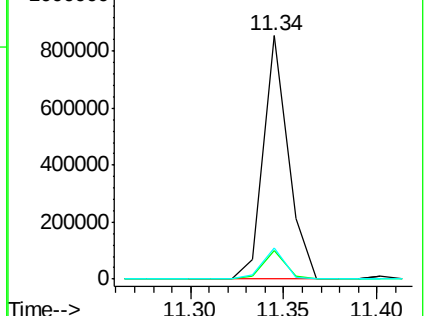



#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.99 min Scan# 1041

Delta R.T. -0.03 min

Lab File: BF082839.D

Acq: 9 Nov 2015 19:55

Instrument :

BNA_F

ClientSampleId :

D2


Tot Ion:240 Resp: 765789

Ion Ratio Lower Upper

240 100

120 7.4 10.9 16.3#




236 26.3 21.6 32.4



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

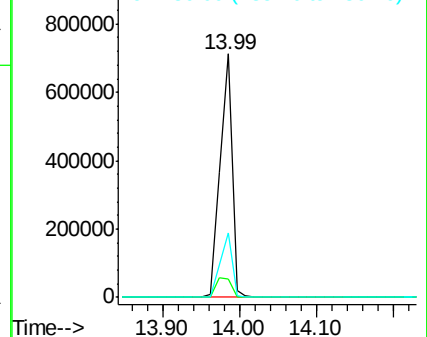

#78

Terphenyl-d14

Concen: 80.85 ng

RT: 12.94 min Scan# 950

Delta R.T. -0.02 min

Lab File: BF082839.D

Acq: 9 Nov 2015 19:55


Tgt Ion:244 Resp: 2610309

Ion Ratio Lower Upper

244 100

212 7.7 7.6 11.4



122 6.9 11.3 16.9#




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

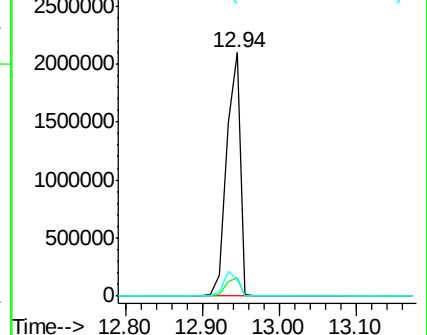

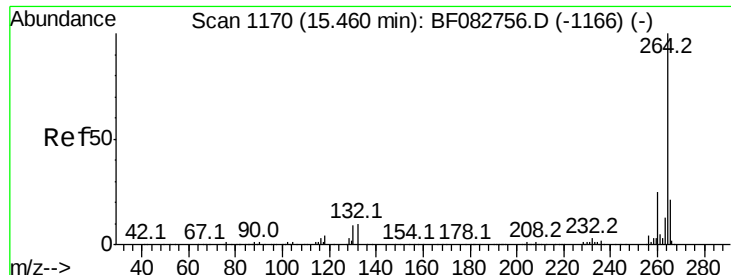

#86
Pervlene-d12
Concen: 20.00 ng
RT: 15.41 min Scan# 1166
Delta R.T. -0.05 min
Lab File: BF082839.D
Acq: 9 Nov 2015 19:55

Instrument :
BNA_F
ClientSampleId :
D2

Tot Ion: 264 Resp: 672762

Ion	Ratio	Lower	Upper
264	100		
260	24.1	19.8	29.6
265	21.8	17.4	26.0

