


Data Path : Z:\HPCHEM1\BNA F\Data\BF110915\
Data File : BF082830.D
Acq On : 9 Nov 2015 11:36 am
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110715.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Nov 07 02:32:49 2015

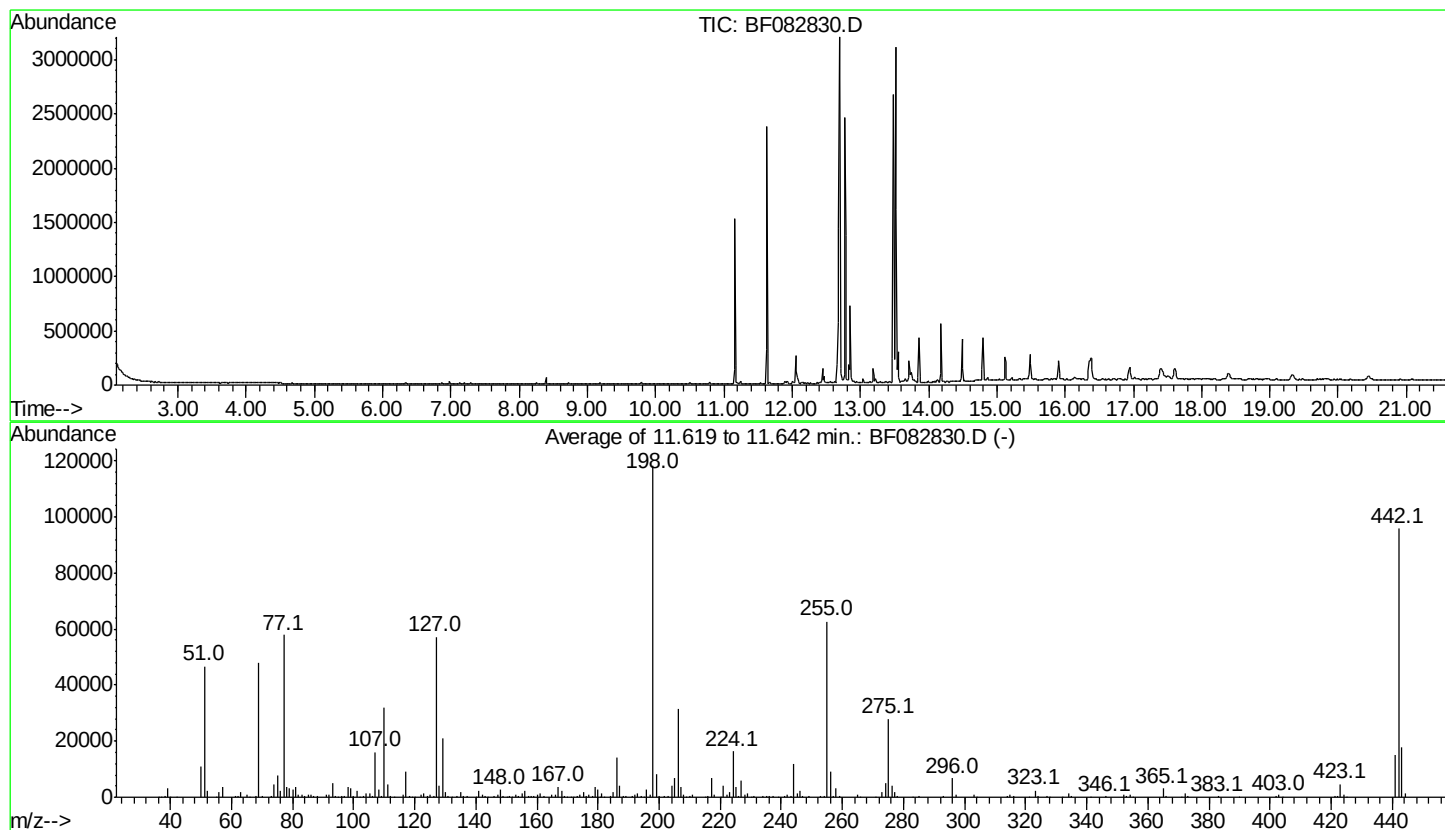

Spectrum Information: Average of 11.619 to 11.642 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.5	46763	PASS
68	69	0.00	2	0.8	388	PASS
69	198	0.00	100	40.4	47850	PASS
70	69	0.00	2	0.5	251	PASS
127	198	10	80	48.4	57250	PASS
197	198	0.00	2	0.7	812	PASS
198	198	100	100	100.0	118296	PASS
199	198	5	9	6.9	8157	PASS
275	198	10	60	23.6	27876	PASS
365	198	1	100	2.7	3177	PASS
441	442	0.01	24	15.9	15234	PASS
442	198	50	100	80.9	95752	PASS
443	442	15	24	18.8	18037	PASS