


Data Path : Z:\HPCHEM1\BNA F\DATA\BF110915\
 Data File : BF082847.D
 Acq On : 10 Nov 2015 1:45
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Nov 07 02:32:49 2015

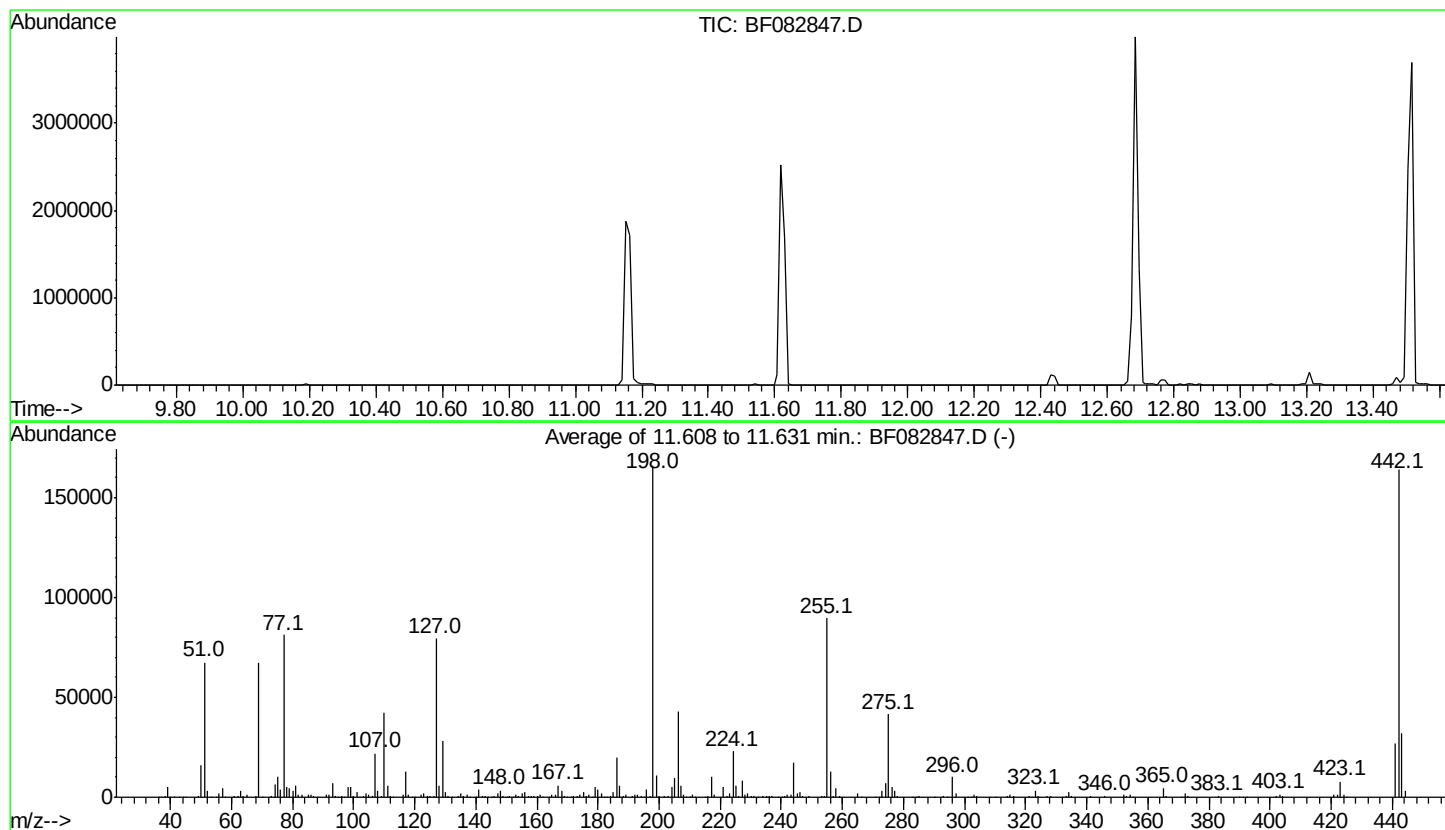

AutoFind: Scans 833, 834, 835; Background Corrected with Scan 830

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.7	67499	PASS
68	69	0.00	2	1.5	982	PASS
69	198	0.00	100	40.7	67604	PASS
70	69	0.00	2	0.5	331	PASS
127	198	10	80	47.8	79255	PASS
197	198	0.00	2	0.5	870	PASS
198	198	100	100	100.0	165959	PASS
199	198	5	9	6.6	11031	PASS
275	198	10	60	24.9	41364	PASS
365	198	1	100	2.8	4595	PASS
441	442	0.01	24	16.5	26957	PASS
442	198	50	100	98.7	163848	PASS
443	442	15	24	19.4	31754	PASS