
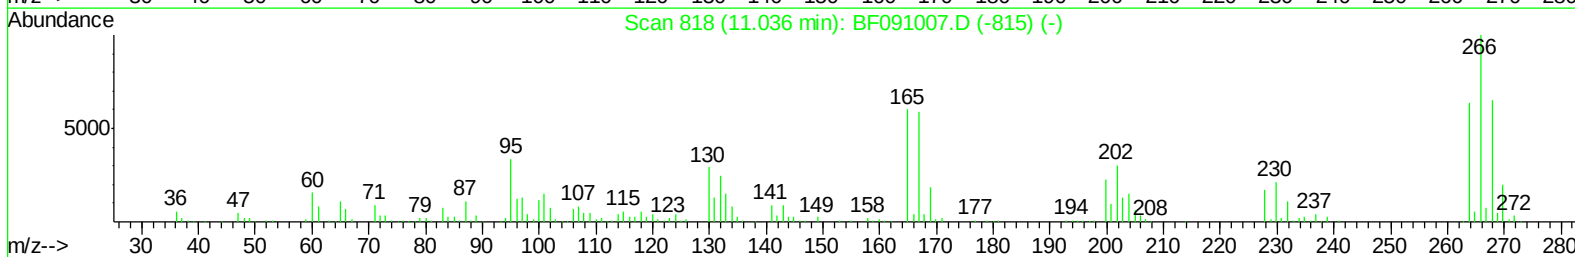
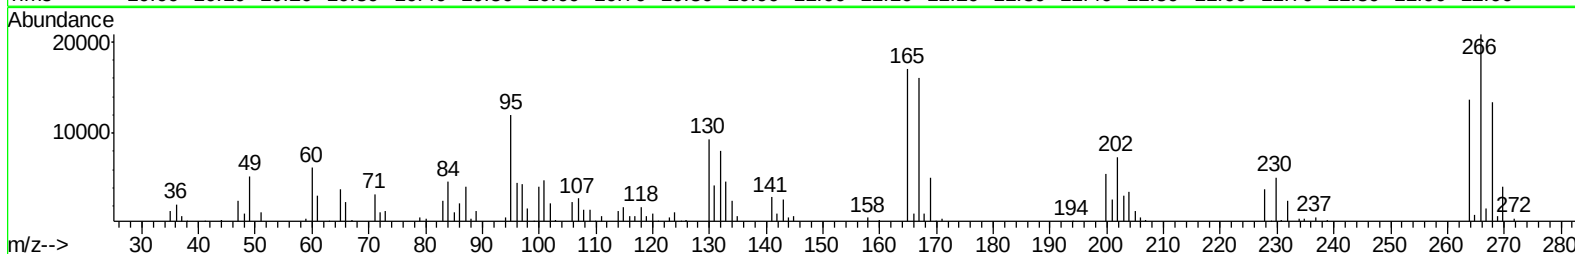


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF110916\
Data File : BF091122.D
Acq On : 9 Nov 2016 13:30
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 10 04:54:14 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 08 12:59:29 2016
Response via : Initial Calibration

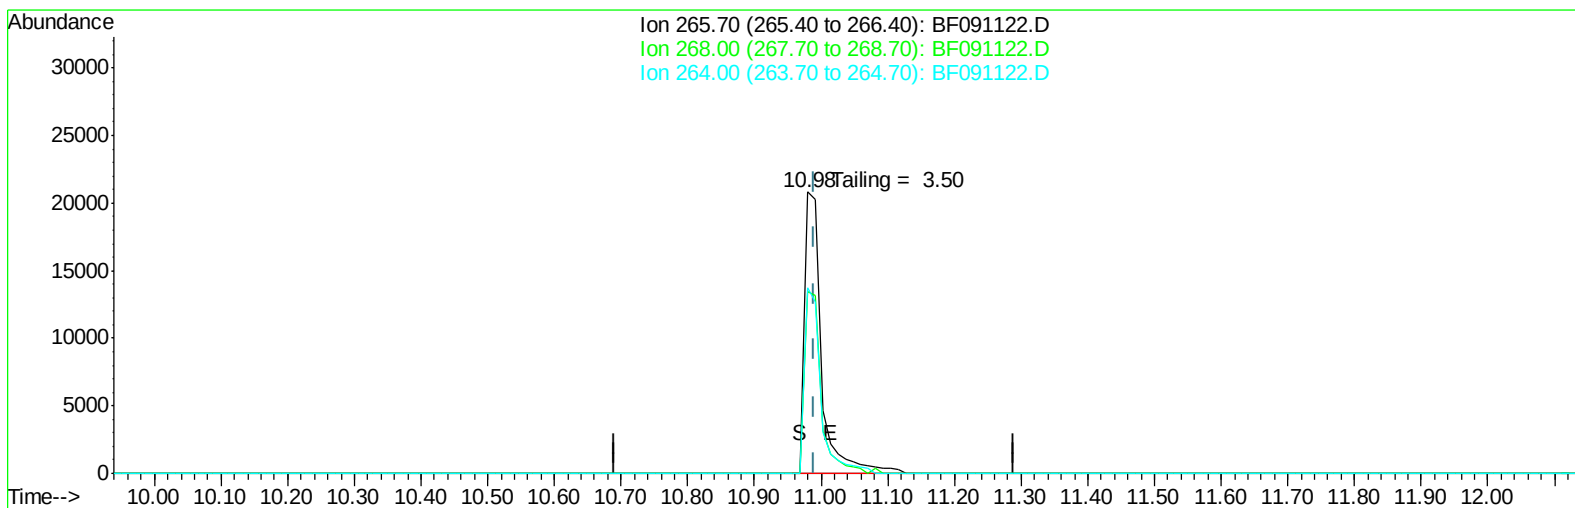

TIC: BF091122.D

(69) Pentachlorophenol (C)




10.979min (-0.011) 24593.29ng

response 37238

Ion	Exp%	Act%
265.70	100	100
268.00	65.10	64.44
264.00	63.90	65.78
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF110916\
Data File : BF091122.D
Acq On : 9 Nov 2016 13:30
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 10 04:54:14 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 08 12:59:29 2016
Response via : Initial Calibration

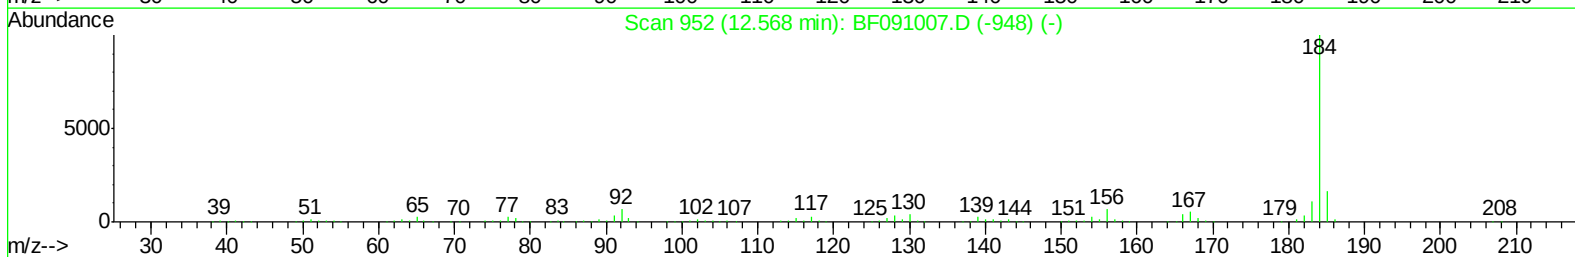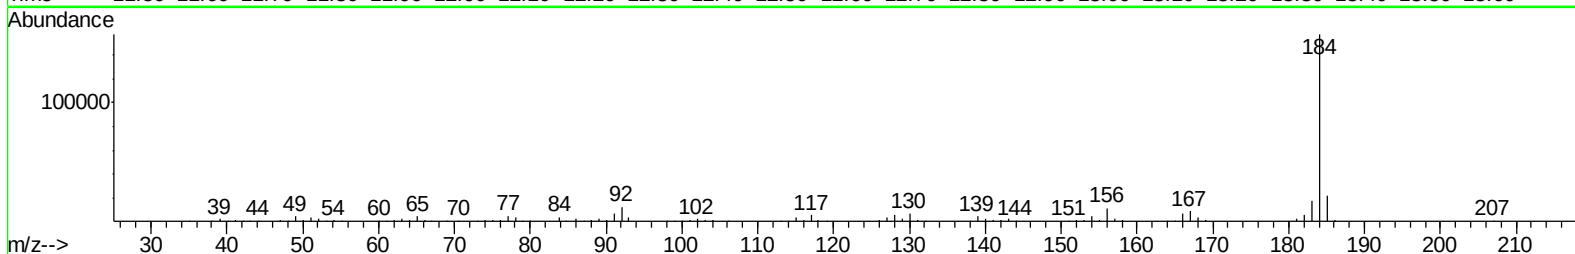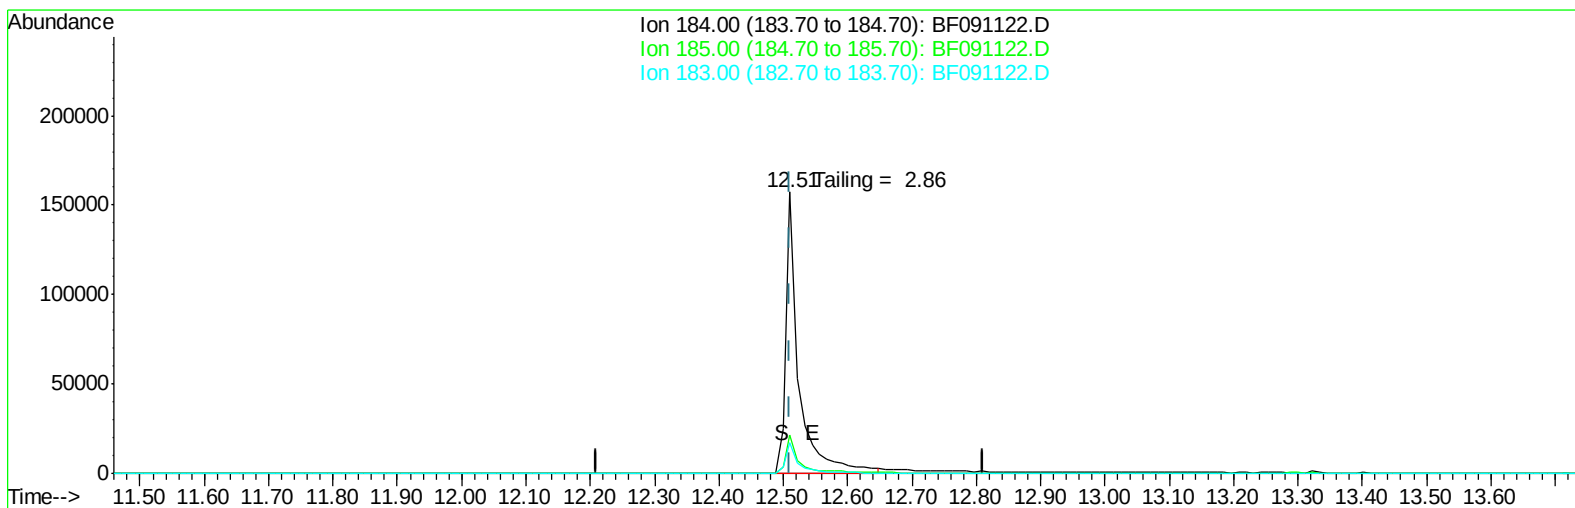

TIC: BF091122.D

(76) Benzidine

12.511min (+0.000) 31212.20ng m

response 224530

Ion	Exp%	Act%
184.00	100	100
185.00	16.20	13.81
183.00	10.90	10.90
0.00	0.00	0.00