

Data Path : Z:\HPCHEM1\BNA F\DATA\BF110916\
 Data File : BF091131.D
 Acq On : 9 Nov 2016 18:29
 Operator : UM/SJ
 Sample : H5586-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 HSR-WC-73-110716

Quant Time: Nov 09 23:04:32 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110316.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 08 12:59:29 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.66	152	166455	20.00	ng	0.00
21) Naphthalene-d8	7.94	136	734710	20.00	ng	-0.01
38) Acenaphthene-d10	9.69	164	379804	20.00	ng	-0.01
63) Phenanthrene-d10	11.16	188	640062	20.00	ng	-0.01
75) Chrysene-d12	13.80	240	449620	20.00	ng	-0.01
86) Perylene-d12	15.17	264	304467	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.26	112	1392215	138.13	ng	0.02
7) Phenol-d6	6.32	99	1796323	131.31	ng	0.00
23) Nitrobenzene-d5	7.23	82	1294193	96.09	ng	-0.01
41) 2,4,6-Tribromophenol	10.49	330	498486	145.18	ng	0.00
44) 2-Fluorobiphenyl	9.02	172	2064983	93.60	ng	-0.01
78) Terphenyl-d14	12.76	244	2209827	122.65	ng	0.00
Target Compounds						
31) Naphthalene	7.96	128	205116	5.84	ng	Qvalue 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF110916\
Data File : BF091131.D
Acq On : 9 Nov 2016 18:29
Operator : UM/SJ
Sample : H5586-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
HSR-WC-73-110716

Quant Time: Nov 09 23:04:32 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 08 12:59:29 2016
Response via : Initial Calibration

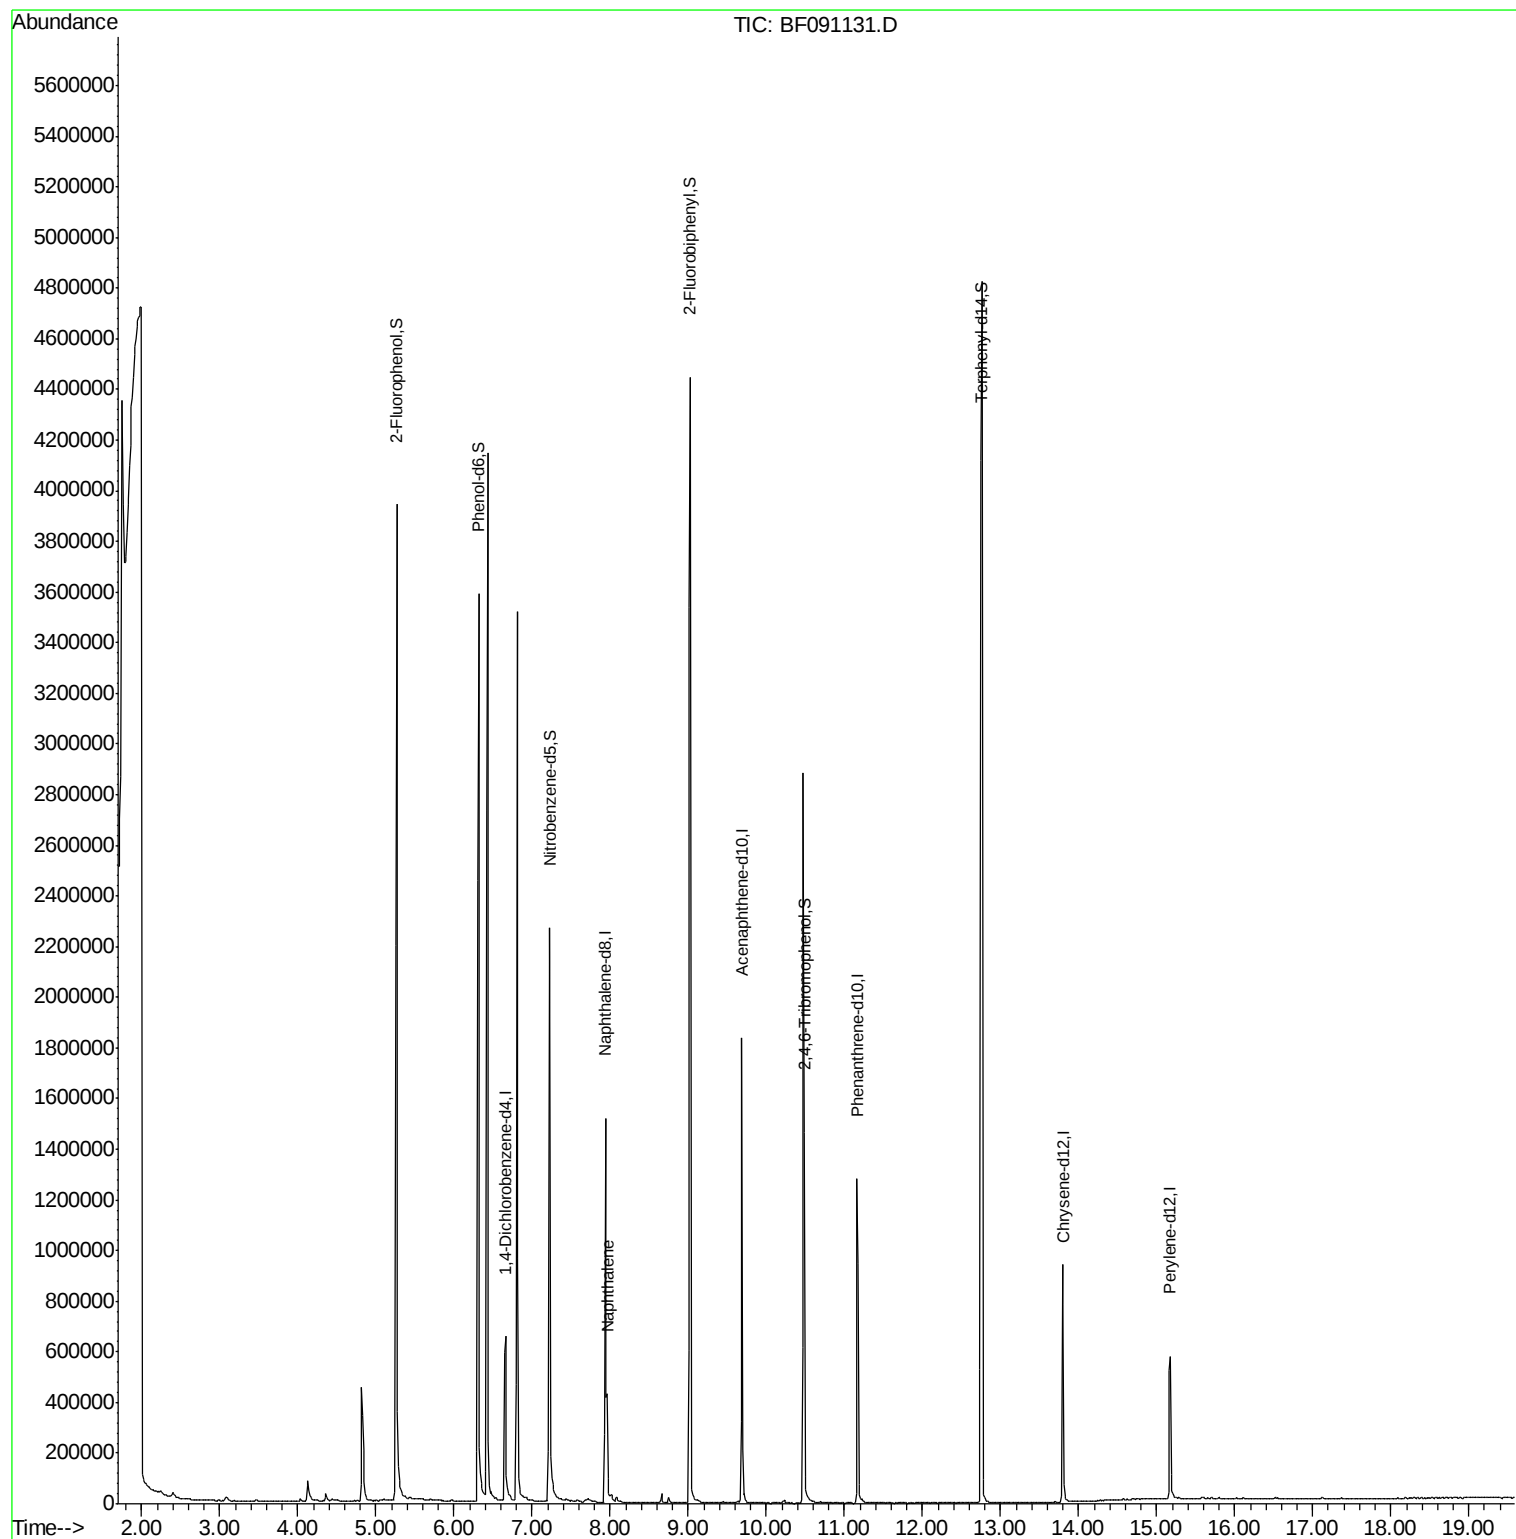



#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.66 min Scan# 435

Delta R.T. 0.00 min

Lab File: BF091131.D

Acq: 9 Nov 2016 18:29

Instrument :

BNA_F

ClientSampleId :

HSR-WC-73-110716


Tot Ion:152 Resp: 166455

Ion Ratio Lower Upper

152 100

150 151.4 126.8 190.2




115 55.3 53.3 79.9

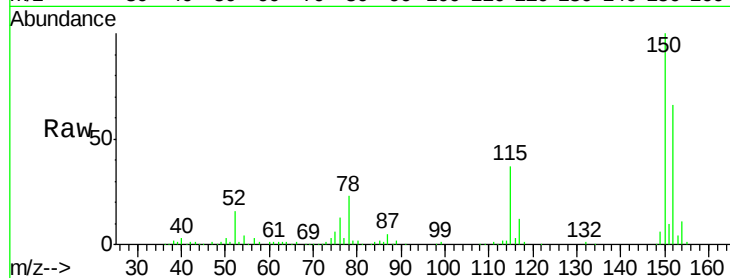

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

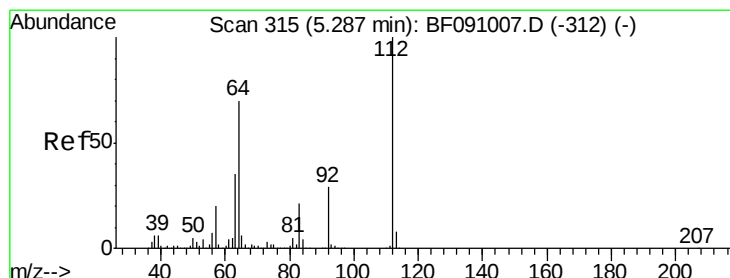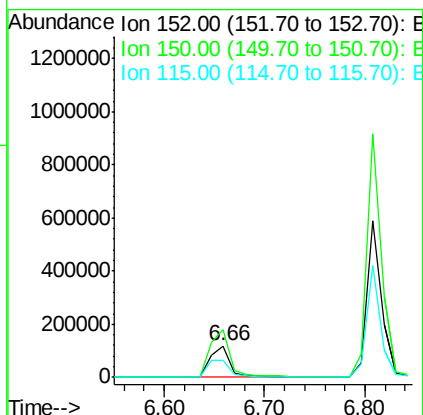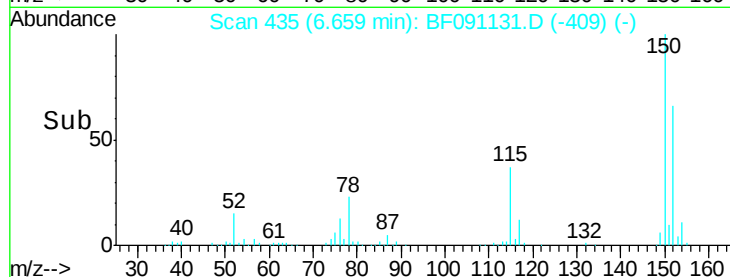

#5

2-Fluorophenol

Concen: 138.13 ng

RT: 5.26 min Scan# 313

Delta R.T. 0.02 min

Lab File: BF091131.D

Acq: 9 Nov 2016 18:29


Tgt Ion:112 Resp: 1392215

Ion Ratio Lower Upper

112 100

64 57.7 55.8 83.6



63 29.0 28.0 42.0

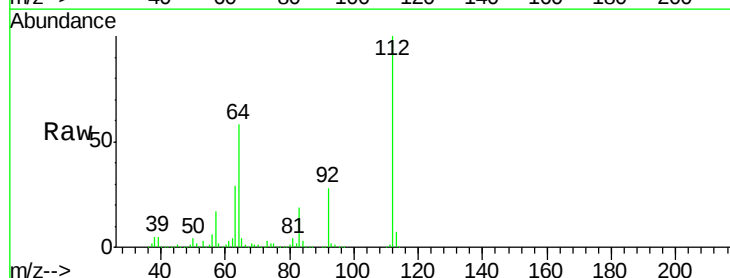

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

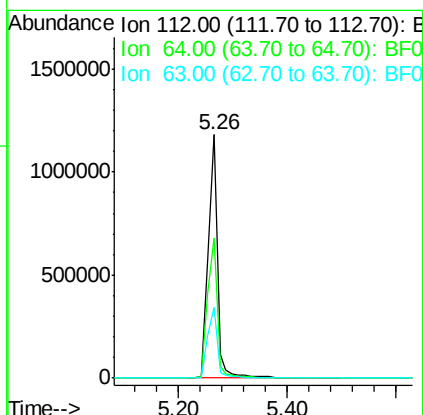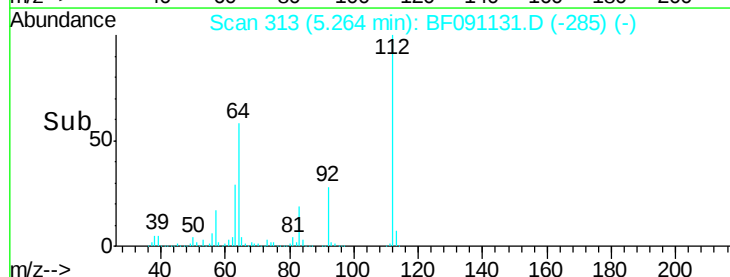



#7

Phenol-d6

Concen: 131.31 ng

RT: 6.32 min Scan# 405

Delta R.T. 0.00 min

Lab File: BF091131.D

Acq: 9 Nov 2016 18:29

Instrument :

BNA_F

ClientSampleId :

HSR-WC-73-110716


Tot Ion: 99 Resp: 1796323

Ion Ratio Lower Upper

99 100

42 14.2 13.9 20.9




71 31.6 27.8 41.8

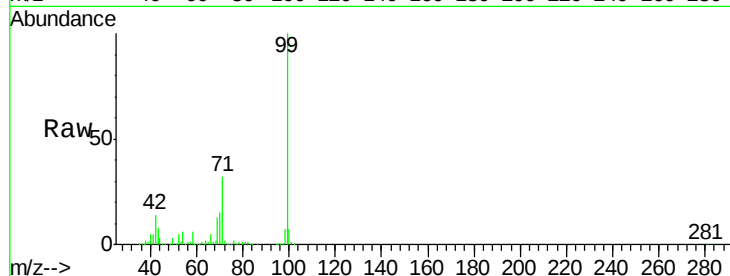

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

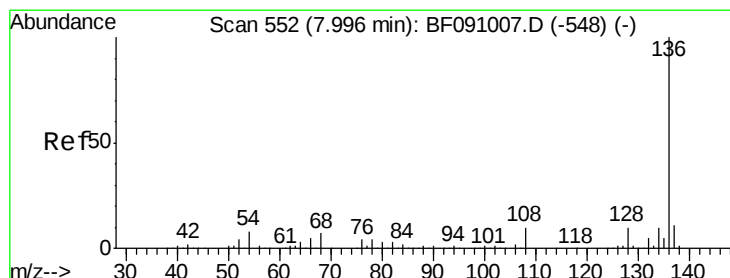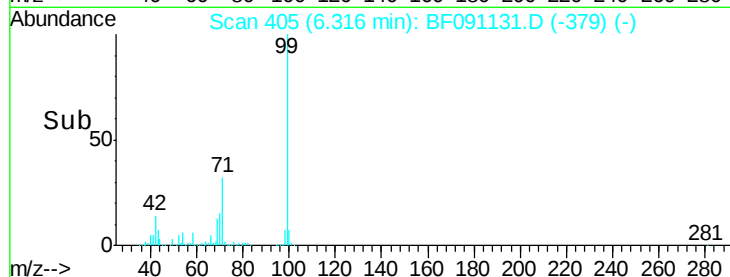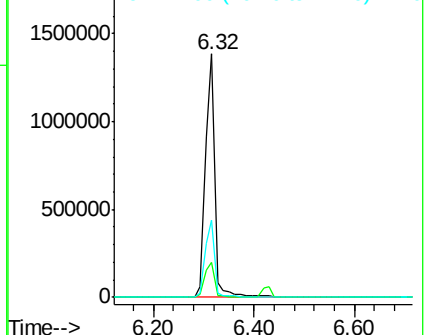

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.94 min Scan# 547

Delta R.T. -0.01 min

Lab File: BF091131.D

Acq: 9 Nov 2016 18:29

Tgt Ion: 136 Resp: 734710


Ion Ratio Lower Upper

136 100

137 11.5 8.9 13.3

54 9.2 6.2 9.2

68 7.9 5.5 8.3


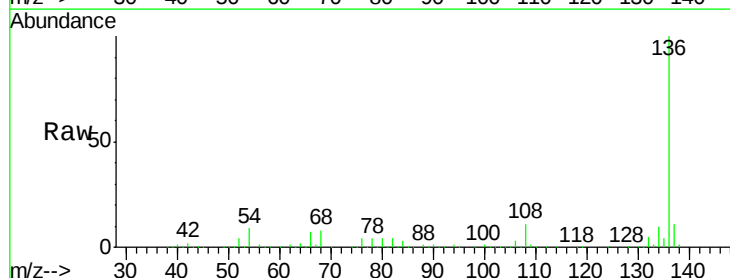



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0



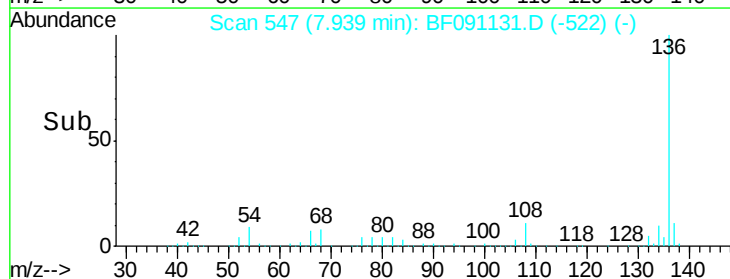
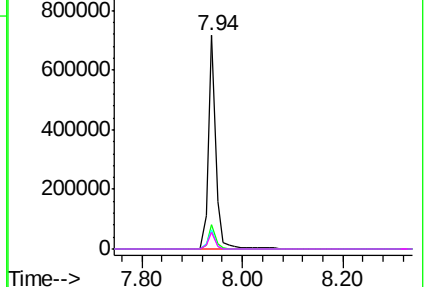


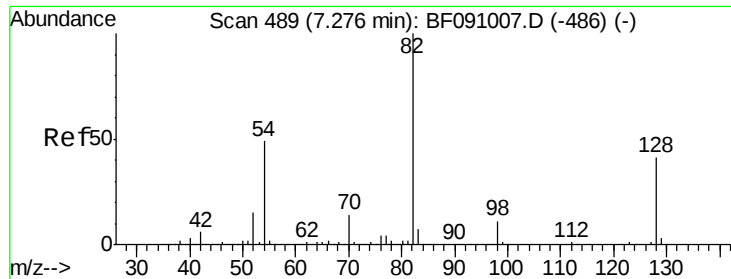

#23
Nitrobenzene-d5
Concen: 96.09 ng
RT: 7.23 min Scan# 485
Delta R.T. -0.01 min
Lab File: BF091131.D
Acq: 9 Nov 2016 18:29




Instrument :
BNA_F
ClientSampleId :
HSR-WC-73-110716


Tot Ion: 82 Resp: 1294193
Ion Ratio Lower Upper
82 100
128 50.6 32.4 48.6#
54 41.6 39.2 58.8

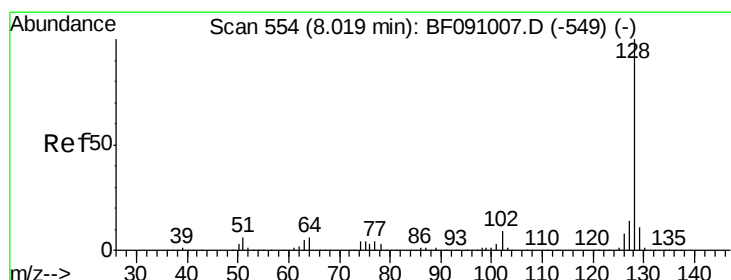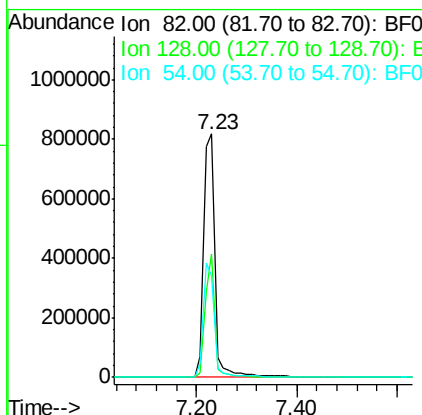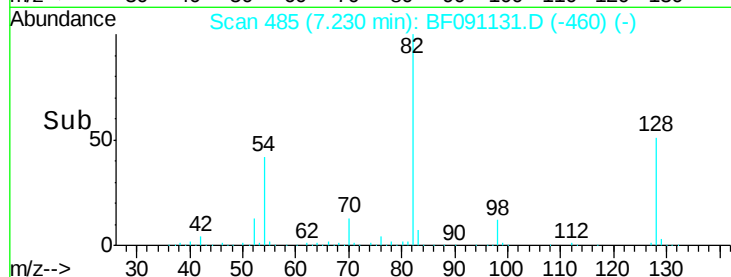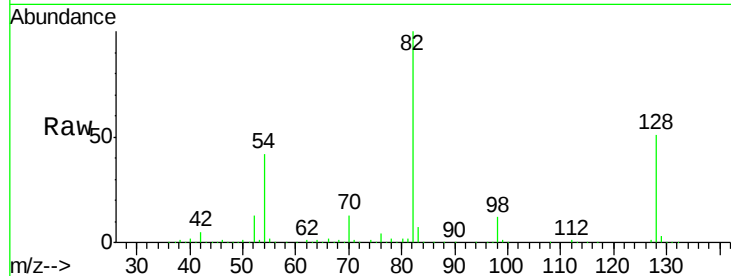

#31
Naphthalene
Concen: 5.84 ng
RT: 7.96 min Scan# 549
Delta R.T. -0.01 min
Lab File: BF091131.D
Acq: 9 Nov 2016 18:29

Tgt Ion:128 Resp: 205116
Ion Ratio Lower Upper
128 100
129 10.9 9.0 13.6
127 12.5 10.9 16.3

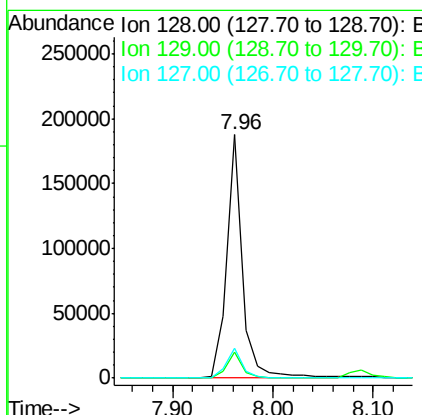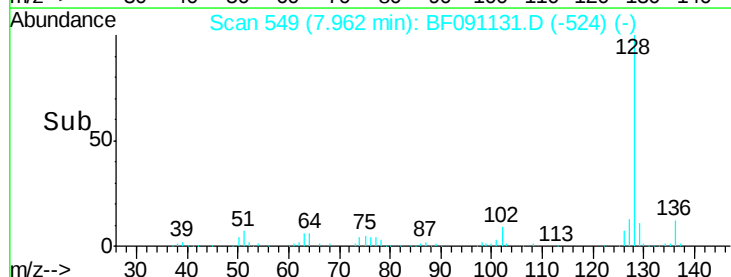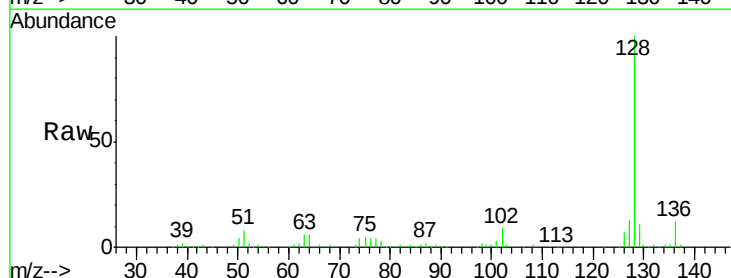

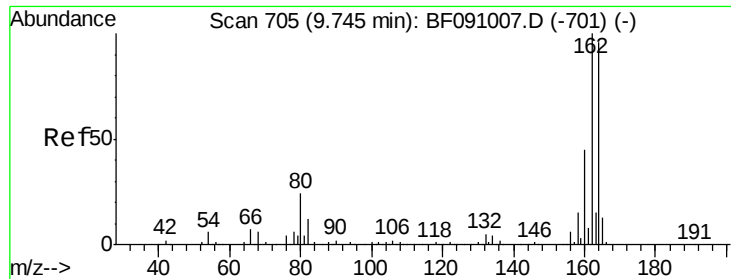

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.69 min Scan# 700

Delta R.T. -0.01 min

Lab File: BF091131.D

Acq: 9 Nov 2016 18:29

Instrument :

BNA_F

ClientSampleId :

HSR-WC-73-110716


Tot Ion:164 Resp: 379804

Ion Ratio Lower Upper

164 100

162 103.4 83.6 125.4




160 47.7 37.9 56.9

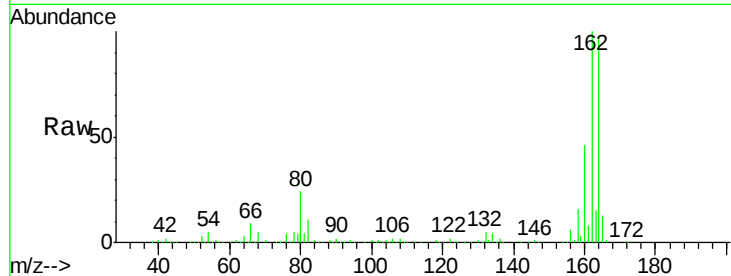

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

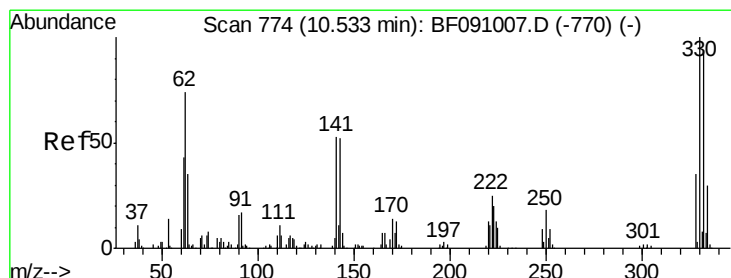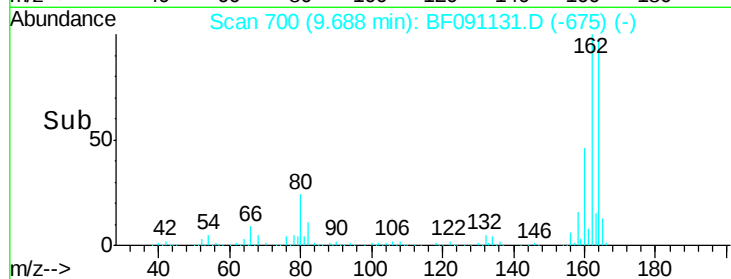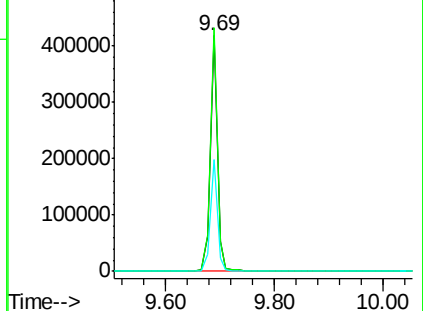

#41

2,4,6-Tribromophenol

Concen: 145.18 ng

RT: 10.49 min Scan# 770

Delta R.T. 0.00 min

Lab File: BF091131.D

Acq: 9 Nov 2016 18:29


Tgt Ion:330 Resp: 498486

Ion Ratio Lower Upper

330 100

332 96.7 75.9 113.9



141 32.0 36.1 54.1#

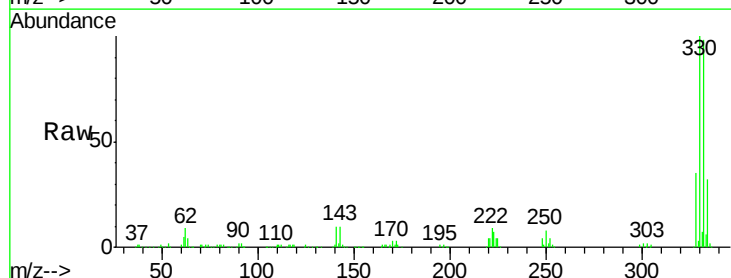


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



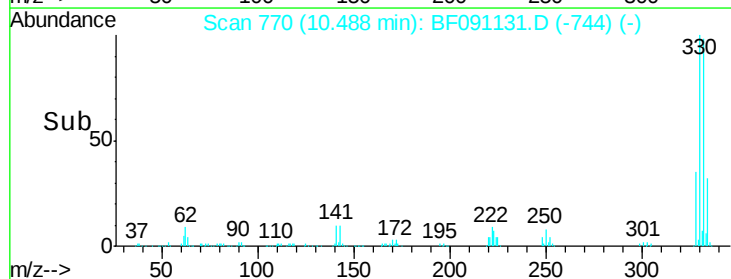
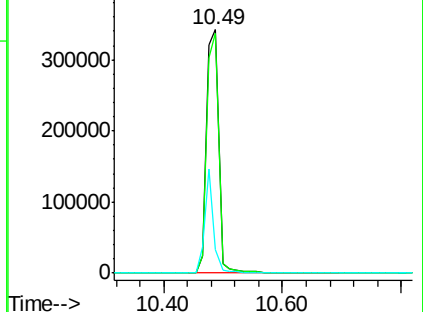


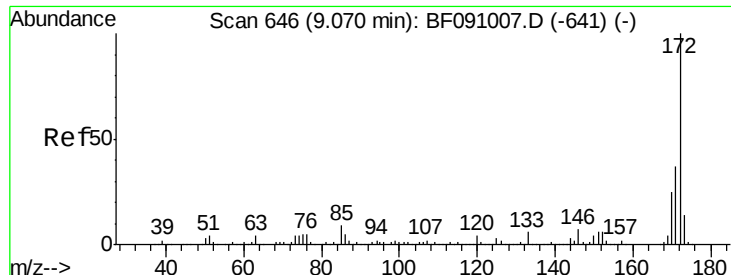

#44
 2-Fluorobiphenyl
 Concen: 93.60 ng
 RT: 9.02 min Scan# 642
 Delta R.T. -0.01 min
 Lab File: BF091131.D
 Acq: 9 Nov 2016 18:29




Instrument :
 BNA_F
 ClientSampleId :
 HSR-WC-73-110716


Tot Ion:172 Resp: 2064983
 Ion Ratio Lower Upper
 172 100
 171 36.7 29.8 44.6
 170 25.3 20.3 30.5

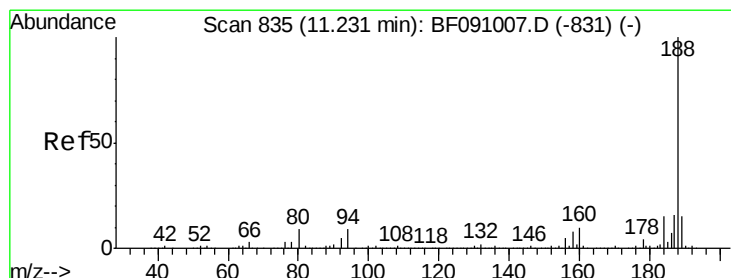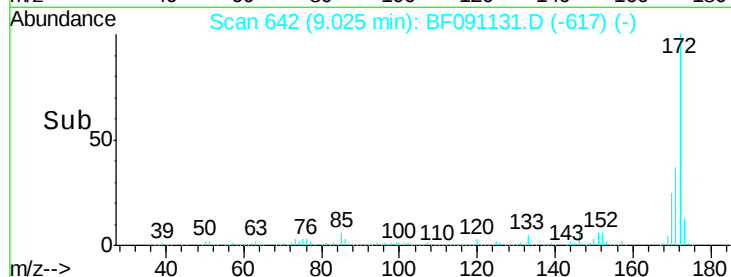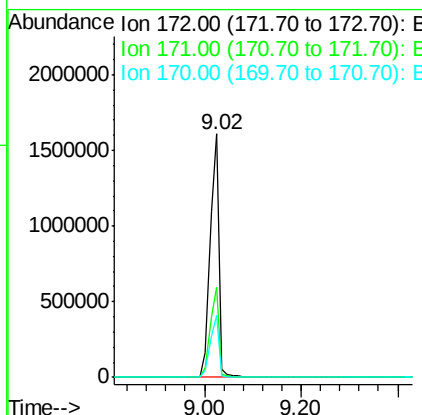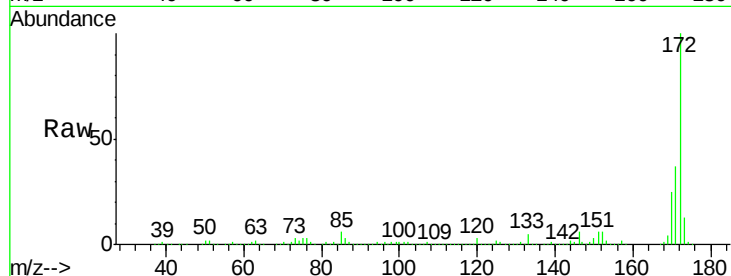

#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 11.16 min Scan# 829
 Delta R.T. -0.01 min
 Lab File: BF091131.D
 Acq: 9 Nov 2016 18:29

Tgt Ion:188 Resp: 640062
 Ion Ratio Lower Upper
 188 100
 94 16.2 7.0 10.4#
 80 18.5 7.5 11.3#

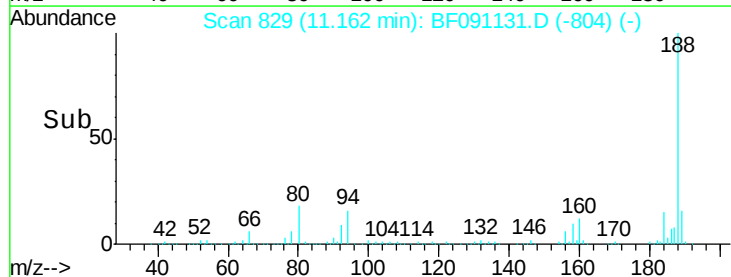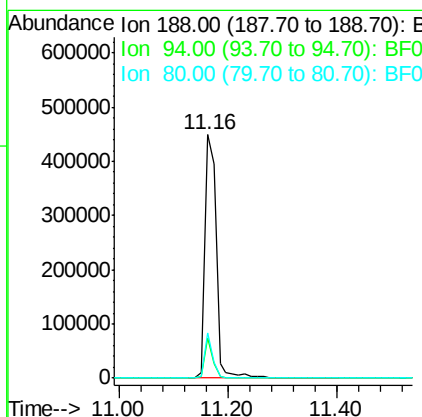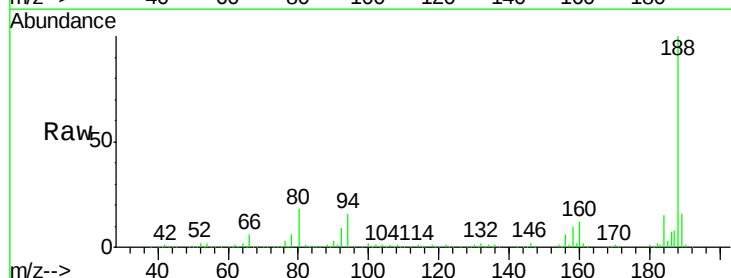

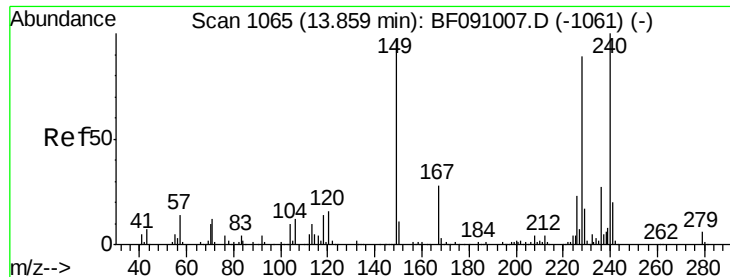

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.80 min Scan# 1060

Delta R.T. -0.01 min

Lab File: BF091131.D

Acq: 9 Nov 2016 18:29

Instrument :

BNA_F

ClientSampleId :

HSR-WC-73-110716


Tot Ion:240 Resp: 449620

Ion Ratio Lower Upper




240 100

120 8.1 12.9 19.3#

236 27.1 21.9 32.9

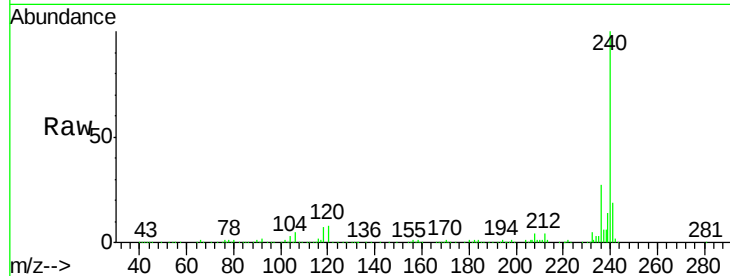

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

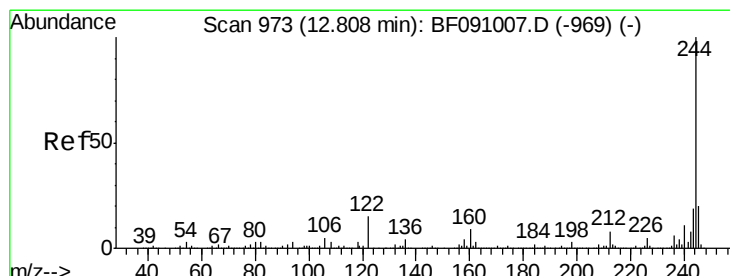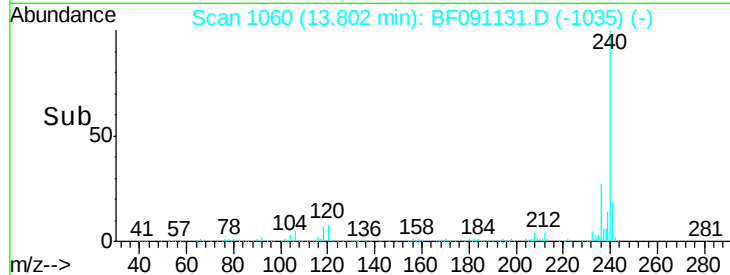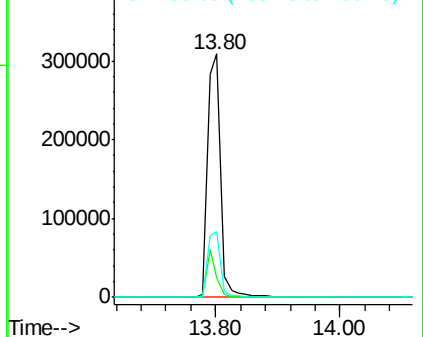

#78

Terphenyl-d14

Concen: 122.65 ng

RT: 12.76 min Scan# 969

Delta R.T. 0.00 min

Lab File: BF091131.D

Acq: 9 Nov 2016 18:29


Tgt Ion:244 Resp: 2209827

Ion Ratio Lower Upper



244 100


212 7.2 6.4 9.6

122 8.3 12.3 18.5#

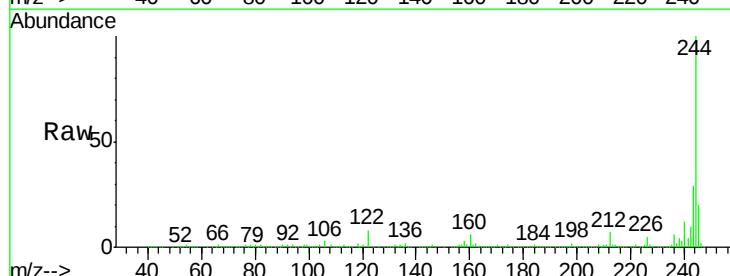

Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

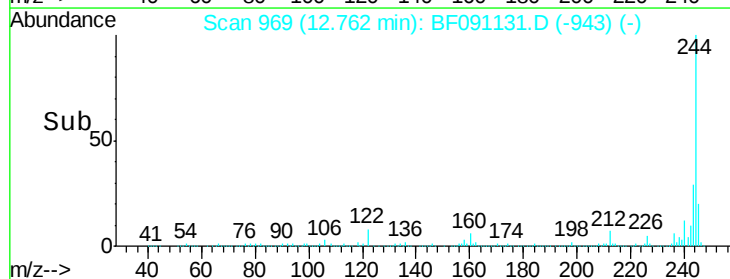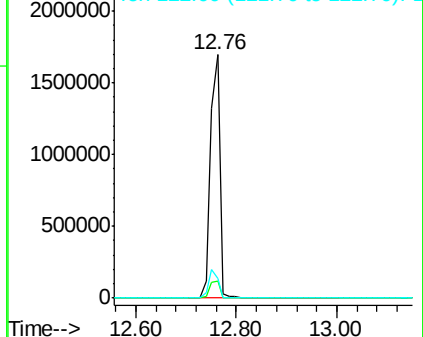


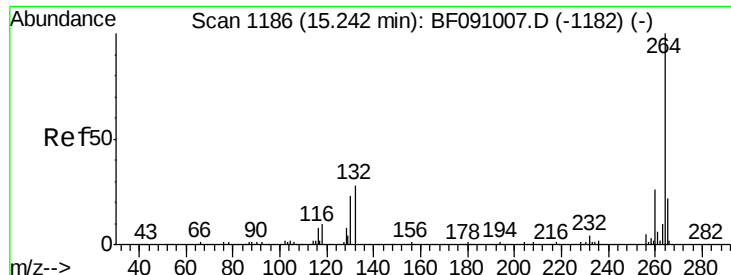

#86
Pervlene-d12
Concen: 20.00 ng
RT: 15.17 min Scan# 1180
Delta R.T. -0.01 min
Lab File: BF091131.D
Acq: 9 Nov 2016 18:29

Instrument :
BNA_F
ClientSampleId :
HSR-WC-73-110716

Tot Ion:264 Resp: 304467
Ion Ratio Lower Upper
264 100
260 24.5 20.6 30.8
265 20.7 17.8 26.8

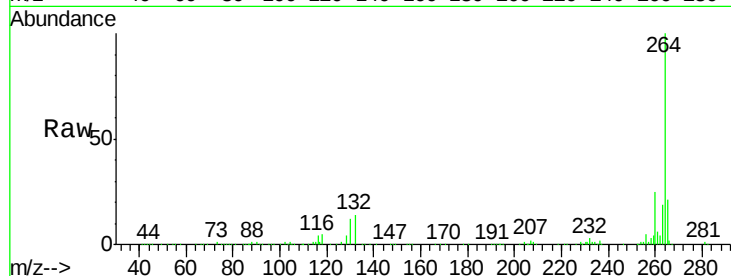

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

