
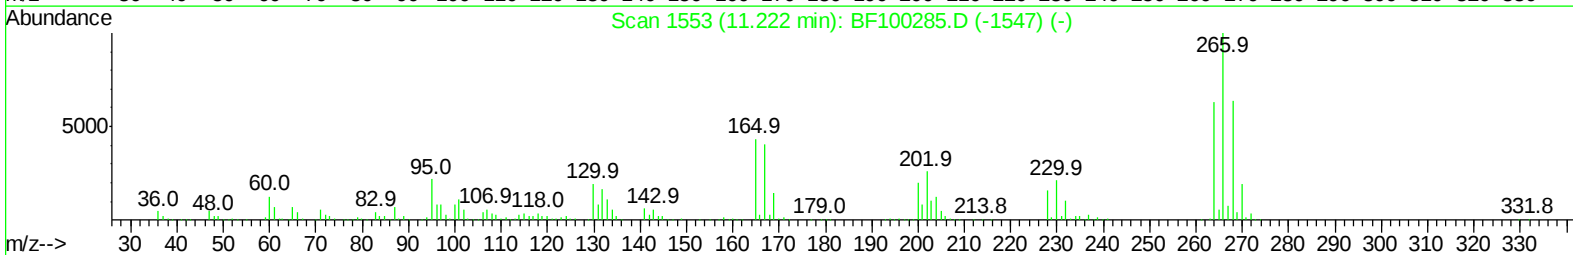
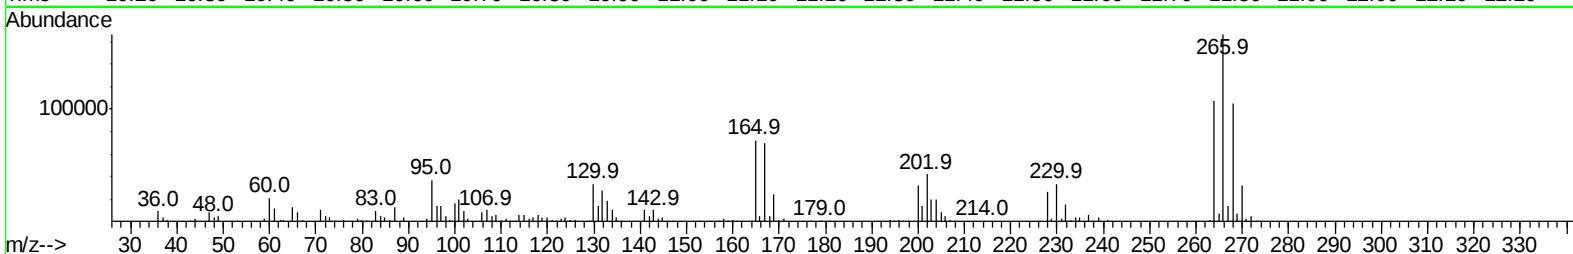


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF110917\
Data File : BF100343.D
Acq On : 9 Nov 2017 16:15
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 10 08:03:36 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 09 16:04:38 2017
Response via : Initial Calibration

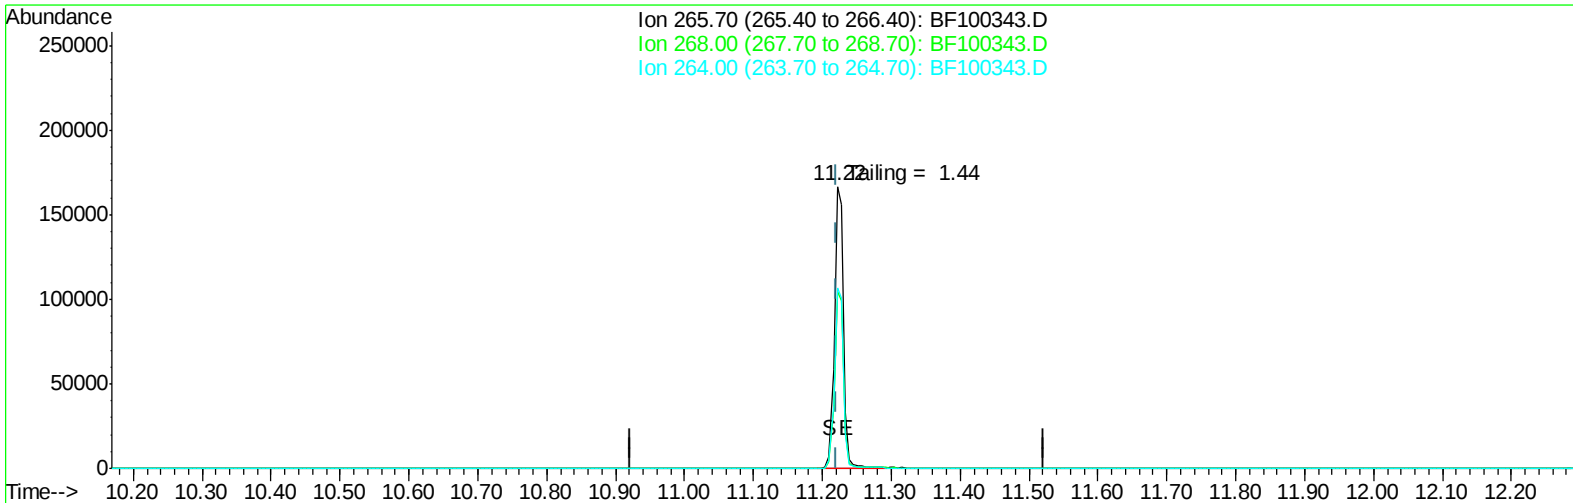

TIC: BF100343.D

(69) Pentachlorophenol (C)




11.222min (+0.000) 164700.39ng

response 153595

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.80
264.00	61.90	64.13
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF110917\
Data File : BF100343.D
Acq On : 9 Nov 2017 16:15
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 10 08:03:36 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 09 16:04:38 2017
Response via : Initial Calibration

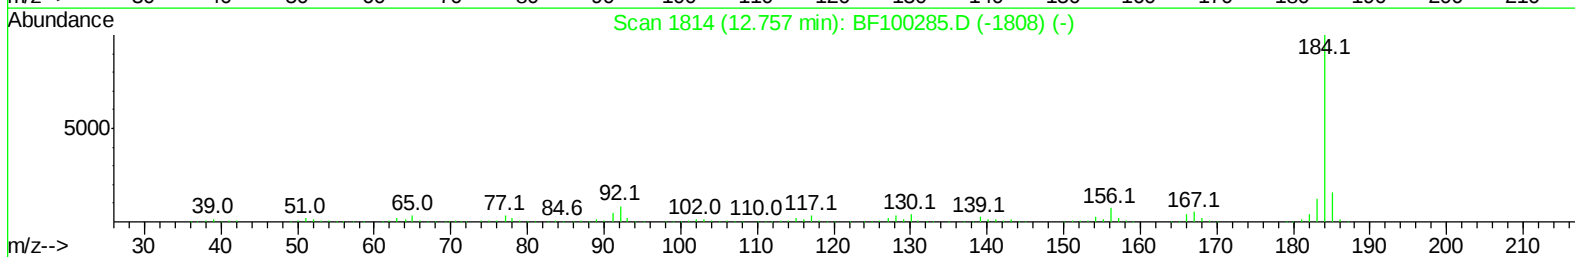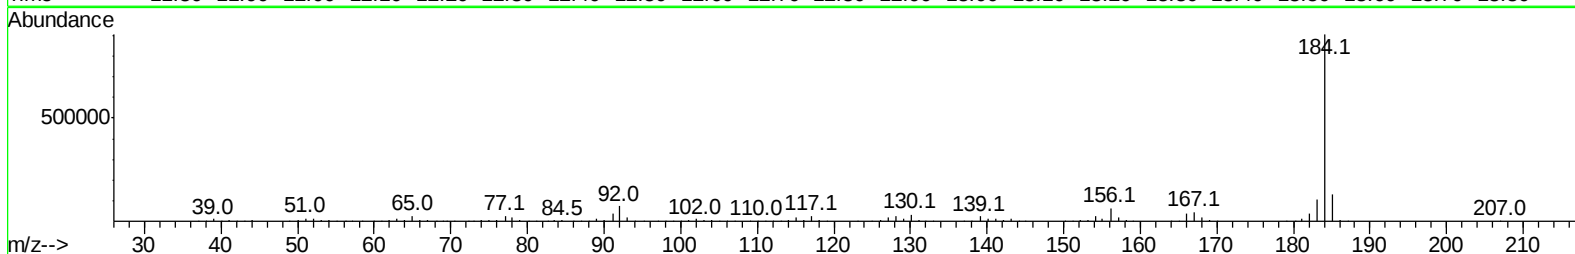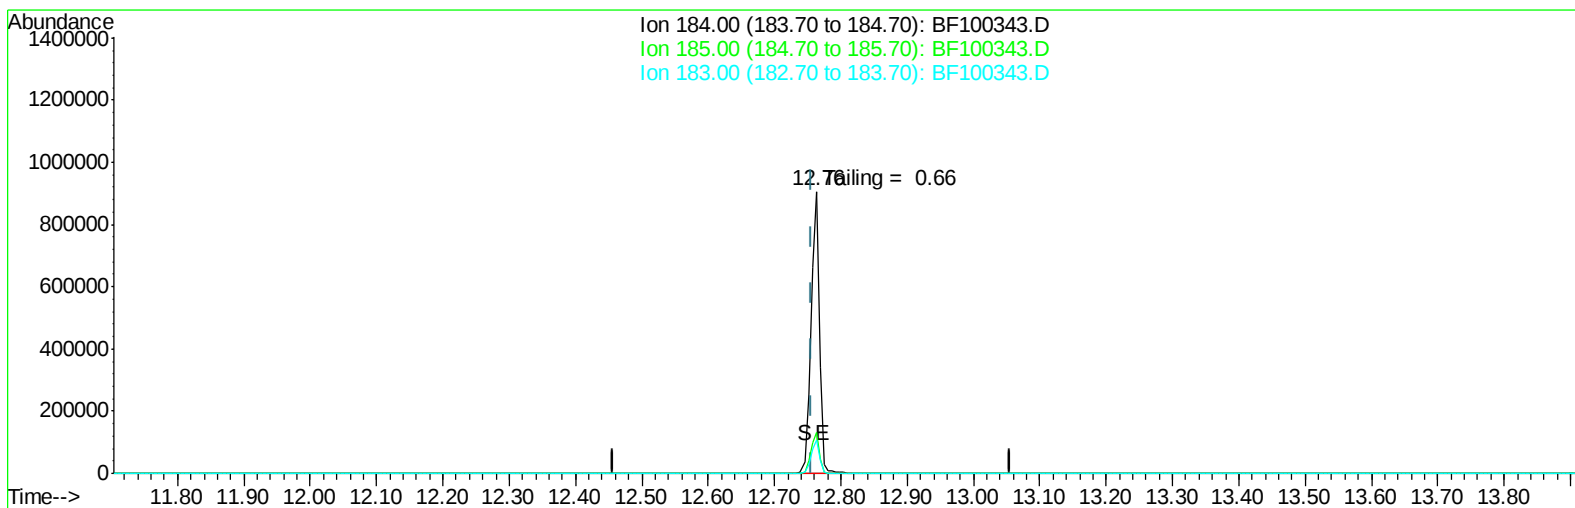

TIC: BF100343.D

(76) Benzidine

12.763min (+0.006) 188077.36ng

response 805933

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.42
183.00	11.60	11.99
0.00	0.00	0.00