
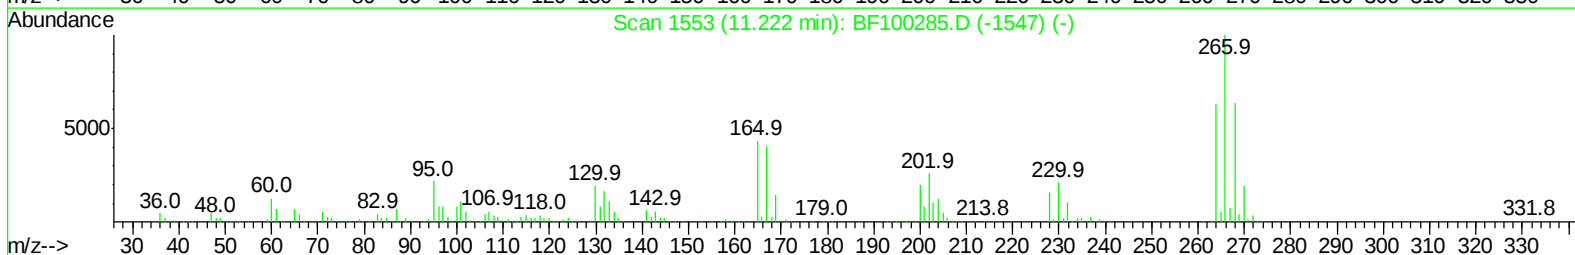
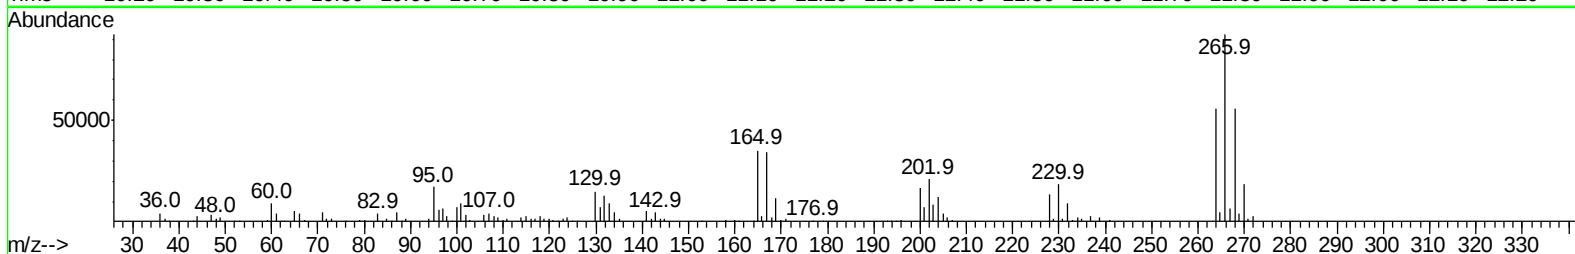


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF110917\
Data File : BF100369.D
Acq On : 10 Nov 2017 4:42
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 10 08:05:02 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 09 16:04:38 2017
Response via : Initial Calibration

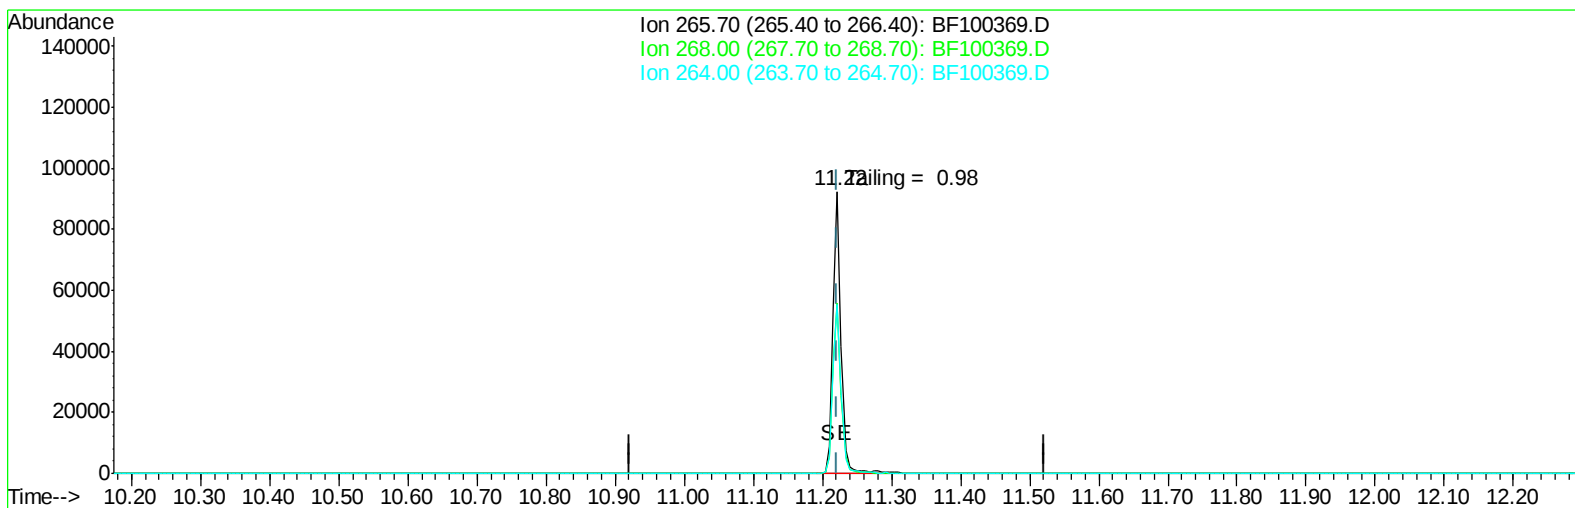

TIC: BF100369.D

(69) Pentachlorophenol (C)




11.221min (-0.000) 74457.56ng

response 75423

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	60.38
264.00	61.90	60.23
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF110917\
 Data File : BF100369.D
 Acq On : 10 Nov 2017 4:42
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 10 08:05:02 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 09 16:04:38 2017
 Response via : Initial Calibration

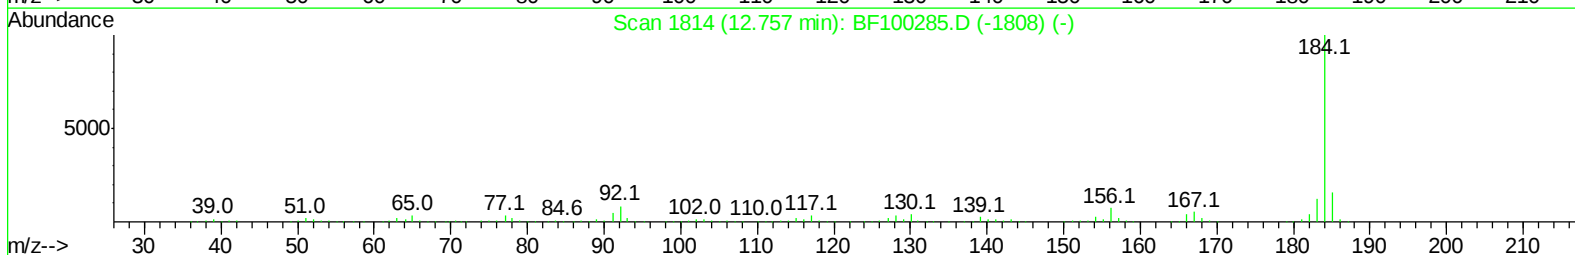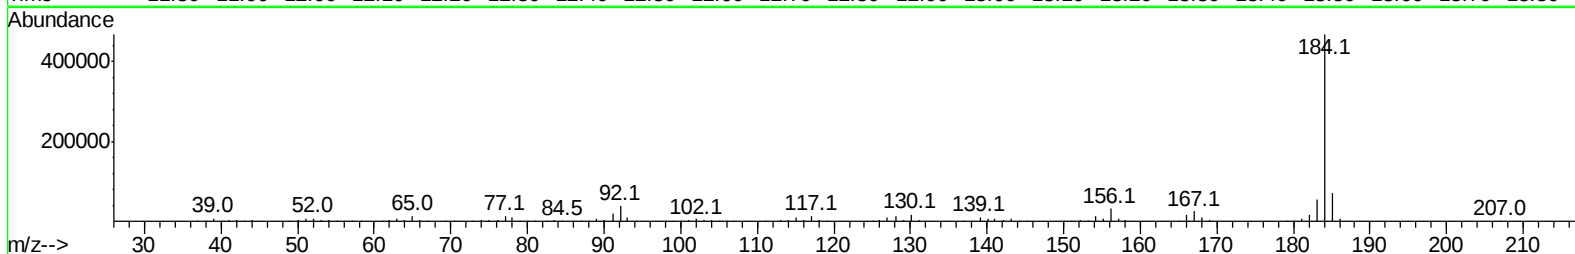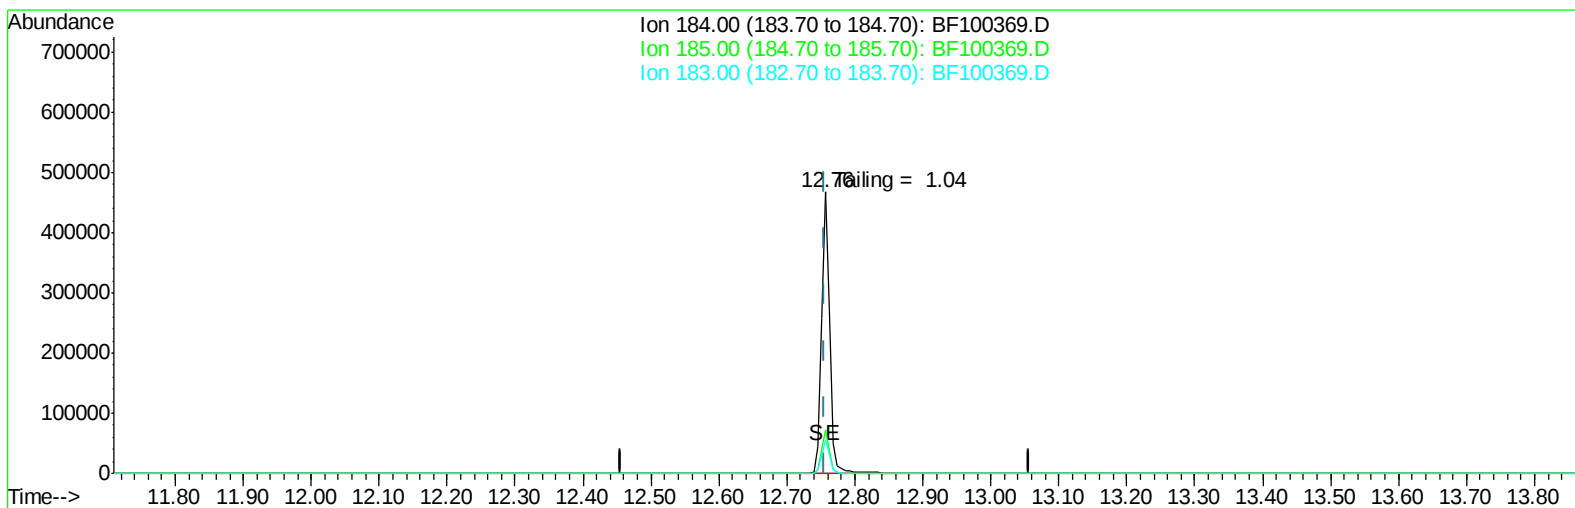

TIC: BF100369.D

(76) Benzidine

12.757min (-0.000) 0.00ng

response 401504

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.25
183.00	11.60	11.68
0.00	0.00	0.00