

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF110917\
 Data File : BF100376.D
 Acq On : 10 Nov 2017 8:18
 Operator : SJ/JU
 Sample : I6355-02
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 110317-TIDO-F-D-S

Quant Time: Nov 10 11:32:51 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 09 16:04:38 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.90	152	184584	20.00	ng	0.00
21) Naphthalene-d8	8.18	136	707843	20.00	ng	0.00
38) Acenaphthene-d10	9.94	164	312384	20.00	ng	0.00
63) Phenanthrene-d10	11.42	188	518467	20.00	ng	0.00
75) Chrysene-d12	14.06	240	356602	20.00	ng	-0.01
86) Perylene-d12	15.54	264	355685	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.52	112	572318	49.70	ng	0.00
7) Phenol-d6	6.52	99	518388	36.51	ng	0.00
23) Nitrobenzene-d5	7.47	82	1203801	112.44	ng	0.00
41) 2,4,6-Tribromophenol	10.73	330	310561	97.56	ng	0.00
44) 2-Fluorobiphenyl	9.26	172	1963678	95.72	ng	0.00
78) Terphenyl-d14	13.01	244	1395005	89.88	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA F\DATA\BF110917\
Data File : BF100376.D
Acq On : 10 Nov 2017 8:18
Operator : SJ/JU
Sample : I6355-02
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
110317-TIDO-F-D-S

Quant Time: Nov 10 11:32:51 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 09 16:04:38 2017
Response via : Initial Calibration

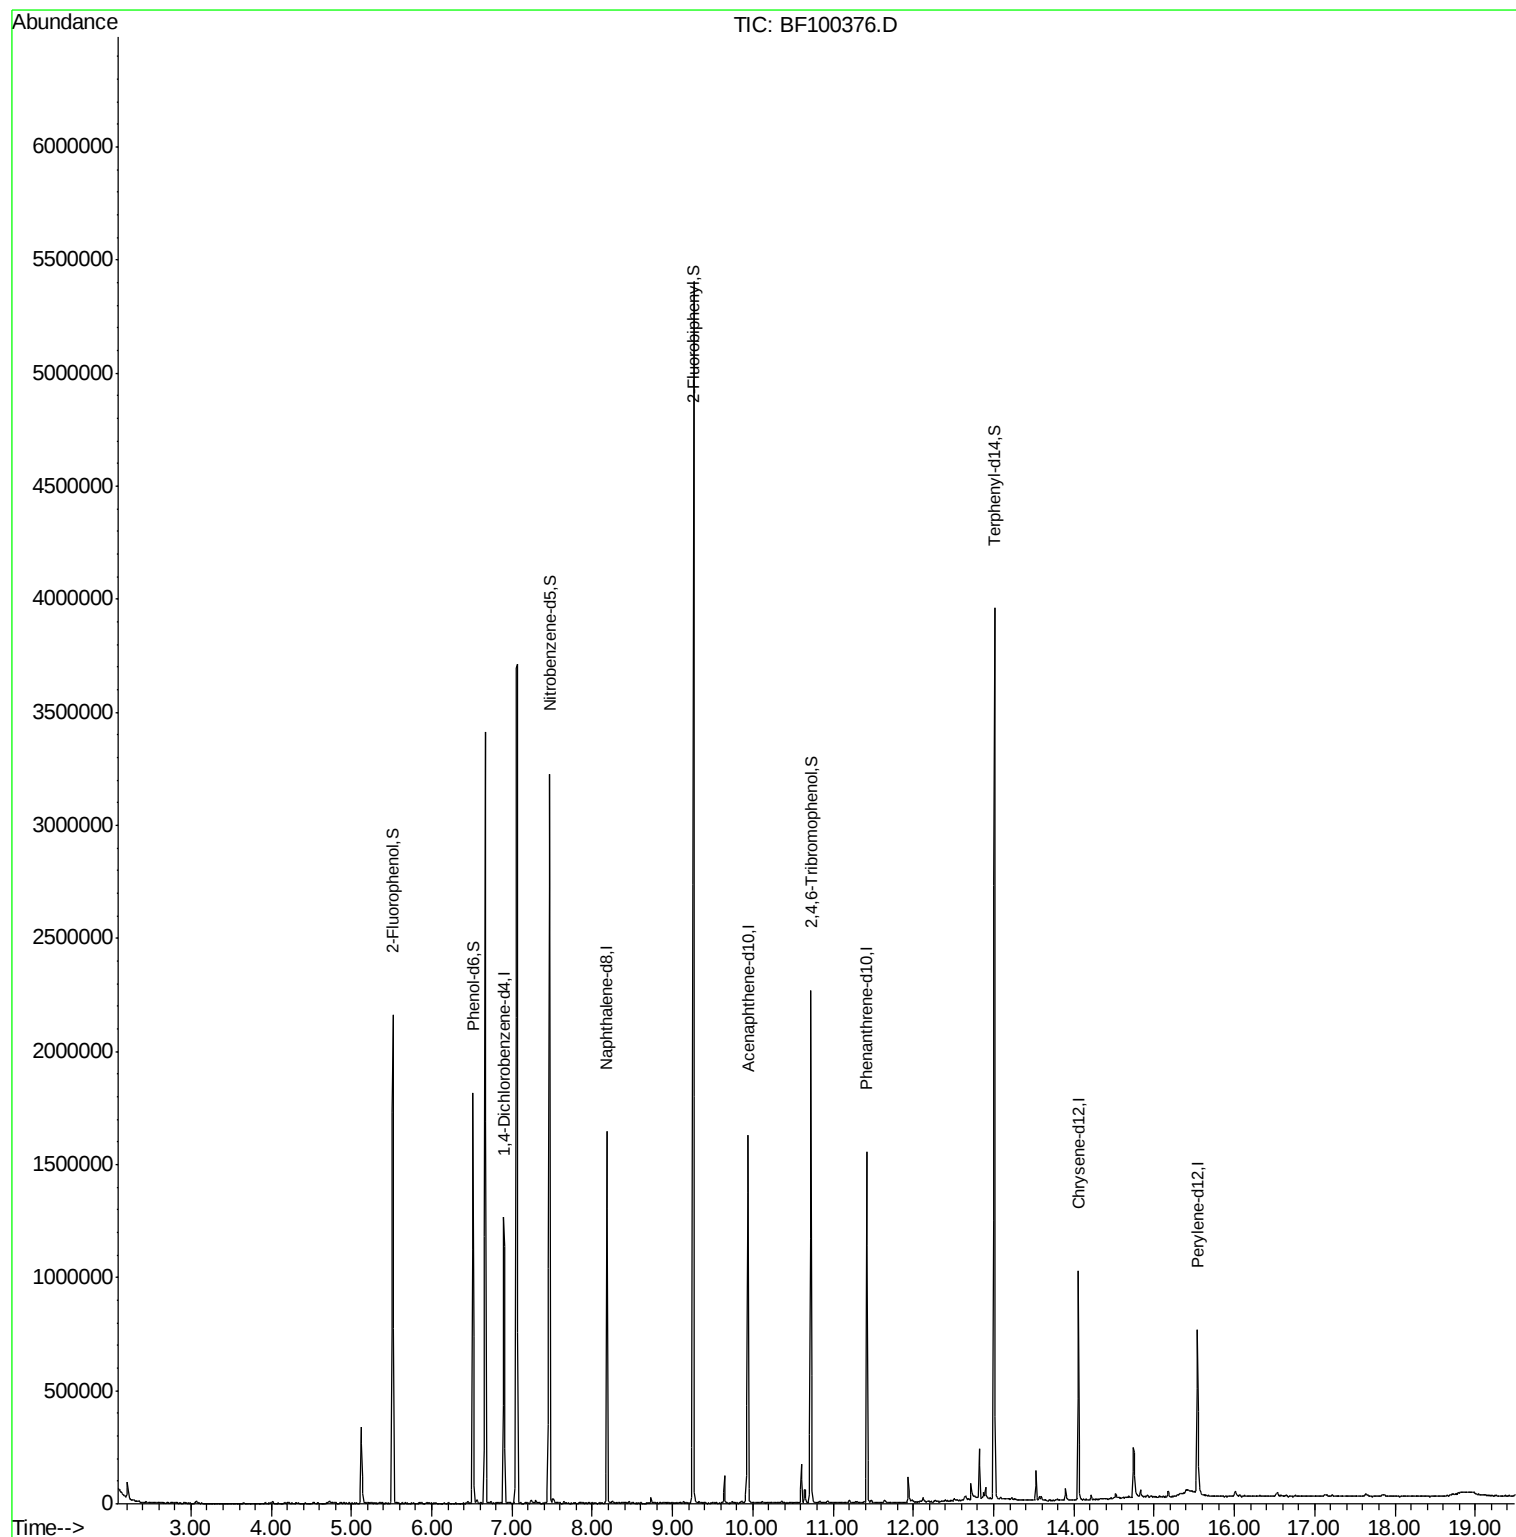

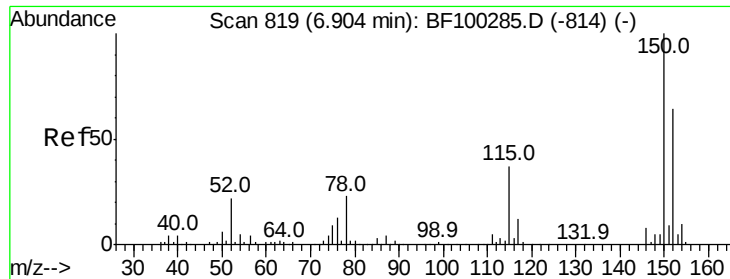


#1




1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.90 min Scan# 818
 Delta R.T. -0.01 min
 Lab File: BF100376.D
 Acq: 10 Nov 2017 8:18

Instrument :
 BNA_F
 ClientSampleId :
 110317-TIDO-F-D-S

Tot Ion	Ratio	Lower	Upper
152	100		
150	160.4	124.6	186.8
115	63.3	50.1	75.1

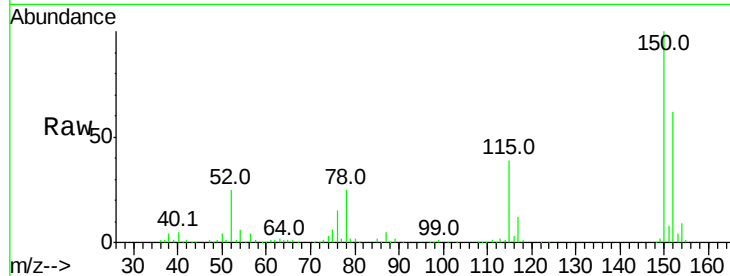


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

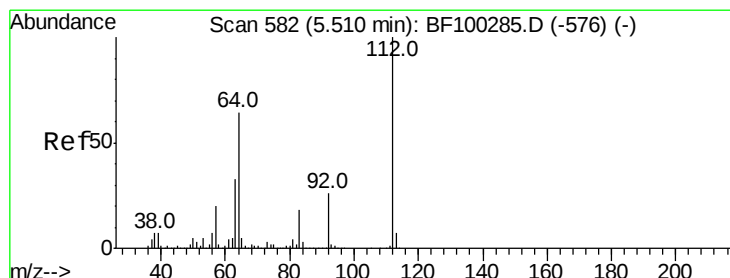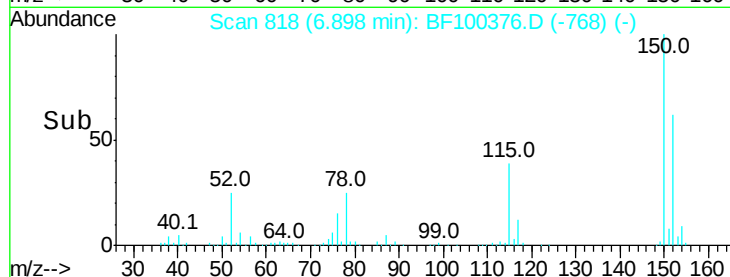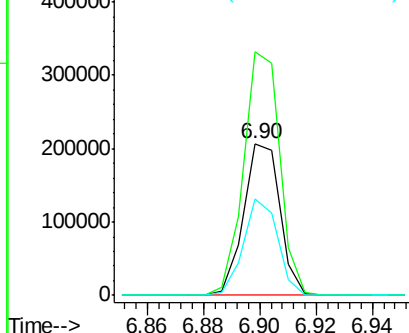



#5

2-Fluorophenol
 Concen: 49.702 ng
 RT: 5.52 min Scan# 583
 Delta R.T. 0.01 min
 Lab File: BF100376.D
 Acq: 10 Nov 2017 8:18

Tgt Ion	Ratio	Lower	Upper
112	100		
64	60.4	47.9	71.9
63	30.5	23.7	35.5

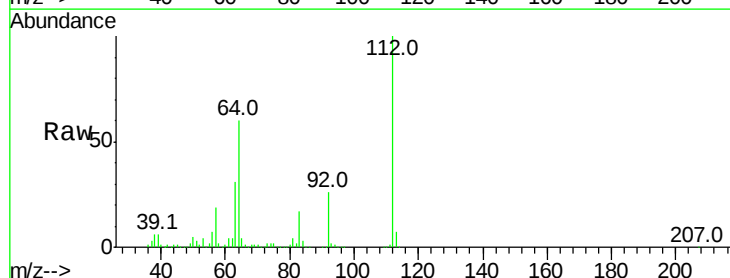

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF1
 Ion 63.00 (62.70 to 63.70): BF1

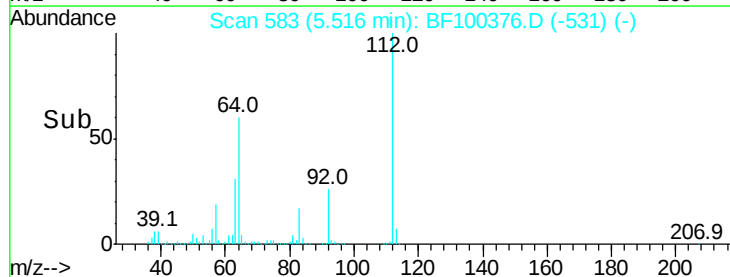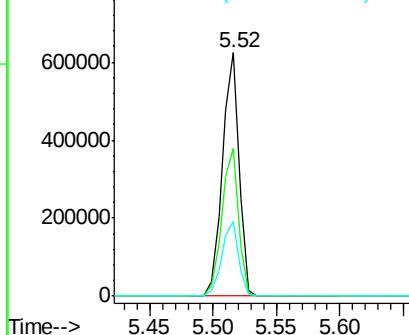



#7

Phenol-d6

Concen: 36.507 ng

RT: 6.52 min Scan# 753

Delta R.T. -0.01 min

Lab File: BF100376.D

Acq: 10 Nov 2017 8:18

Instrument :

BNA_F

ClientSampleId :

110317-TIDO-F-D-S





Tot Ion: 99 Resp: 518388

Ion Ratio Lower Upper

99 100

42 20.3 14.5 21.7

71 31.7 25.4 38.0

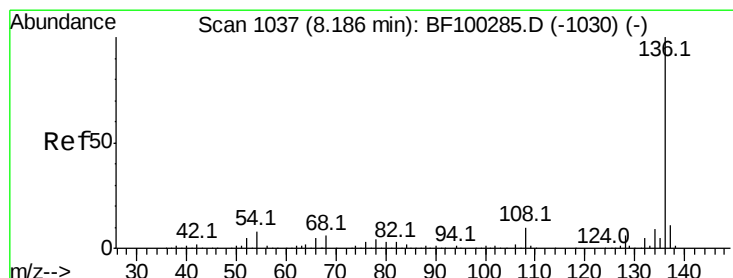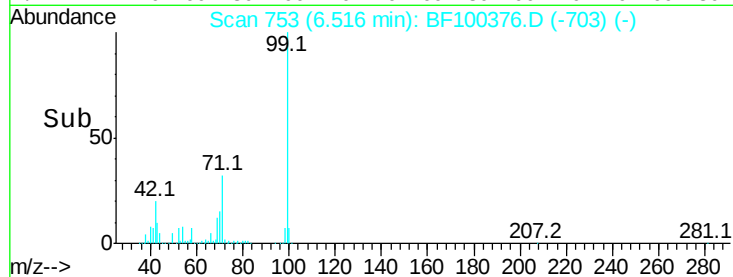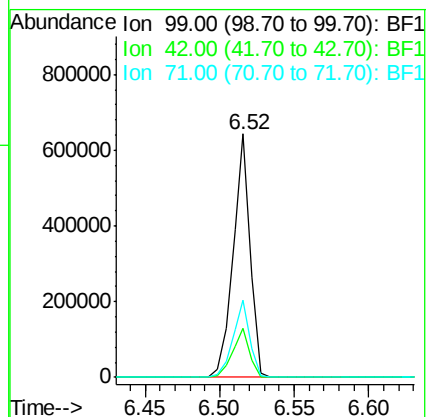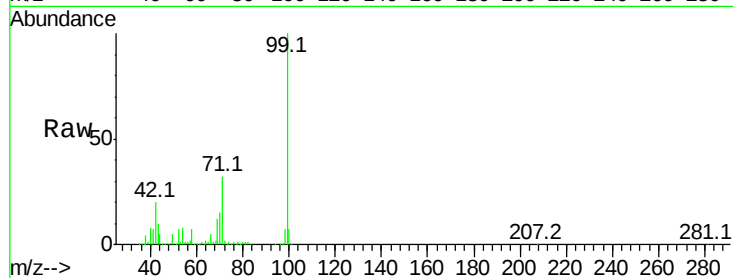

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.18 min Scan# 1036

Delta R.T. -0.01 min

Lab File: BF100376.D

Acq: 10 Nov 2017 8:18

Tgt Ion: 136 Resp: 707843




Ion Ratio Lower Upper


136 100

137 11.2 8.9 13.3

54 9.6 6.6 9.8

68 6.6 5.0 7.4

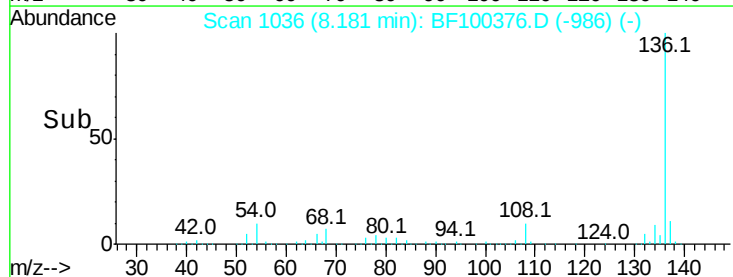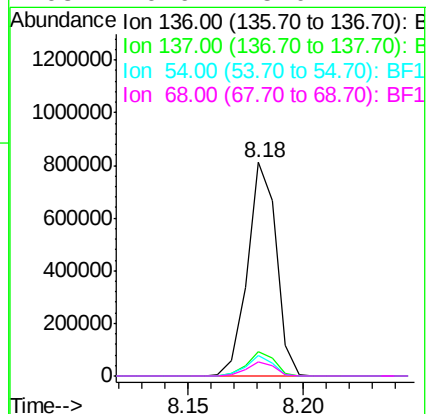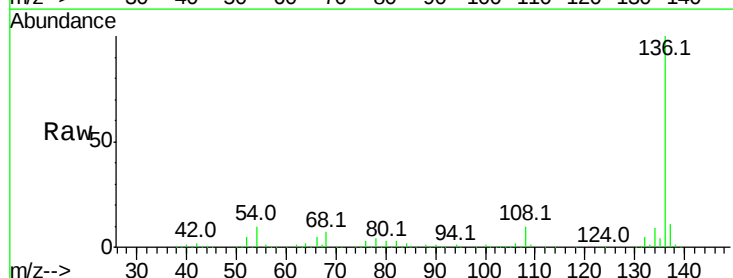

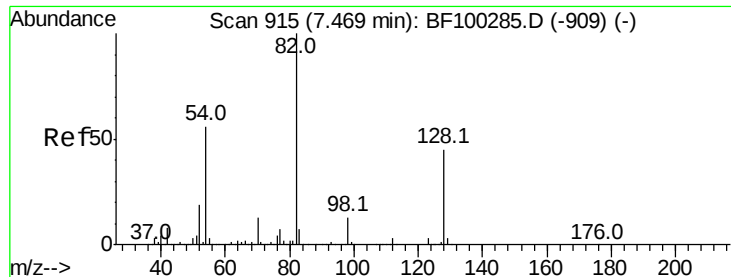

#23

Nitrobenzene-d5

Concen: 112.436 ng

RT: 7.47 min Scan# 915

Delta R.T. 0.00 min

Lab File: BF100376.D

Acq: 10 Nov 2017 8:18

Instrument :


BNA_F

ClientSampleId :

110317-TIDO-F-D-S

Tot Ion: 82 Resp: 1203801

Ion	Ratio	Lower	Upper
82	100		
128	46.0	36.1	54.1
54	55.0	41.4	62.2



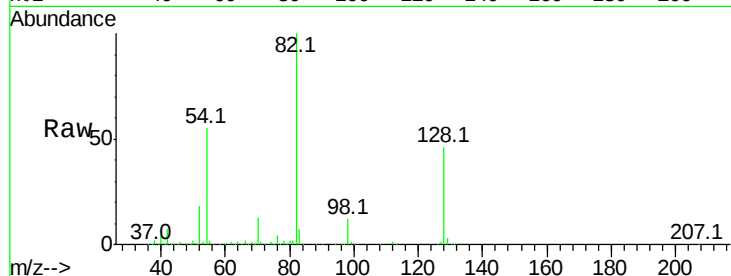


Abundance

Ion 82.00 (81.70 to 82.70): BF1

Ion 128.00 (127.70 to 128.70): BF1

Ion 54.00 (53.70 to 54.70): BF1

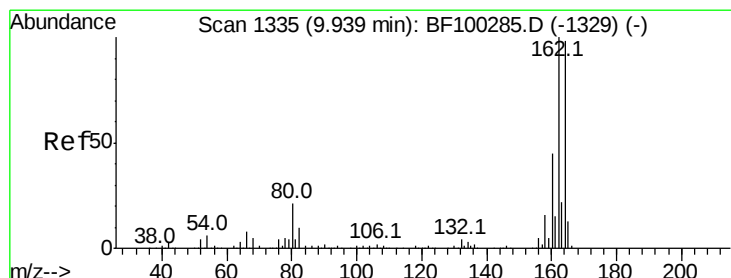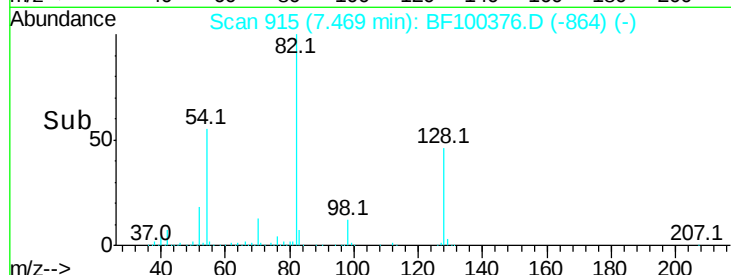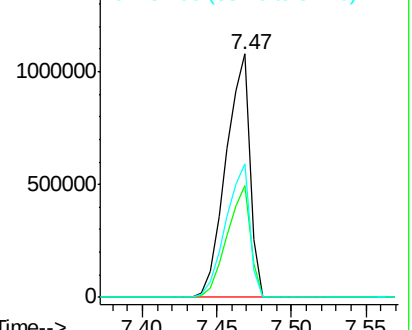

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.94 min Scan# 1335


Delta R.T. 0.00 min

Lab File: BF100376.D

Acq: 10 Nov 2017 8:18

Tgt Ion:164 Resp: 312384

Ion	Ratio	Lower	Upper
164	100		
162	103.8	86.1	129.1
160	48.4	38.3	57.5


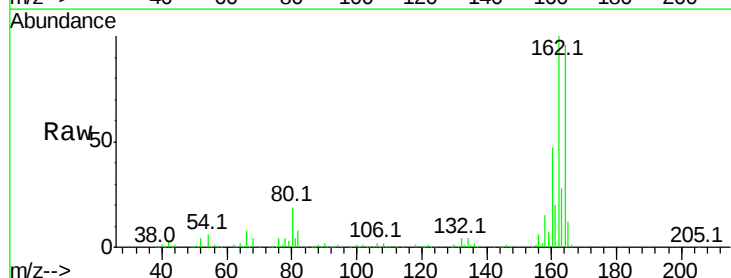



Abundance

Ion 164.00 (163.70 to 164.70): BF1

Ion 162.00 (161.70 to 162.70): BF1

Ion 160.00 (159.70 to 160.70): BF1

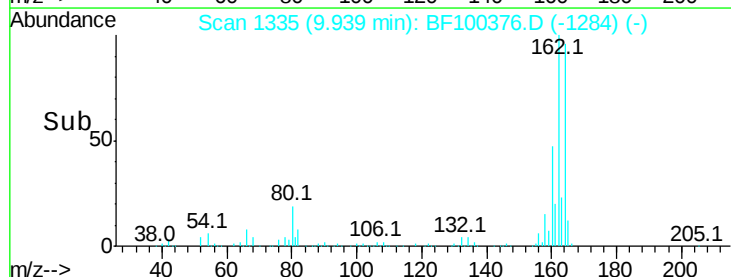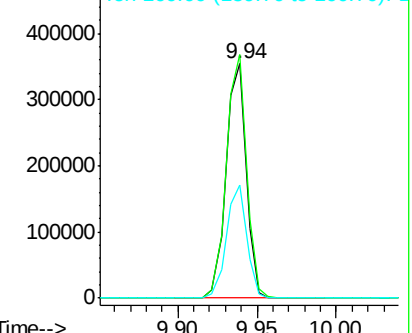


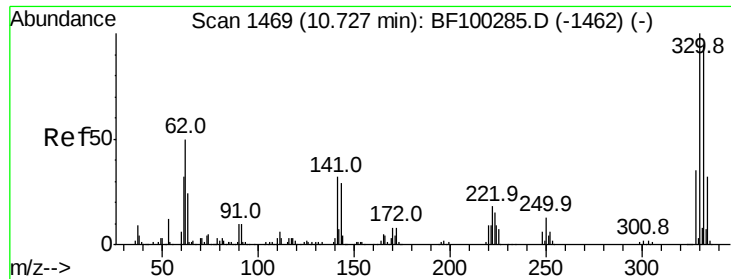




#41
 2,4,6-Tribromophenol
 Concen: 97.563 ng
 RT: 10.73 min Scan# 1469
 Delta R.T. 0.00 min
 Lab File: BF100376.D
 Acq: 10 Nov 2017 8:18

Instrument :
 BNA_F
 ClientSampleId :
 110317-TIDO-F-D-S

Tot Ion	Ratio	Lower	Upper
330	100		
332	94.9	77.0	115.6
141	30.6	29.9	44.9

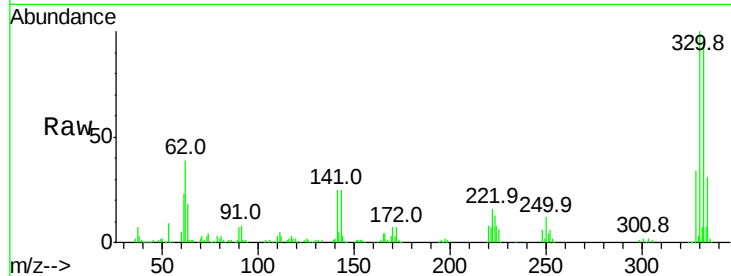


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

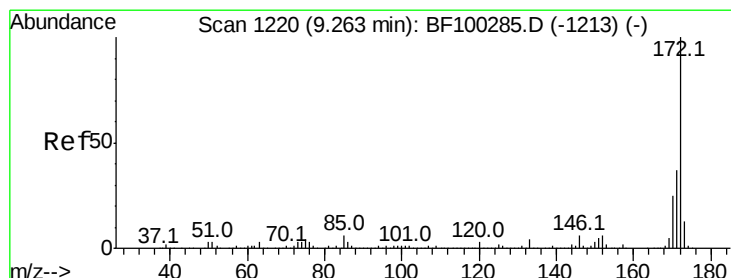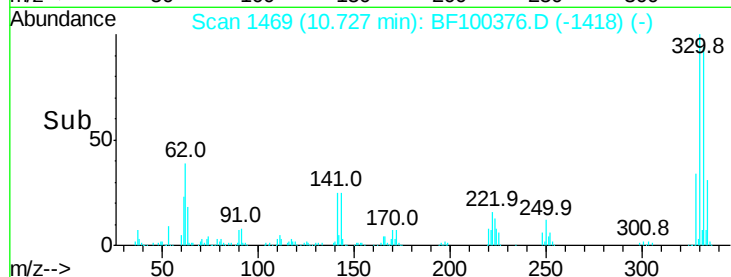
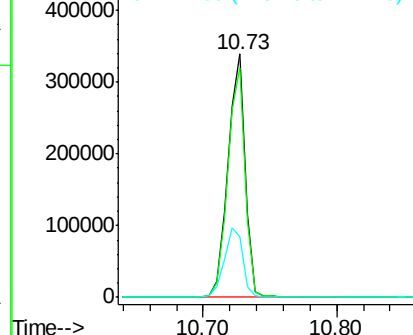


#44
 2-Fluorobiphenyl
 Concen: 95.719 ng
 RT: 9.26 min Scan# 1220
 Delta R.T. 0.00 min
 Lab File: BF100376.D
 Acq: 10 Nov 2017 8:18

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.6	29.7	44.5
170	24.7	19.6	29.4

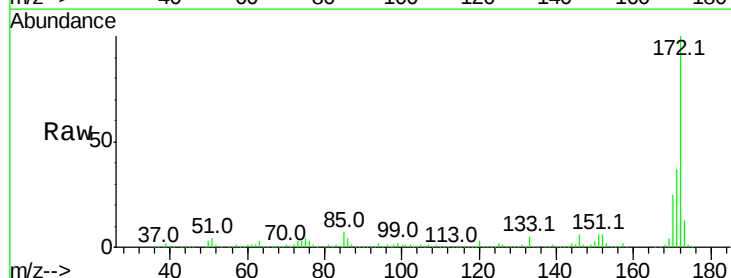

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

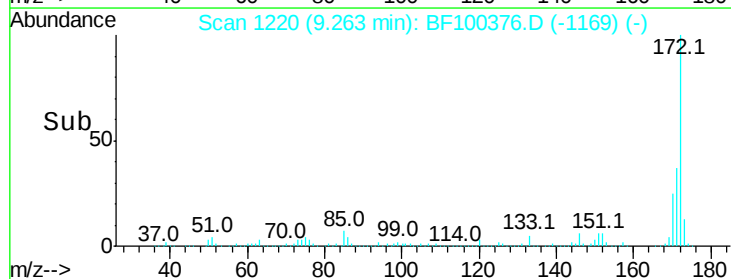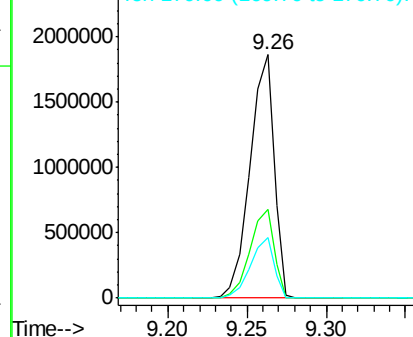



#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.42 min Scan# 1587

Delta R.T. -0.01 min

Lab File: BF100376.D

Acq: 10 Nov 2017 8:18

Instrument :

BNA_F

ClientSampleId :

110317-TIDO-F-D-S


Tot Ion:188 Resp: 518467

Ion Ratio Lower Upper

188 100

94 10.4 8.5 12.7




80 11.2 9.2 13.8

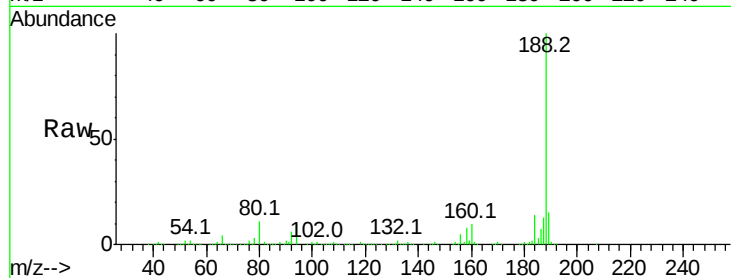

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

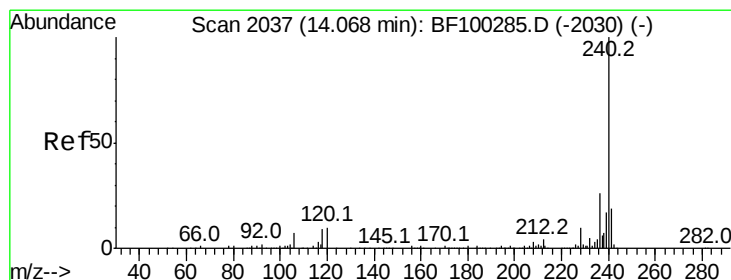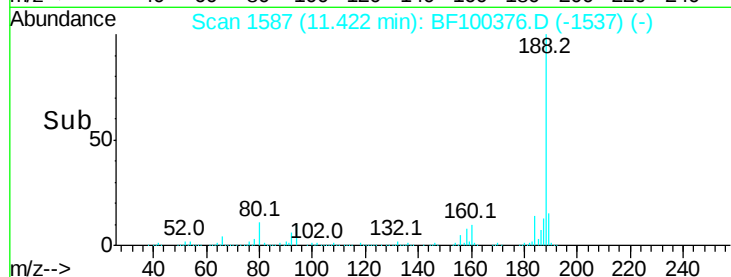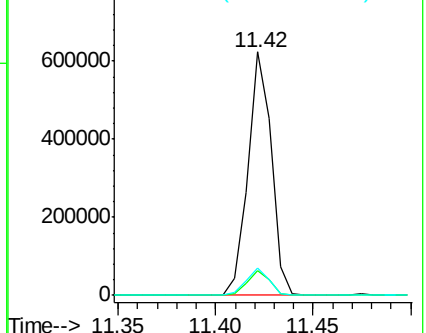

#75

Chrysene-d12

Concen: 20.000 ng

RT: 14.06 min Scan# 2035

Delta R.T. -0.01 min

Lab File: BF100376.D

Acq: 10 Nov 2017 8:18


Tgt Ion:240 Resp: 356602

Ion Ratio Lower Upper

240 100

120 13.1 9.5 14.3



236 25.6 20.7 31.1

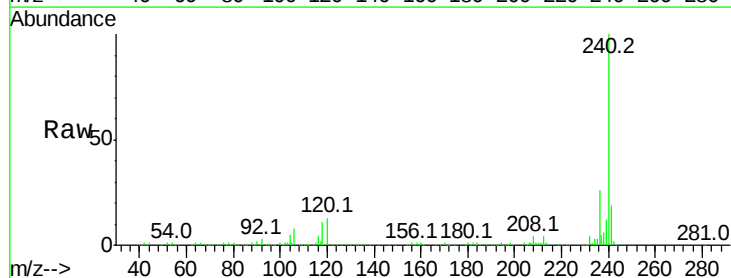

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

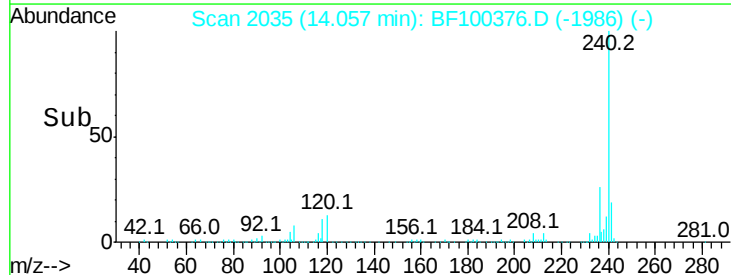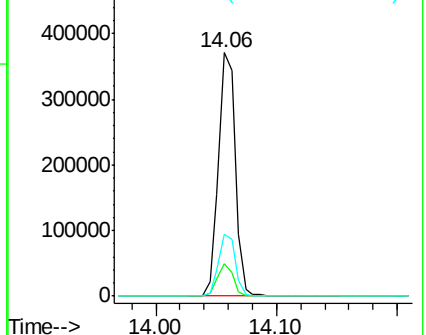



#78

Terphenyl-d14

Concen: 89.885 ng

RT: 13.01 min Scan# 1857

Delta R.T. 0.00 min

Lab File: BF100376.D

Acq: 10 Nov 2017 8:18

Instrument :

BNA_F

ClientSampleId :

110317-TIDO-F-D-S


Tot Ion:244 Resp: 1395005

Ion Ratio Lower Upper

244 100

212 7.1 5.4 8.0




122 12.1 11.0 16.4

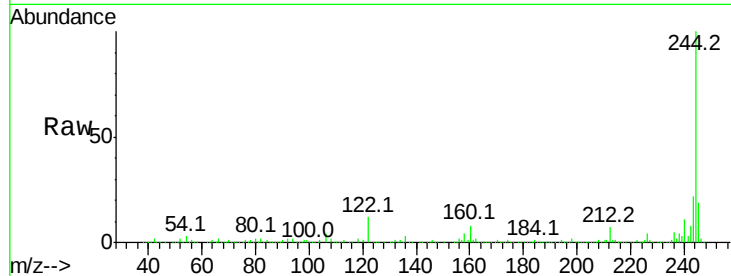

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

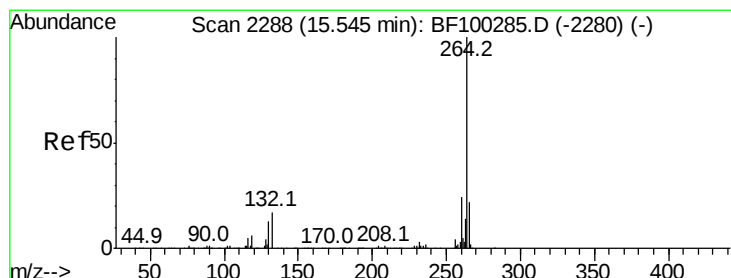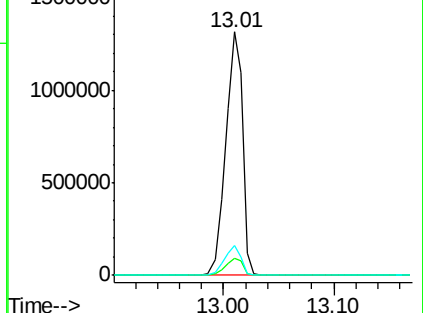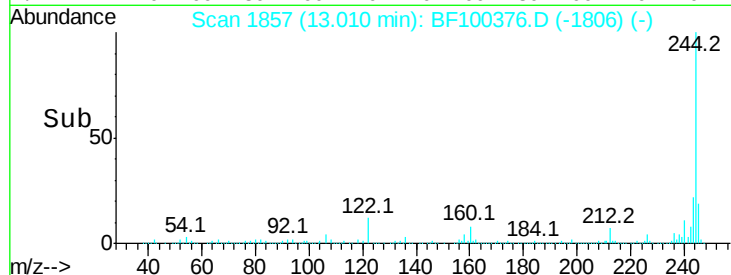

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.54 min Scan# 2287

Delta R.T. -0.01 min

Lab File: BF100376.D

Acq: 10 Nov 2017 8:18


Tgt Ion:264 Resp: 355685

Ion Ratio Lower Upper

264 100

260 23.3 19.2 28.8

265 21.1 17.5 26.3

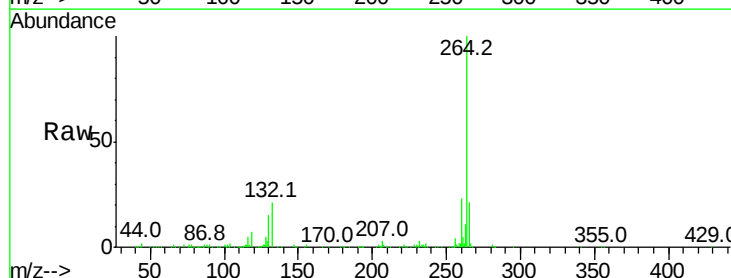

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

