

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF110917\
 Data File : BF100349.D
 Acq On : 9 Nov 2017 19:14
 Operator : SJ/JU
 Sample : PB104087BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB104087BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.140	514	519	529	rBV	479627	586409	15.79%	1.875%
2	5.528	579	585	588	rBV	2947959	2975869	80.11%	9.517%
3	6.522	748	754	757	rBV	3071541	2928387	78.83%	9.365%
4	6.669	774	779	782	rBV	3186265	3022503	81.37%	9.666%
5	6.898	815	818	822	rVB	1052137	928286	24.99%	2.969%
6	7.057	841	845	848	rBV	2752617	2393694	64.44%	7.655%
7	7.457	908	913	917	rBV	1805772	1917162	51.61%	6.131%
8	8.181	1031	1036	1040	rBV	1394985	1268029	34.14%	4.055%
9	9.257	1213	1219	1222	rBV	3692064	3596375	96.82%	11.501%
10	9.939	1329	1335	1338	rBV	1500863	1435097	38.63%	4.589%
11	10.728	1463	1469	1472	rBV	2165743	2217944	59.71%	7.093%
12	11.422	1583	1587	1591	rBV	1688821	1551276	41.76%	4.961%
13	13.010	1852	1857	1860	rBV	3862332	3714599	100.00%	11.879%
14	14.063	2032	2036	2039	rBV	1527187	1356912	36.53%	4.339%
15	15.180	2223	2226	2230	rVB	48125	50122	1.35%	0.160%
16	15.545	2282	2288	2298	rVB	809339	1082687	29.15%	3.462%
17	16.015	2363	2368	2373	rVB2	55268	77765	2.09%	0.249%
18	16.533	2451	2456	2464	rVB2	54241	99013	2.67%	0.317%
19	17.145	2556	2560	2570	rVB5	31966	68104	1.83%	0.218%


Sum of corrected areas: 31270233

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF110917\
Data File : BF100349.D
Acq On : 9 Nov 2017 19:14
Operator : SJ/JU
Sample : PB104087BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB104087BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

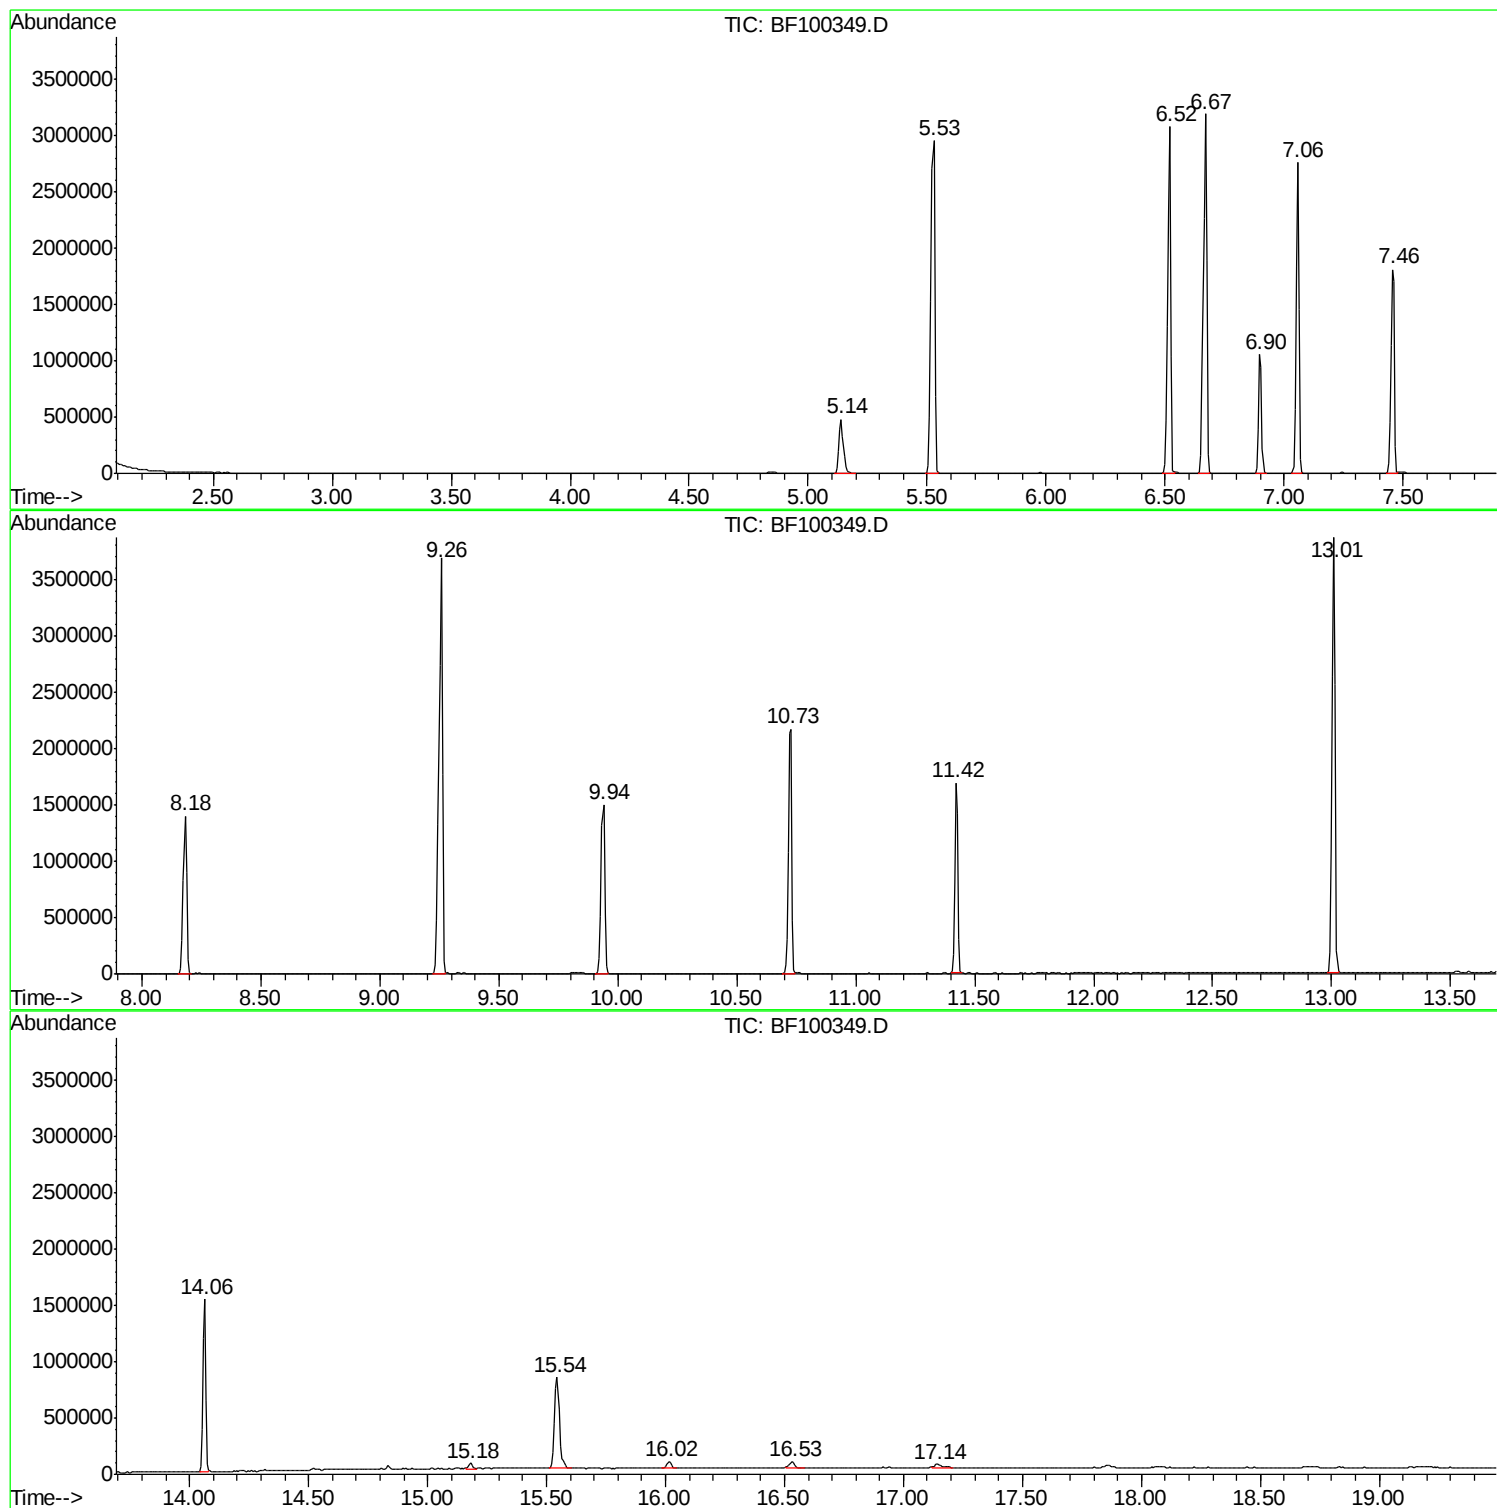

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF110917\
Data File : BF100349.D
Acq On : 9 Nov 2017 19:14
Operator : SJ/JU
Sample : PB104087BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB104087BL










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.14	12.63 ng	586409	1,4-Dichlorobenzene-d4	6.90

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	64
2			3-Hexanol, 4-methyl-	116	C7H16O	000615-29-2	33
3			Acetic acid, cyano-, 1,1-dimethyl...	141	C7H11NO2	001116-98-9	25
4			1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10
5			2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	9

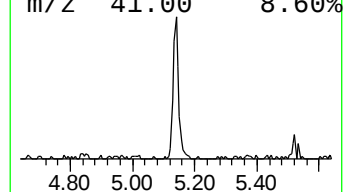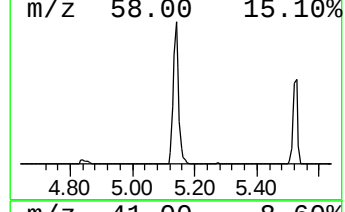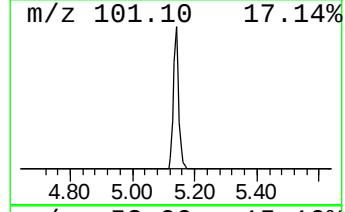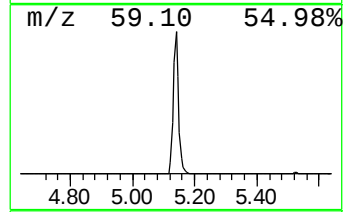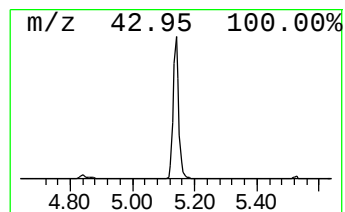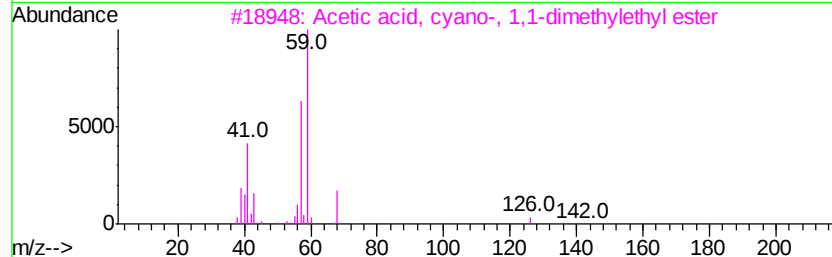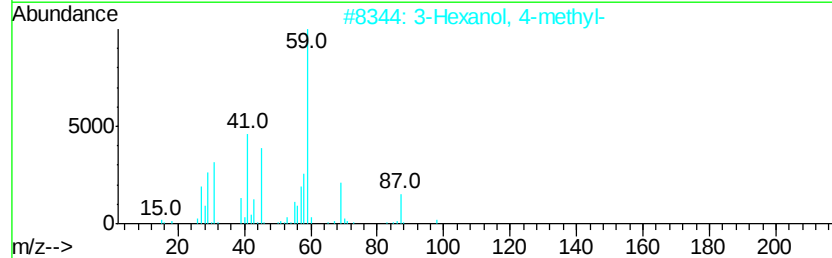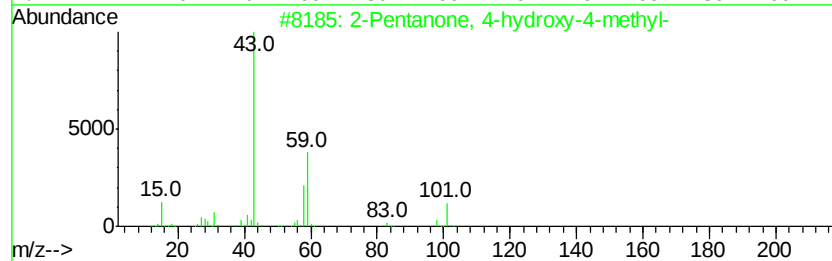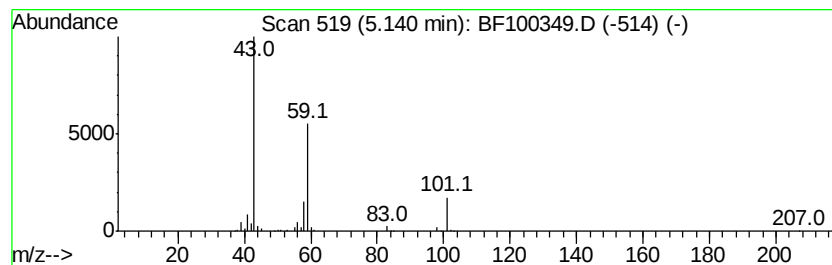

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA F\DATA\BF110917\
Data File : BF100349.D
Acq On : 9 Nov 2017 19:14
Operator : SJ/JU
Sample : PB104087BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB104087BL










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.67 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.67	65.12 ng	3022500	1,4-Dichlorobenzene-d4	6.90

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		5-Aminoindole	132	C8H8N2	005192-03-0	12
3		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	9
4		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
5		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9

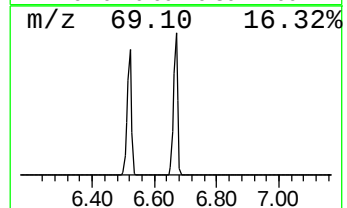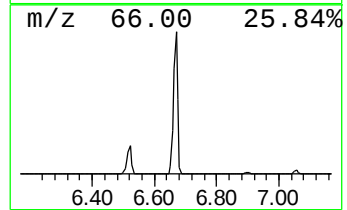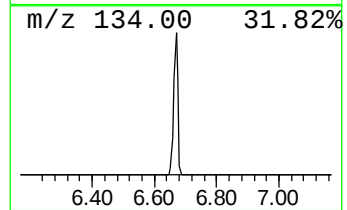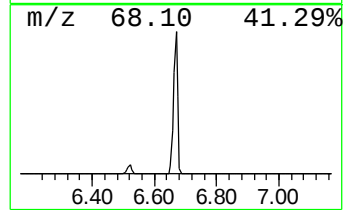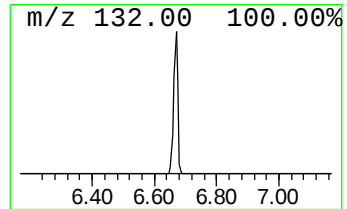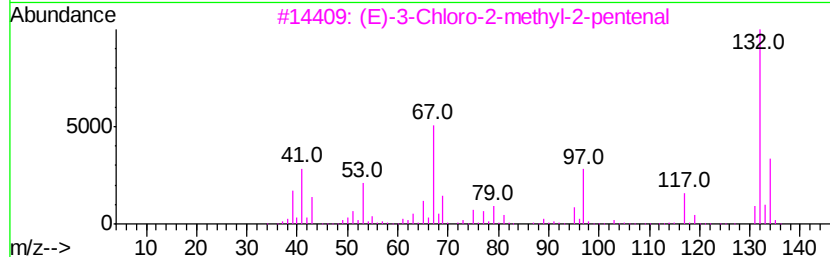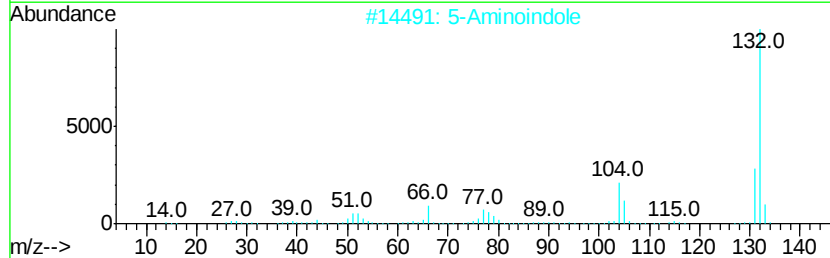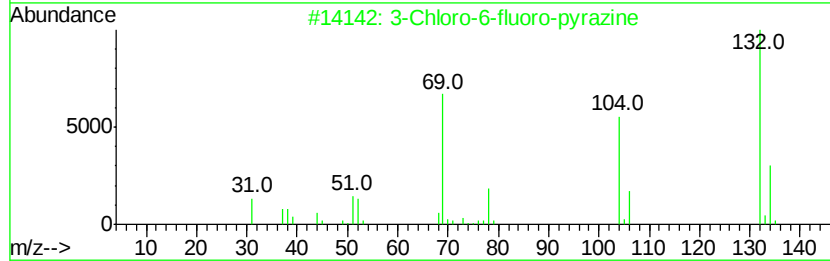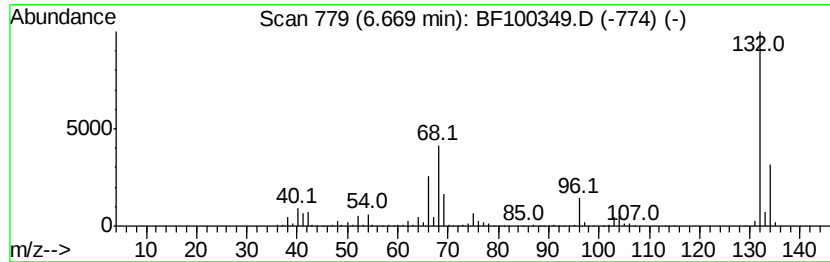

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF110917\
Data File : BF100349.D
Acq On : 9 Nov 2017 19:14
Operator : SJ/JU
Sample : PB104087BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB104087BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	5.14	12.6	ng	586409	1	6.90	928286	20.0
unknown6.67	6.67	65.1	ng	3022500	1	6.90	928286	20.0