


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF110917\
 Data File : BF100331.D
 Acq On : 9 Nov 2017 10:12
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Nov 09 16:04:38 2017

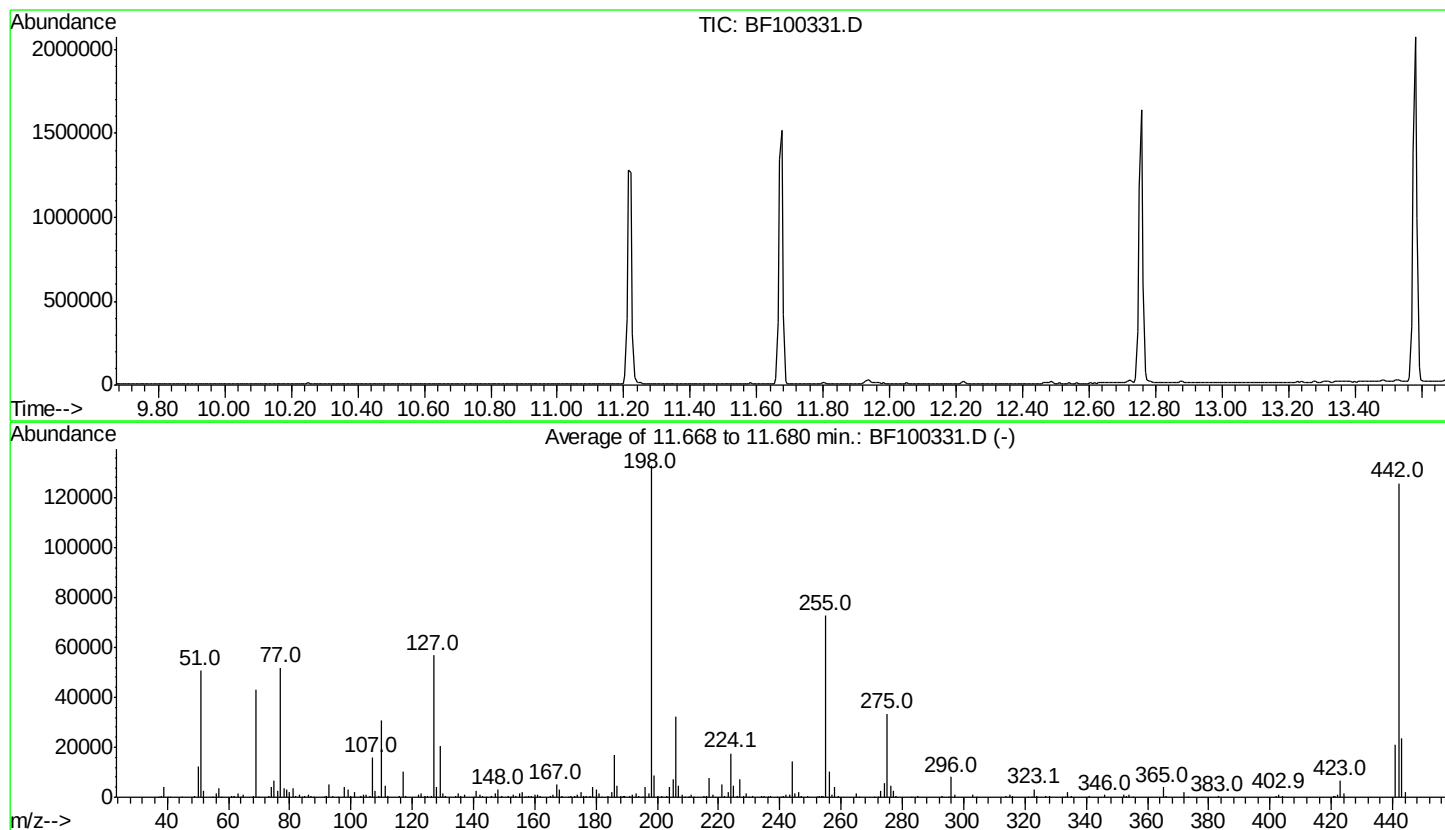

AutoFind: Scans 1629, 1630, 1631; Background Corrected with Scan 1623

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.2	50709	PASS
68	69	0.00	2	1.5	652	PASS
69	198	0.00	100	32.3	42915	PASS
70	69	0.00	2	0.6	257	PASS
127	198	10	80	42.8	56909	PASS
197	198	0.00	2	1.1	1400	PASS
198	198	100	100	100.0	132861	PASS
199	198	5	9	6.5	8589	PASS
275	198	10	60	25.2	33497	PASS
365	198	1	100	3.1	4054	PASS
441	443	0.01	100	87.8	20912	PASS
442	198	50	100	94.7	125762	PASS
443	442	15	24	18.9	23808	PASS