


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF110917\
 Data File : BF100343.D
 Acq On : 9 Nov 2017 16:15
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Nov 09 16:04:38 2017

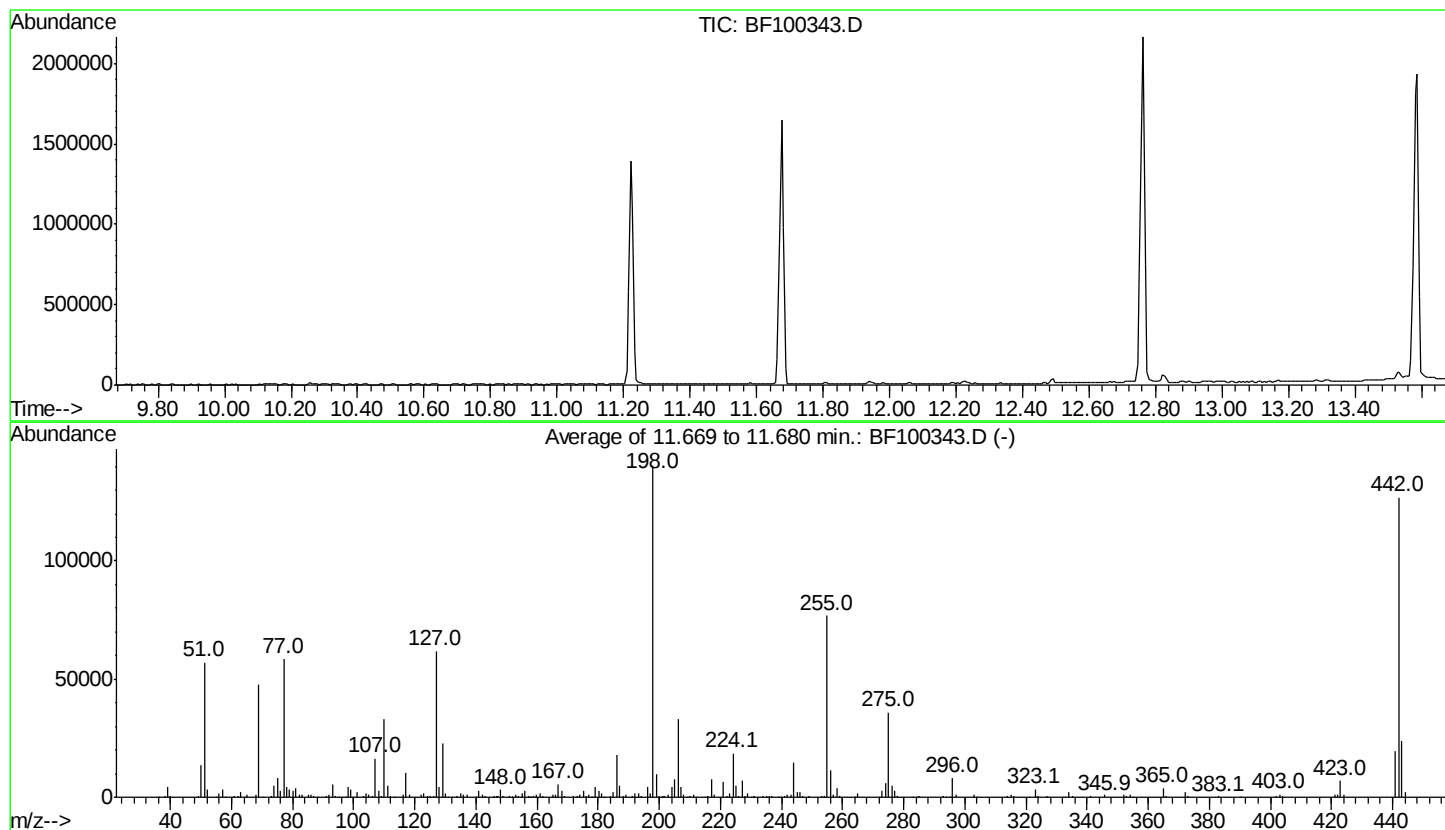

AutoFind: Scans 1629, 1630, 1631; Background Corrected with Scan 1624

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.7	57125	PASS
68	69	0.00	2	1.9	891	PASS
69	198	0.00	100	34.1	47869	PASS
70	69	0.00	2	0.3	143	PASS
127	198	10	80	44.2	62002	PASS
197	198	0.00	2	1.1	1476	PASS
198	198	100	100	100.0	140365	PASS
199	198	5	9	7.0	9776	PASS
275	198	10	60	25.5	35816	PASS
365	198	1	100	2.7	3821	PASS
441	443	0.01	100	82.1	19651	PASS
442	198	50	100	90.4	126837	PASS
443	442	15	24	18.9	23947	PASS