


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF110917\  
 Data File : BF100369.D  
 Acq On : 10 Nov 2017 4:42  
 Operator : SJ/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF110817.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Thu Nov 09 16:04:38 2017

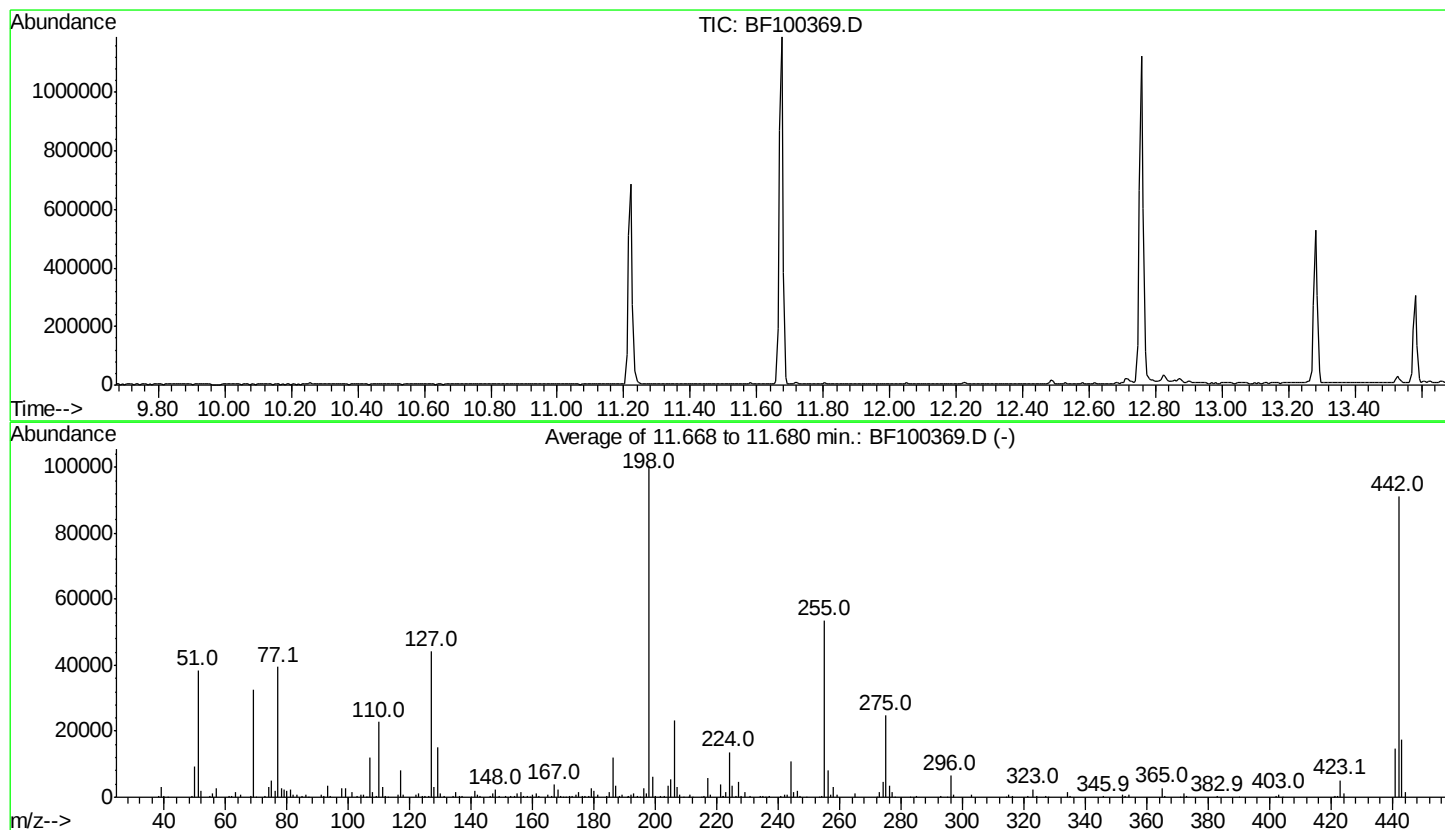

AutoFind: Scans 1629, 1630, 1631; Background Corrected with Scan 1624

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 38.2         | 38352      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.5          | 501        | PASS                |
| 69             | 198             | 0.00            | 100             | 32.5         | 32654      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.4          | 120        | PASS                |
| 127            | 198             | 10              | 80              | 44.0         | 44174      | PASS                |
| 197            | 198             | 0.00            | 2               | 1.0          | 1048       | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 100485     | PASS                |
| 199            | 198             | 5               | 9               | 6.3          | 6285       | PASS                |
| 275            | 198             | 10              | 60              | 24.6         | 24695      | PASS                |
| 365            | 198             | 1               | 100             | 2.8          | 2779       | PASS                |
| 441            | 443             | 0.01            | 100             | 84.8         | 14857      | PASS                |
| 442            | 198             | 50              | 100             | 90.7         | 91125      | PASS                |
| 443            | 442             | 15              | 24              | 19.2         | 17526      | PASS                |