
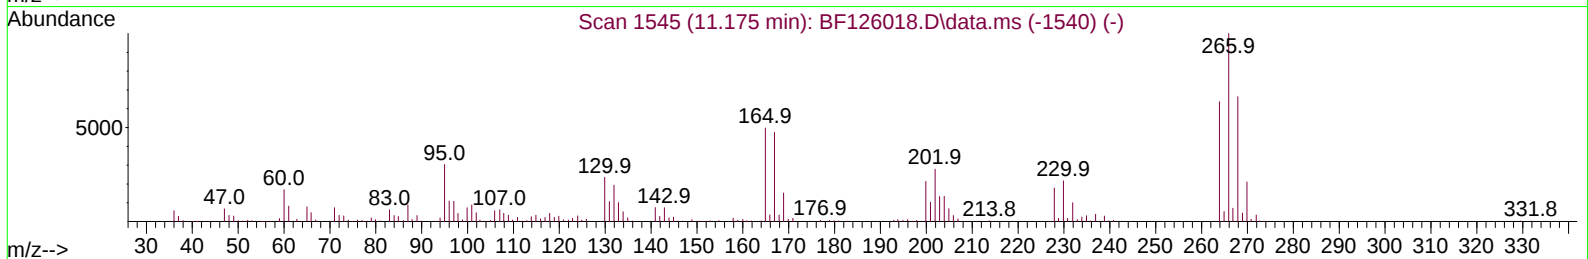
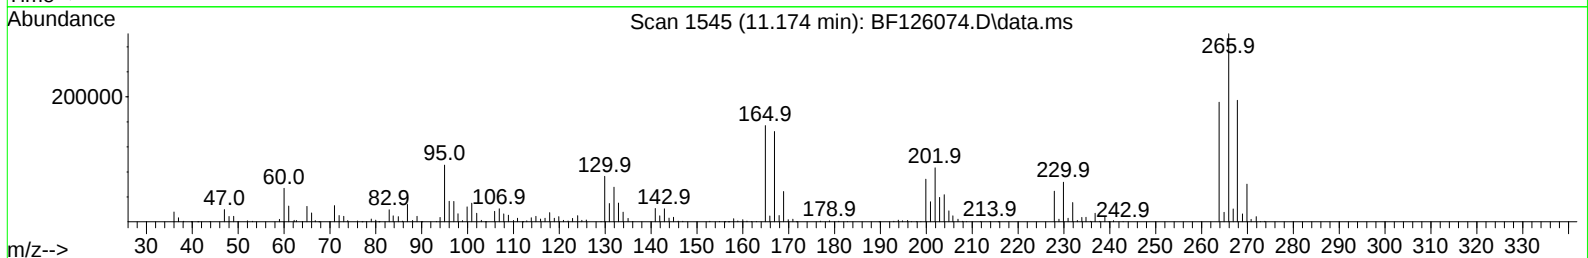


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110921\
 Data File : BF126074.D
 Acq On : 9 Nov 2021 10:18
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 09 12:12:57 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 03 17:21:25 2021
 Response via : Initial Calibration

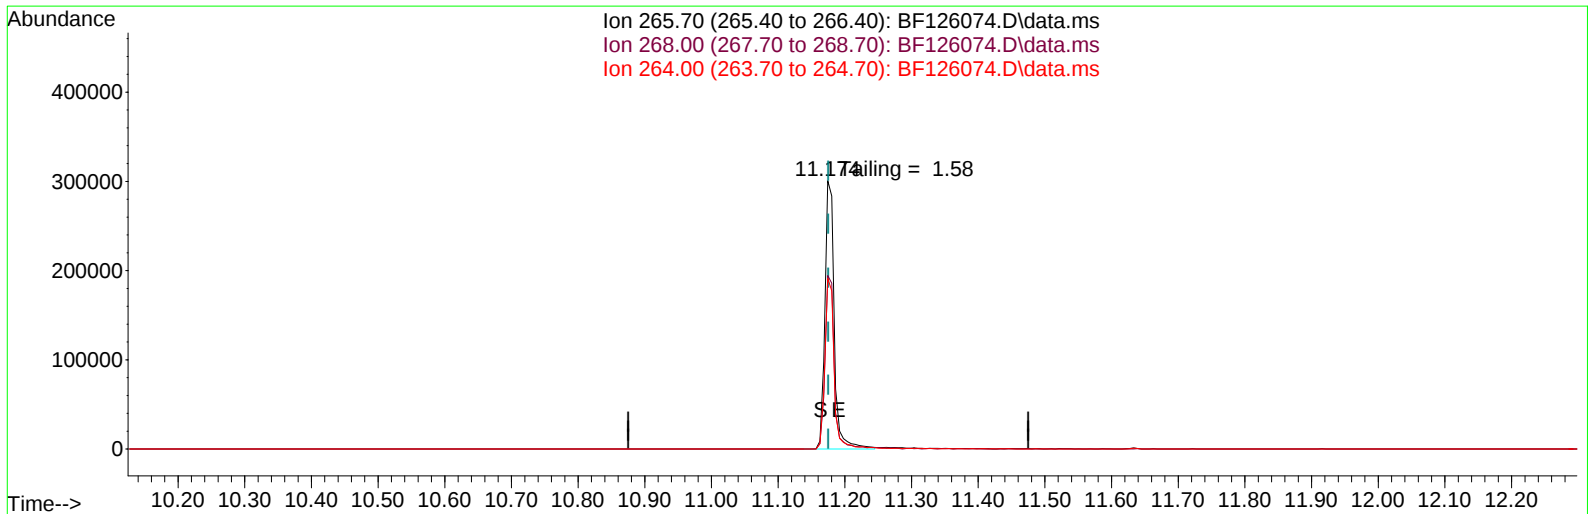

TIC: BF126074.D\data.ms

(70) Pentachlorophenol (C)




11.174min (-0.001) 23815.62 ng

response 295362

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	64.65
264.00	69.90	63.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110921\
 Data File : BF126074.D
 Acq On : 9 Nov 2021 10:18
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 09 12:12:57 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 03 17:21:25 2021
 Response via : Initial Calibration

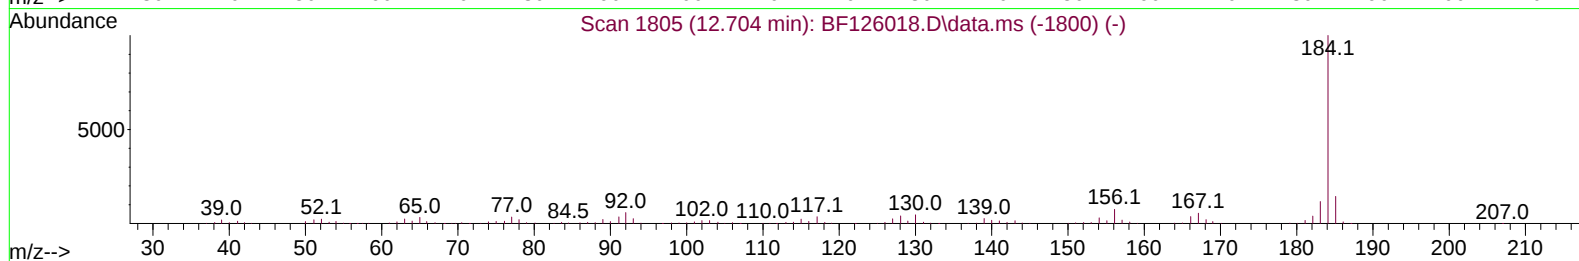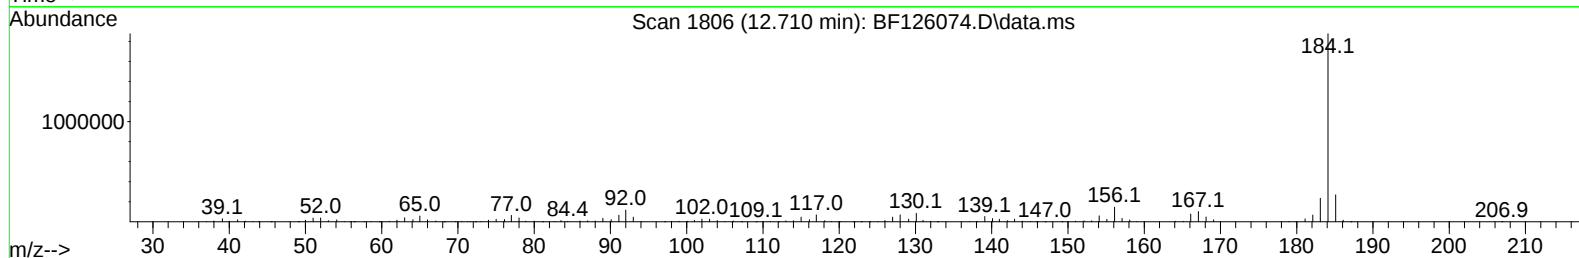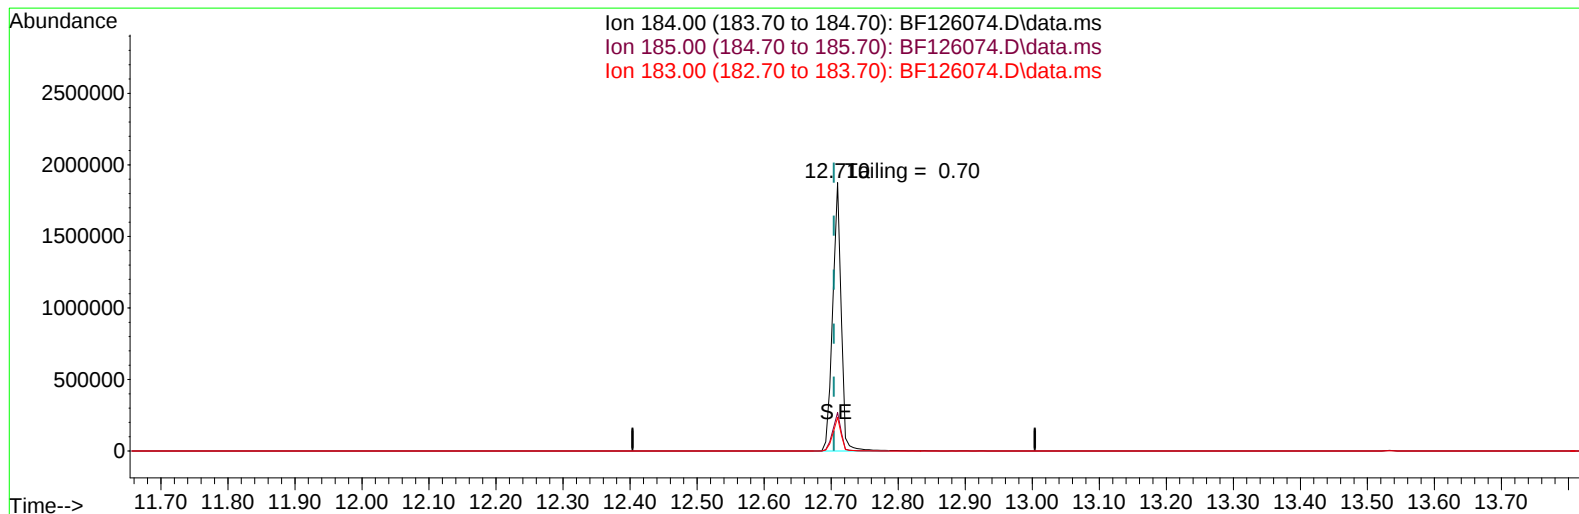

TIC: BF126074.D\data.ms

(77) Benzidine

12.710min (+ 0.006) 0.00 ng

response 1655783

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.36
183.00	10.10	12.52#
0.00	0.00	0.00