

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110921\
 Data File : BF126081.D
 Acq On : 9 Nov 2021 14:19
 Operator : JU/CG
 Sample : M4567-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 BASEMENT

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF126081.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.187	6	17	25	rVB	2653043	3499366	100.00%	20.235%
2	5.063	502	506	514	rVB	90189	86747	2.48%	0.502%
3	5.463	571	574	581	rBV	246732	235581	6.73%	1.362%
4	6.469	741	745	754	rVB	549412	459056	13.12%	2.655%
5	6.851	806	810	813	rBV	1424960	1104051	31.55%	6.384%
6	7.410	900	905	908	rBV	1418299	1367183	39.07%	7.906%
7	8.034	1007	1011	1023	rBV	79840	114355	3.27%	0.661%
8	8.134	1023	1028	1031	rBV	1594085	1405884	40.18%	8.130%
9	9.204	1205	1210	1222	rBV	2345980	2064015	58.98%	11.935%
10	9.886	1321	1326	1336	rBV	1958029	1709854	48.86%	9.887%
11	10.669	1456	1459	1464	rBV	253585	229452	6.56%	1.327%
12	11.369	1574	1578	1585	rBV	1965481	1724249	49.27%	9.971%
13	12.951	1844	1847	1851	rBV	1411405	1123792	32.11%	6.498%
14	14.004	2022	2026	2035	rVB	1088643	1054423	30.13%	6.097%
15	15.468	2270	2275	2281	rBV	792211	1040454	29.73%	6.017%
16	15.951	2352	2357	2361	rVB6	24322	39624	1.13%	0.229%
17	16.457	2440	2443	2448	rVB6	21908	35237	1.01%	0.204%




Sum of corrected areas: 17293323

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110921\
Data File : BF126081.D
Acq On : 9 Nov 2021 14:19
Operator : JU/CG
Sample : M4567-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BASEMENT

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

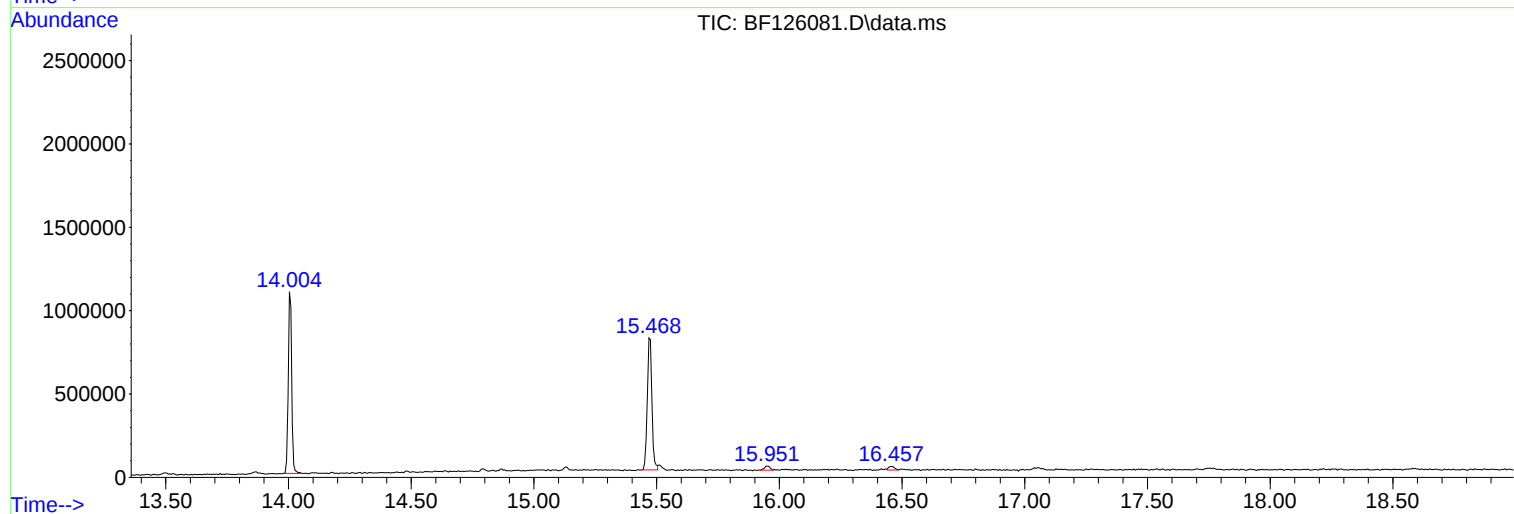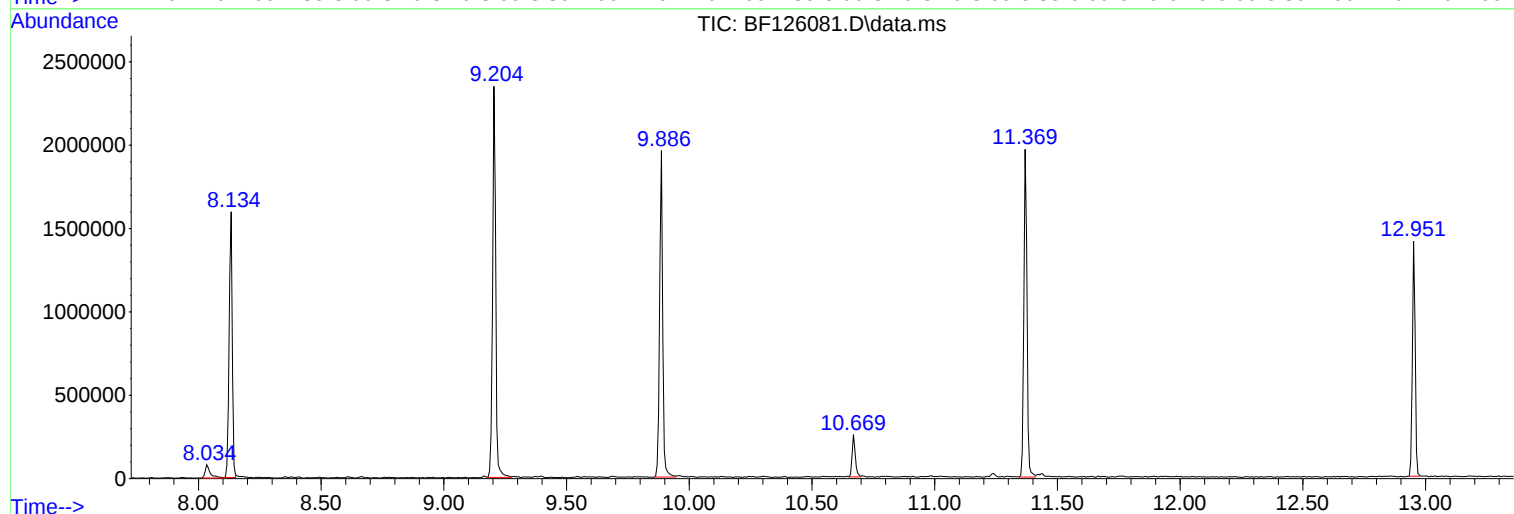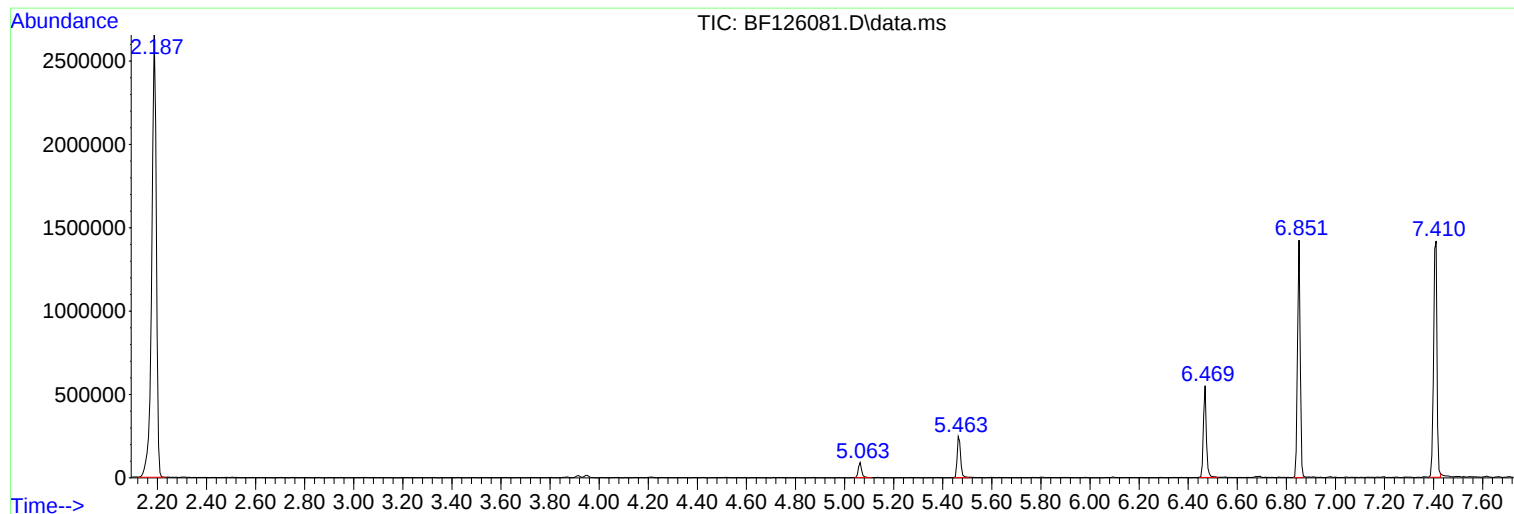

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110921\
Data File : BF126081.D
Acq On : 9 Nov 2021 14:19
Operator : JU/CG
Sample : M4567-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BASEMENT










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.187	63.39 ng	3499370	1,4-Dichlorobenzene-d4	6.851

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40
3			1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	23
4			Silane, tetramethyl-	88	C4H12Si	000075-76-3	17
5			N-Ethylformamide	73	C3H7NO	000627-45-2	9

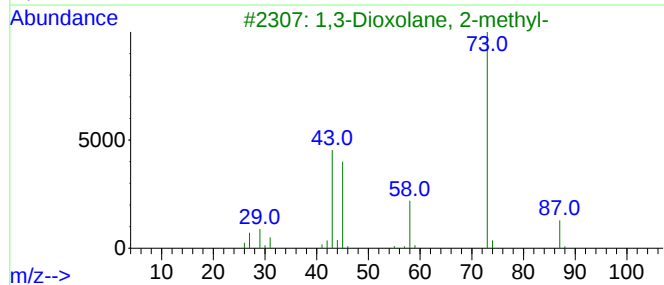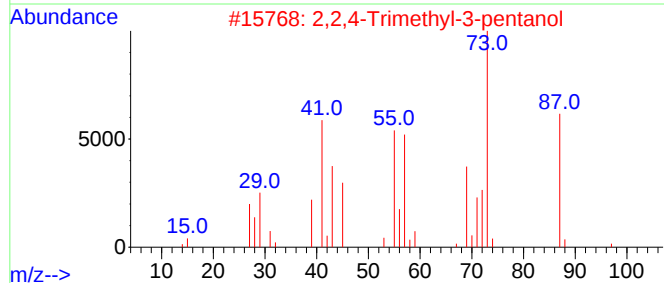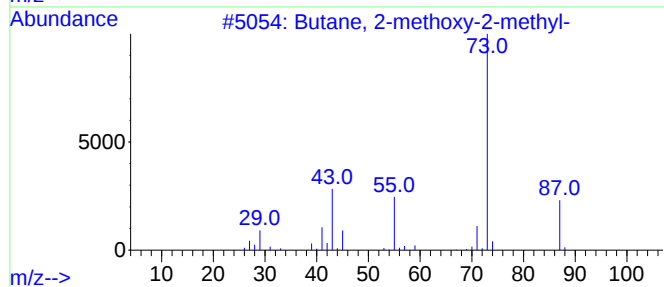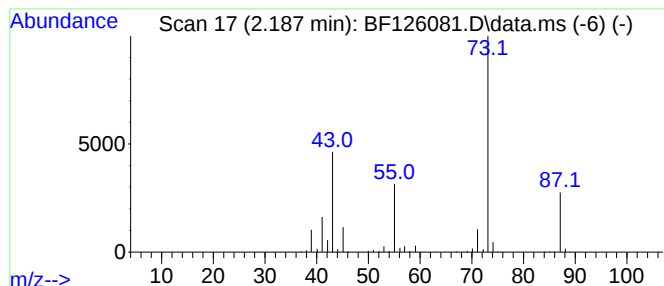

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110921\
Data File : BF126081.D
Acq On : 9 Nov 2021 14:19
Operator : JU/CG
Sample : M4567-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BASEMENT

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.187	63.4	ng	3499370	1	6.851	1104050	20.0