


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110921\
 Data File : BF126082.D
 Acq On : 9 Nov 2021 15:09
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 03 17:21:25 2021

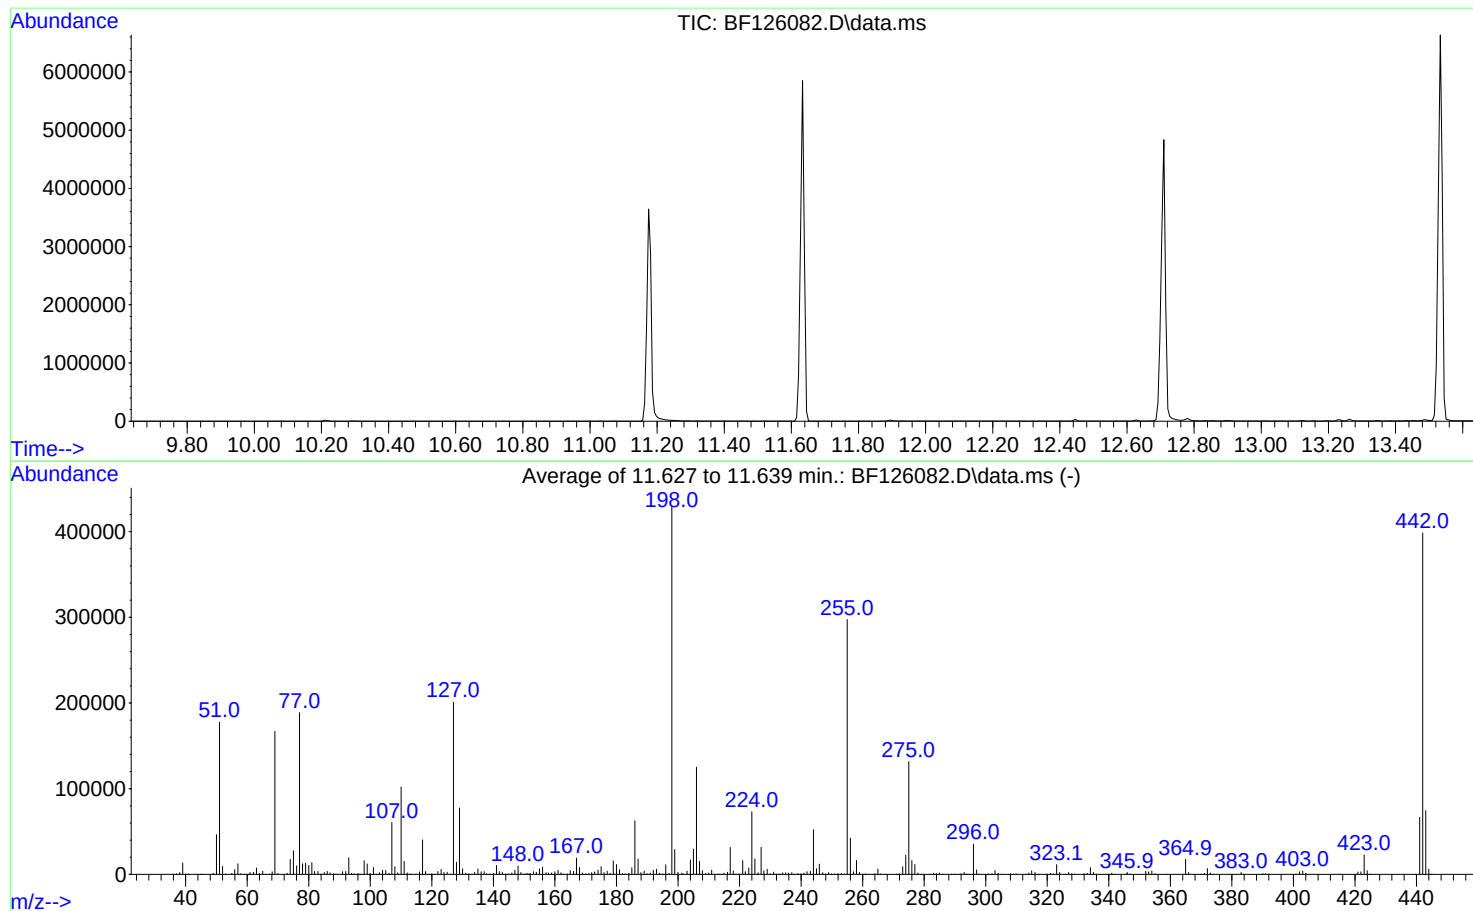




AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.4	177613	PASS
68	69	0.00	2	1.8	3087	PASS
69	198	0.00	100	38.9	166883	PASS
70	69	0.00	2	0.6	948	PASS
127	198	10	80	46.8	200896	PASS
197	198	0.00	2	0.3	1150	PASS
198	198	100	100	100.0	429312	PASS
199	198	5	9	6.7	28968	PASS
275	198	10	60	30.7	131659	PASS
365	198	1	100	4.1	17512	PASS
441	198	0.01	100	15.5	66421	PASS
442	442	50	100	100.0	398571	PASS
443	442	15	24	18.6	74251	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110921\
 Data File : BF126082.D
 Acq On : 9 Nov 2021 15:09
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Nov 09 15:44:35 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 03 17:21:25 2021
 Response via : Initial Calibration

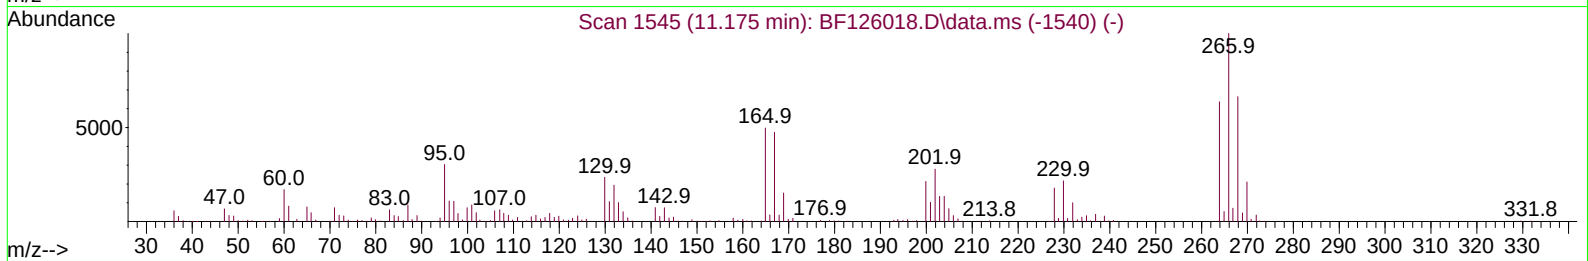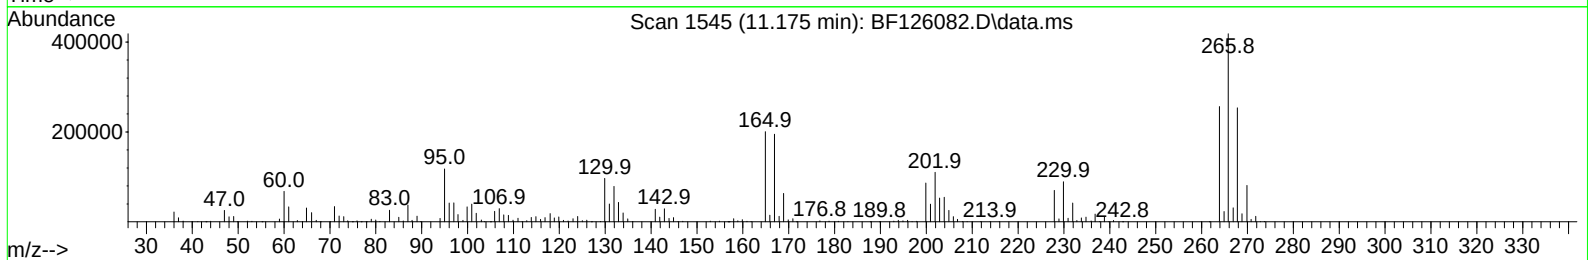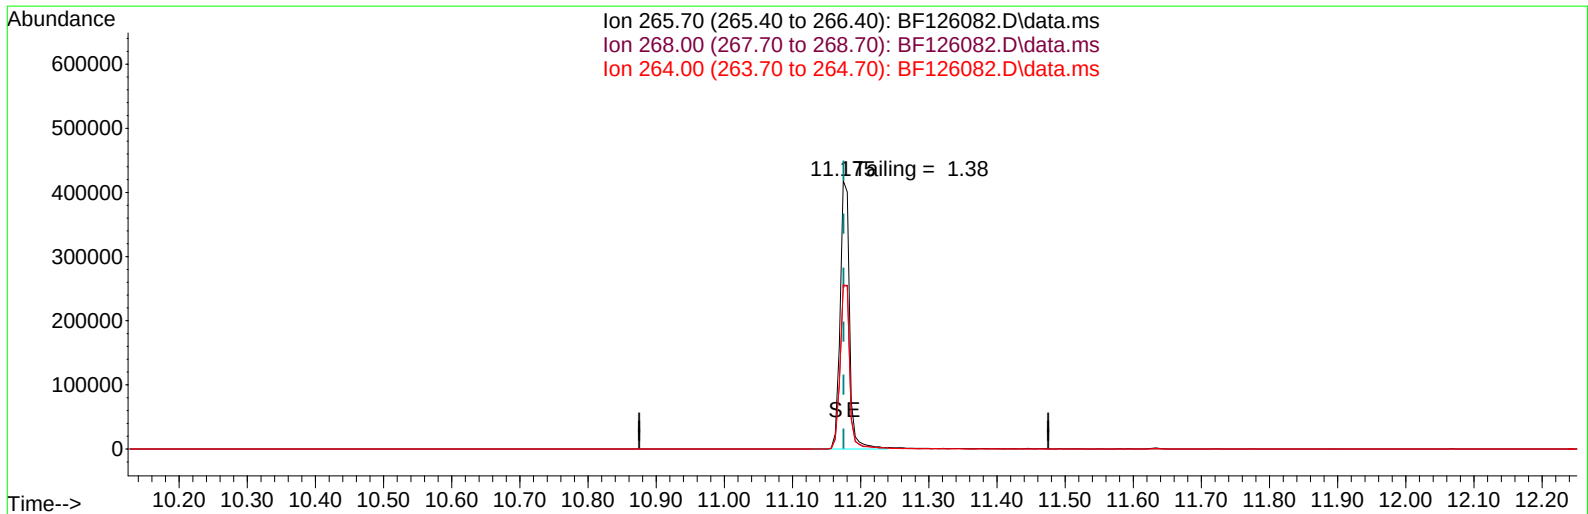

TIC: BF126082.D\data.ms

(70) Pentachlorophenol (C)

11.175min (-0.000) 504490.54 ng




response 402438

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	60.65
264.00	69.90	61.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110921\
Data File : BF126082.D
Acq On : 9 Nov 2021 15:09
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 09 15:44:35 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 03 17:21:25 2021
Response via : Initial Calibration

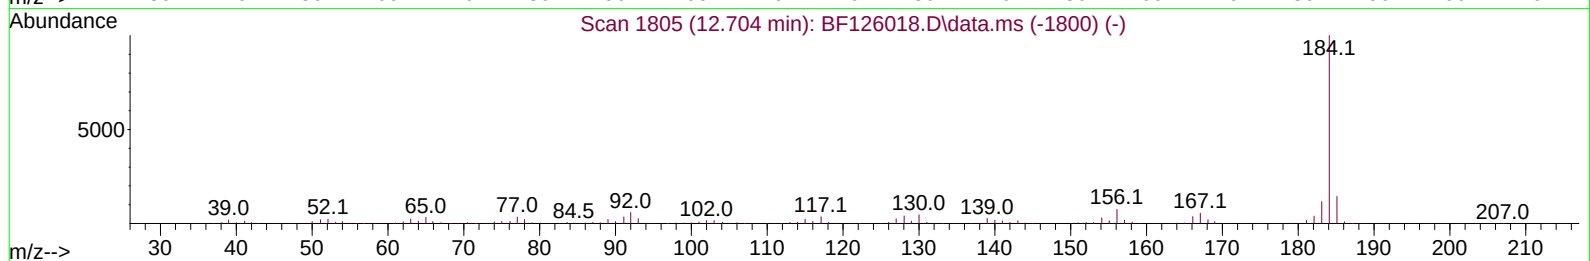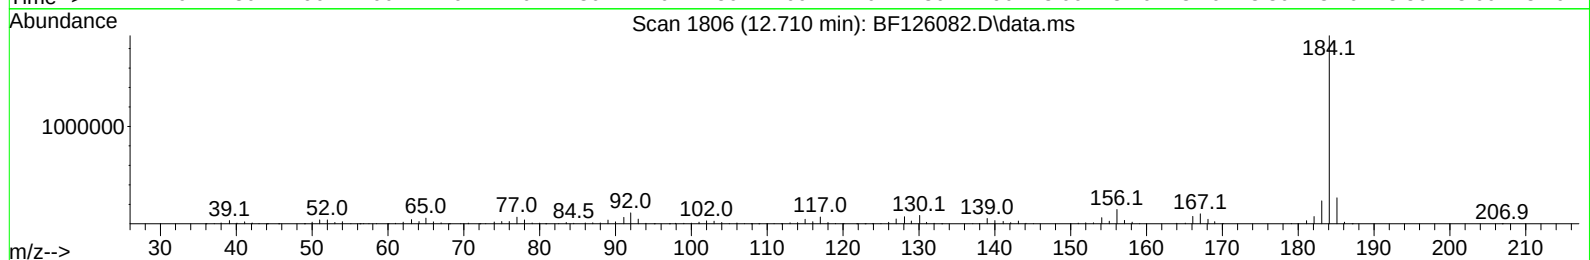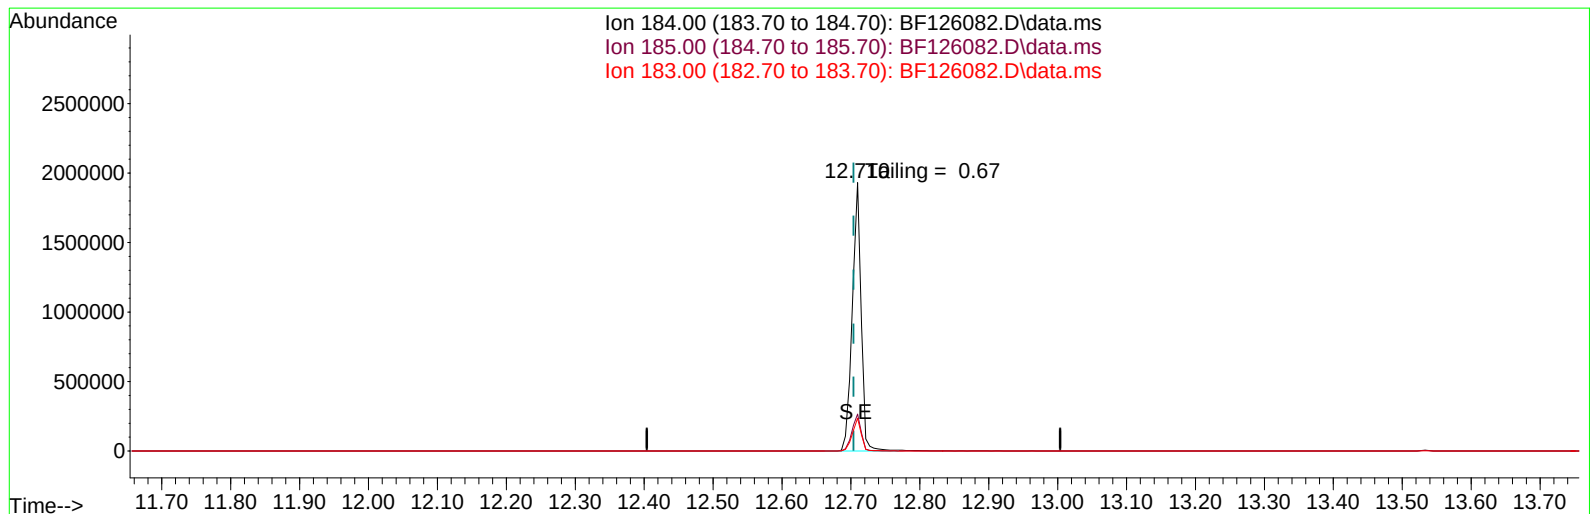

TIC: BF126082.D\data.ms

(77) Benzidine

12.710min (+ 0.006) 3230.33 ng m

response 1734478

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	13.81
183.00	10.10	12.23#
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/9/2021	BNA_F	BF126082.D
Compound Name	Response	Retention Time
DDT	1117331	13.53
DDD	4995	13.23
DDE	1906	12.89
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6901	1124232	0.61