
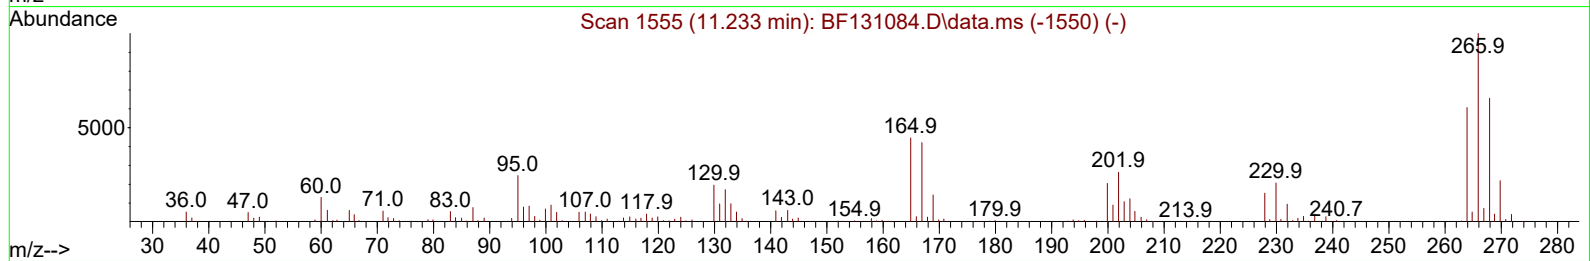
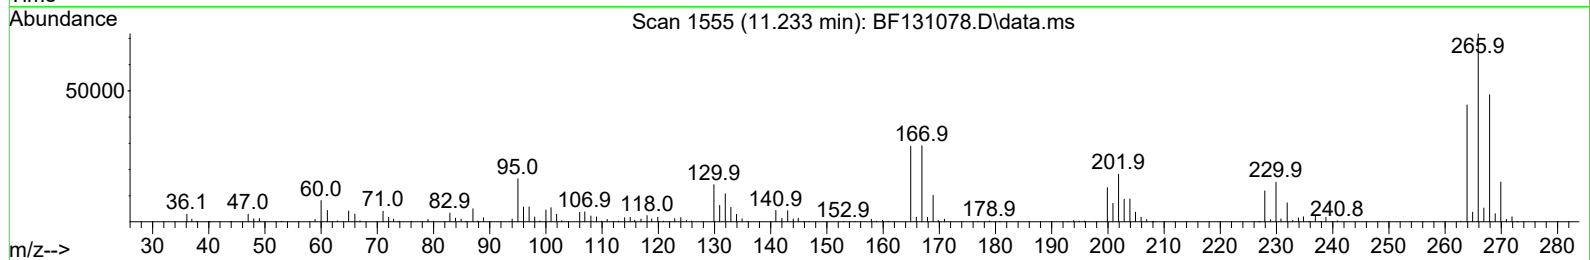


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110922\
Data File : BF131078.D
Acq On : 09 Nov 2022 10:26
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 09 17:28:00 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 09 17:24:26 2022
Response via : Initial Calibration

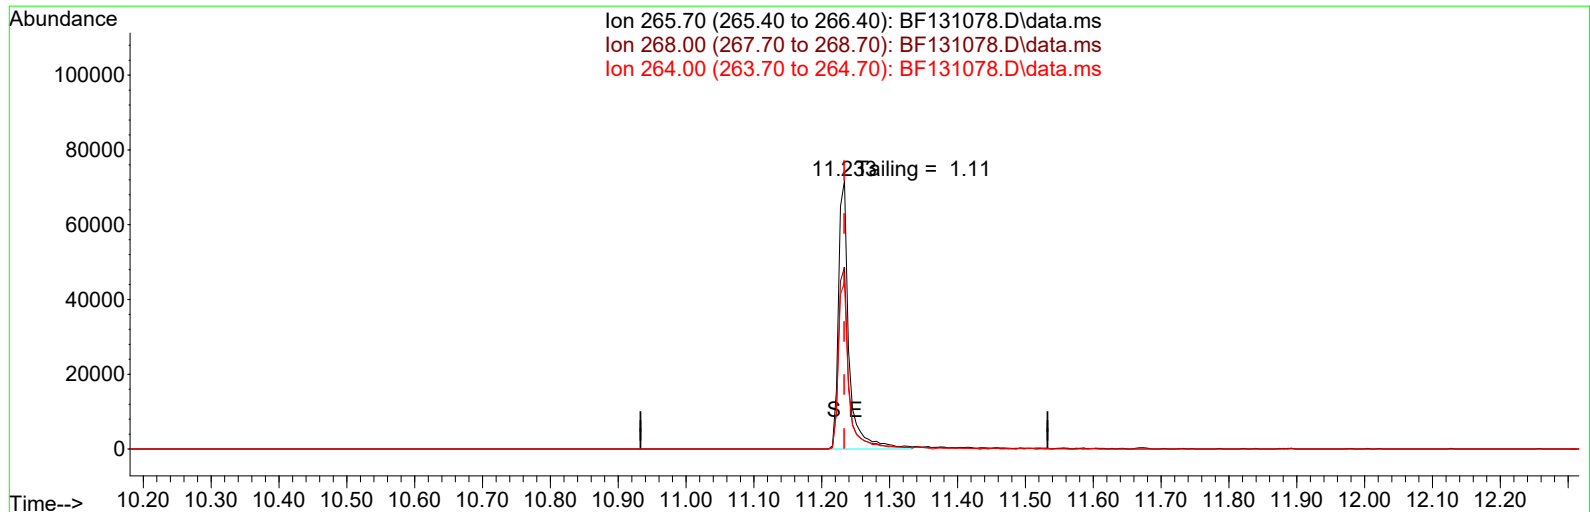

TIC: BF131078.D\data.ms

(70) Pentachlorophenol (C)




11.233min (+ 0.000) 20398.69 ng

response 76948

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.60	67.61
264.00	60.70	62.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110922\
Data File : BF131078.D
Acq On : 09 Nov 2022 10:26
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 09 17:28:00 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 09 17:24:26 2022
Response via : Initial Calibration

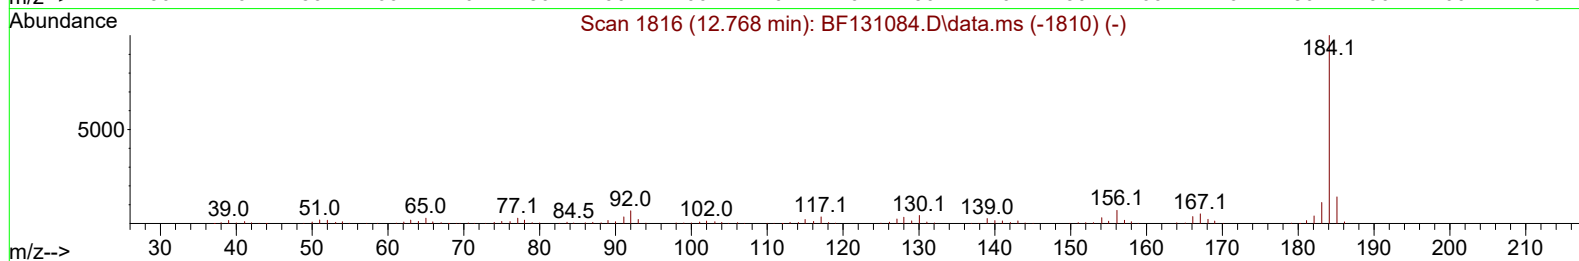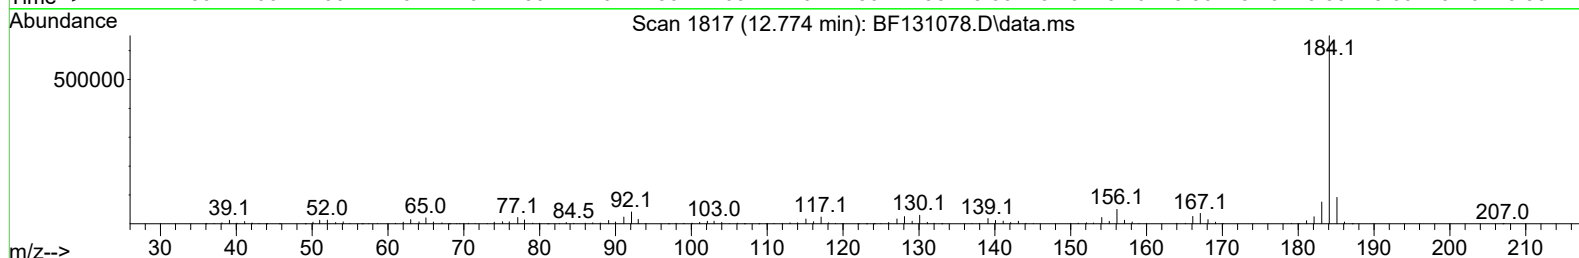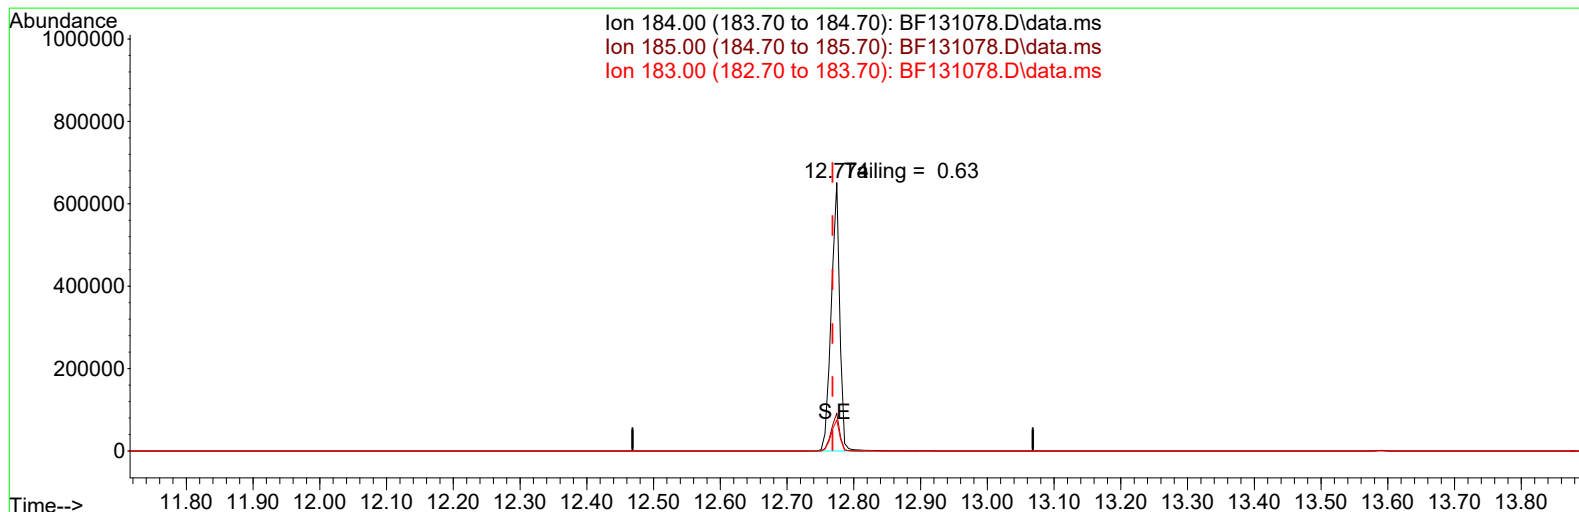

TIC: BF131078.D\data.ms

(77) Benzidine

12.774min (+ 0.006) 0.00 ng

response 579522

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.06
183.00	11.20	11.60
0.00	0.00	0.00