
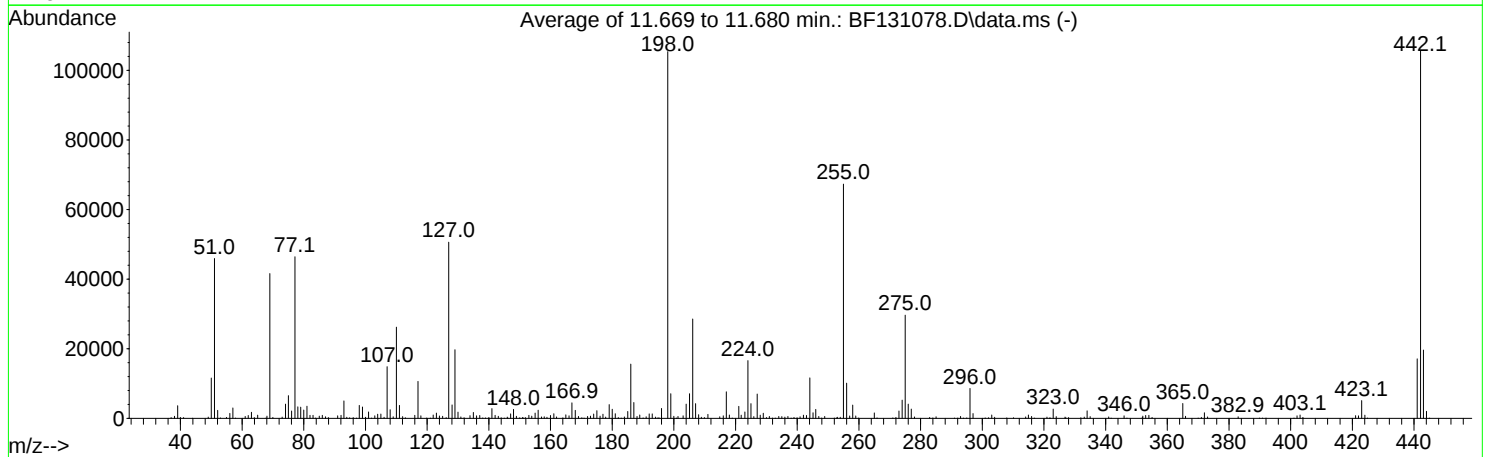


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110922\
 Data File : BF131078.D
 Acq On : 09 Nov 2022 10:26
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Nov 10 04:15:17 2022

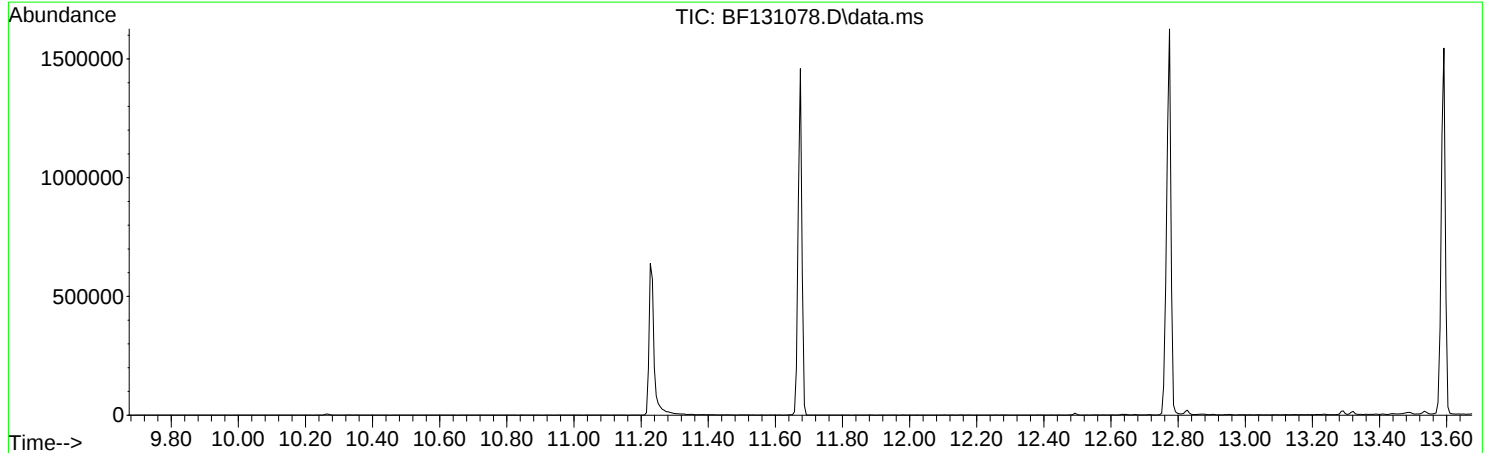




AutoFind: Scans 1629, 1630, 1631; Background Corrected with Scan 1624

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.6	45905	PASS
68	69	0.00	2	1.5	627	PASS
69	198	0.00	100	39.5	41582	PASS
70	69	0.00	2	0.7	279	PASS
127	198	10	80	48.0	50611	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	105347	PASS
199	198	5	9	6.7	7051	PASS
275	198	10	60	28.1	29653	PASS
365	198	1	100	4.1	4269	PASS
441	198	0.01	100	16.2	17065	PASS
442	442	50	100	100.0	105712	PASS
443	442	15	24	18.5	19597	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110922\
 Data File : BF131078.D
 Acq On : 09 Nov 2022 10:26
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Nov 09 17:28:00 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 09 17:24:26 2022
 Response via : Initial Calibration

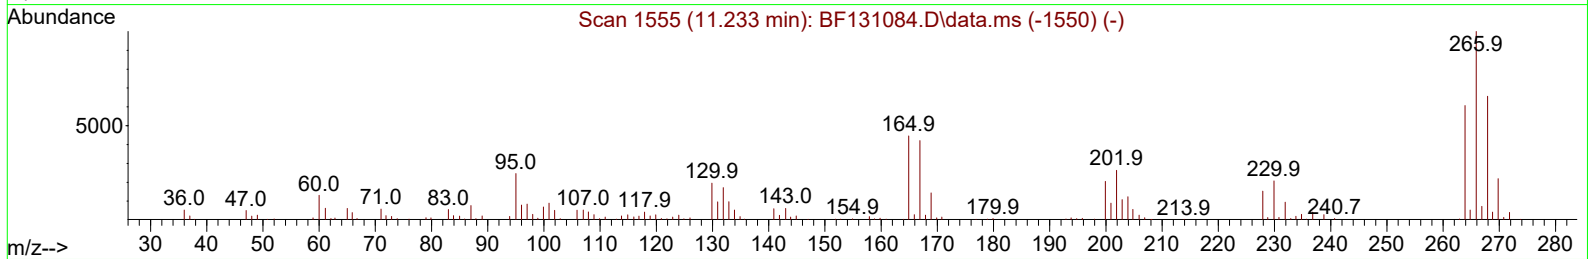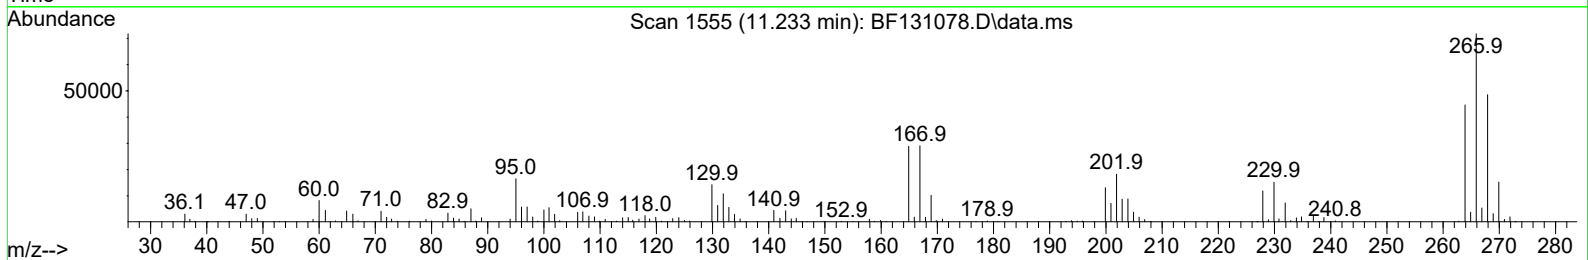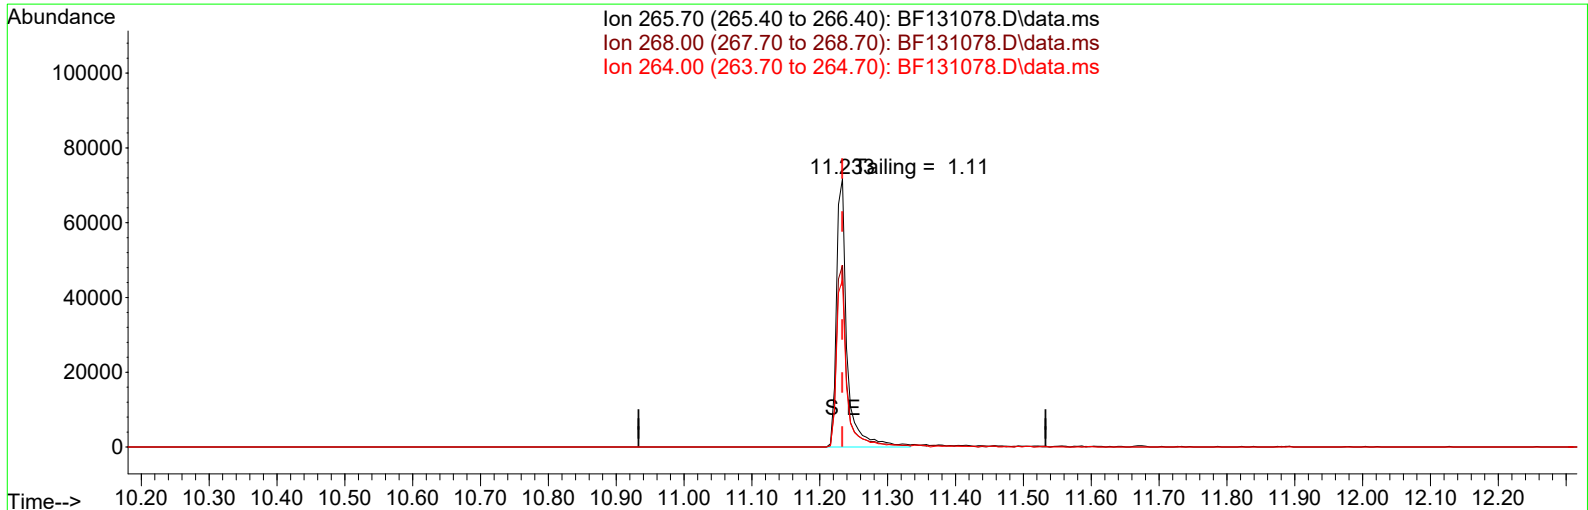

TIC: BF131078.D\data.ms

(70) Pentachlorophenol (C)

11.233min (+ 0.000) 20398.69 ng


response 76948

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.60	67.61
264.00	60.70	62.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110922\
Data File : BF131078.D
Acq On : 09 Nov 2022 10:26
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 09 17:28:00 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 09 17:24:26 2022
Response via : Initial Calibration

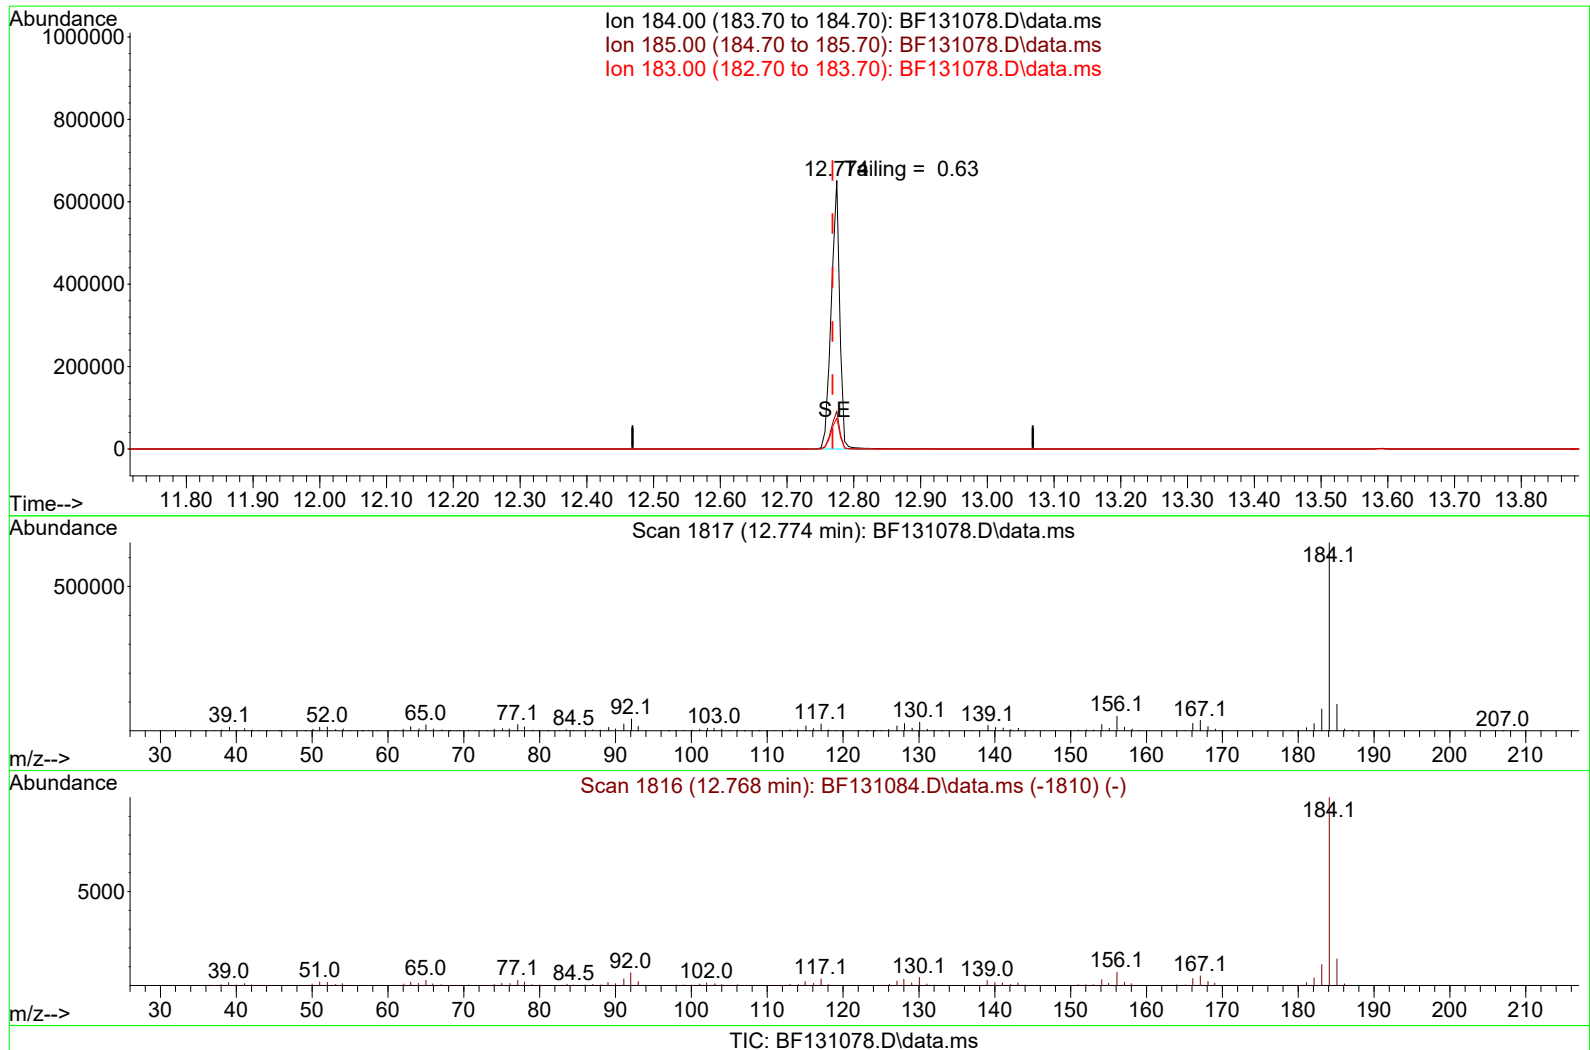

TIC: BF131078.D\data.ms

(77) Benzidine

12.774min (+ 0.006) 0.00 ng

response 579522

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.06
183.00	11.20	11.60
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/9/2022	BNA_F	<u>BF131078.D</u>
Compound Name	Response	Retention Time
DDT	247475	13.592
DDD	5672	13.292
DDE	469	12.951
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6141	253616	2.42

Instrument :
BNA_F
ClientSampleId :
DFTPP