
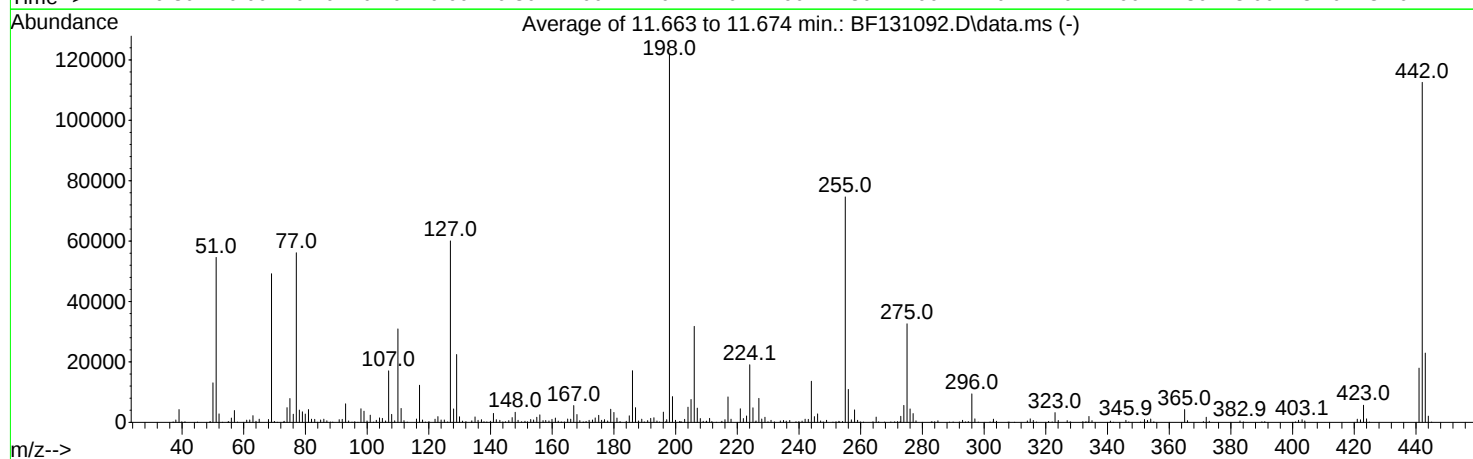


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110922\
 Data File : BF131092.D
 Acq On : 09 Nov 2022 17:56
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Nov 10 04:15:17 2022

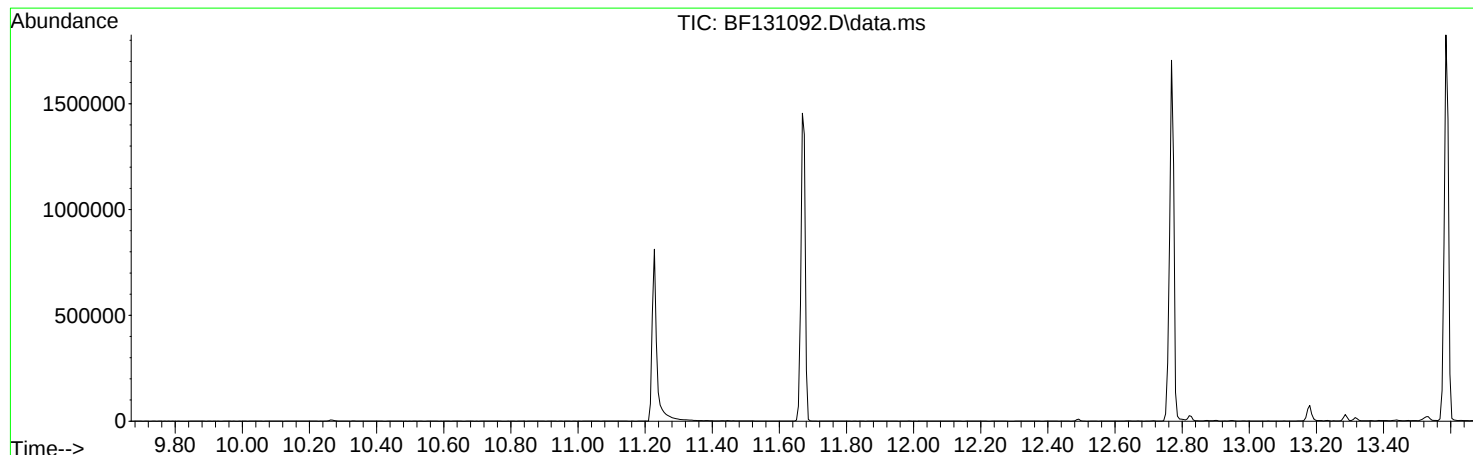




AutoFind: Scans 1628, 1629, 1630; Background Corrected with Scan 1623

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.8	54611	PASS
68	69	0.00	2	1.9	928	PASS
69	198	0.00	100	40.4	49195	PASS
70	69	0.00	2	0.6	300	PASS
127	198	10	80	49.3	60069	PASS
197	198	0.00	2	0.7	902	PASS
198	198	100	100	100.0	121824	PASS
199	198	5	9	7.0	8523	PASS
275	198	10	60	26.8	32643	PASS
365	198	1	100	3.5	4230	PASS
441	198	0.01	100	14.7	17918	PASS
442	442	50	100	100.0	112571	PASS
443	442	15	24	20.4	22923	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110922\
Data File : BF131092.D
Acq On : 09 Nov 2022 17:56
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 10 07:48:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 10 04:15:17 2022
Response via : Initial Calibration

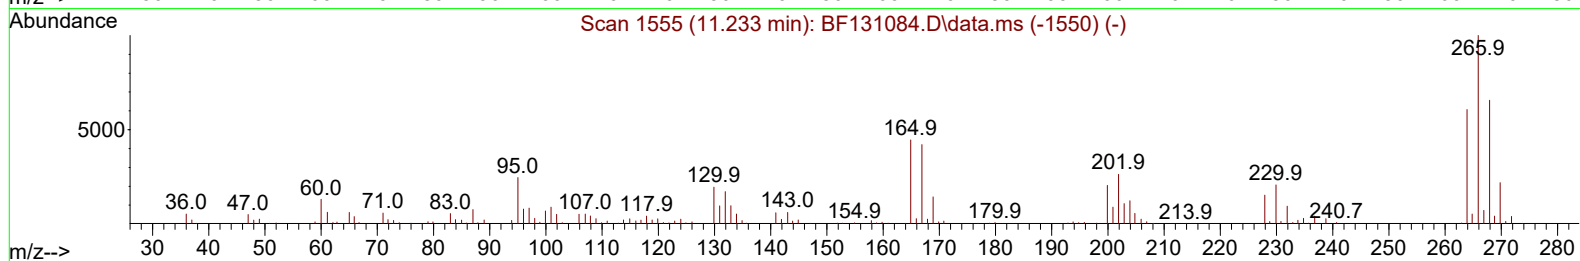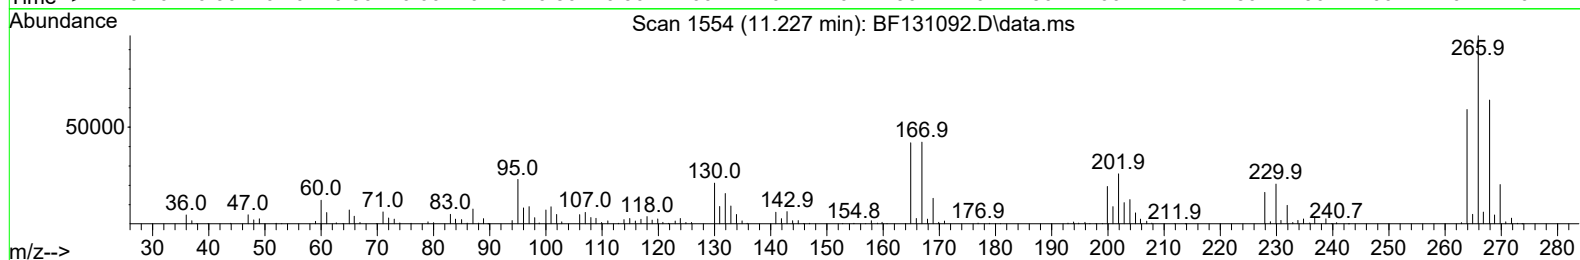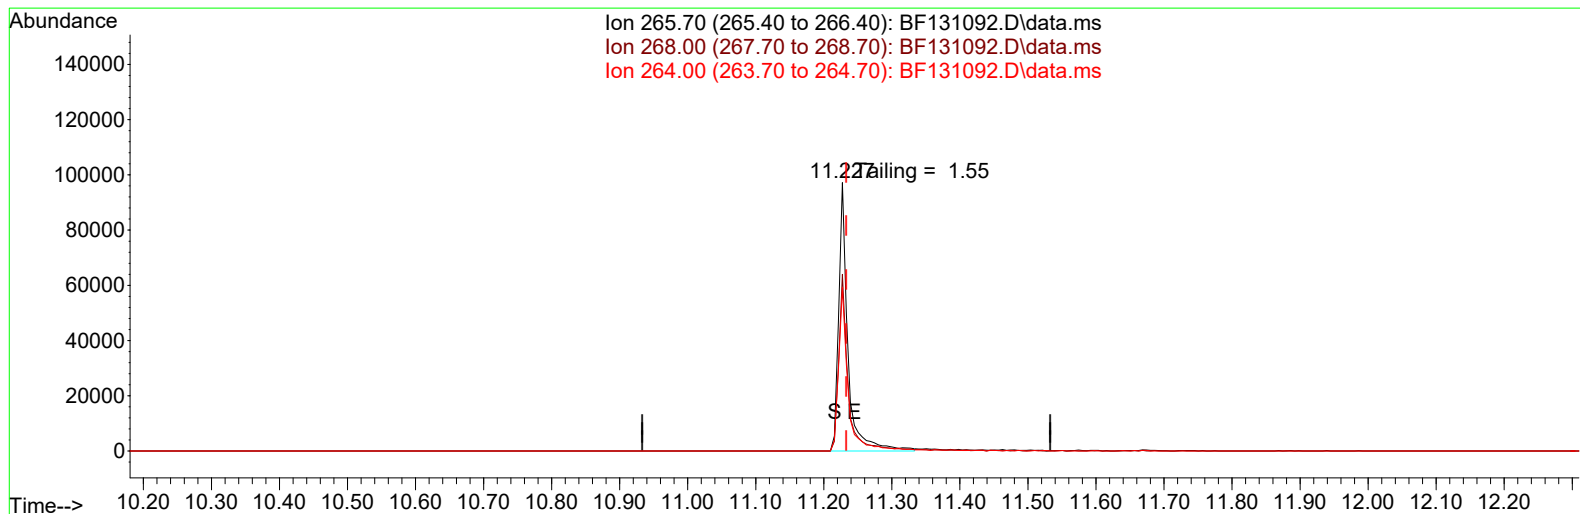

TIC: BF131092.D\data.ms

(70) Pentachlorophenol (C)

11.227min (-0.006) 28789.21 ng




response 90808

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.60	65.86
264.00	60.70	60.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110922\
Data File : BF131092.D
Acq On : 09 Nov 2022 17:56
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 10 07:48:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 10 04:15:17 2022
Response via : Initial Calibration

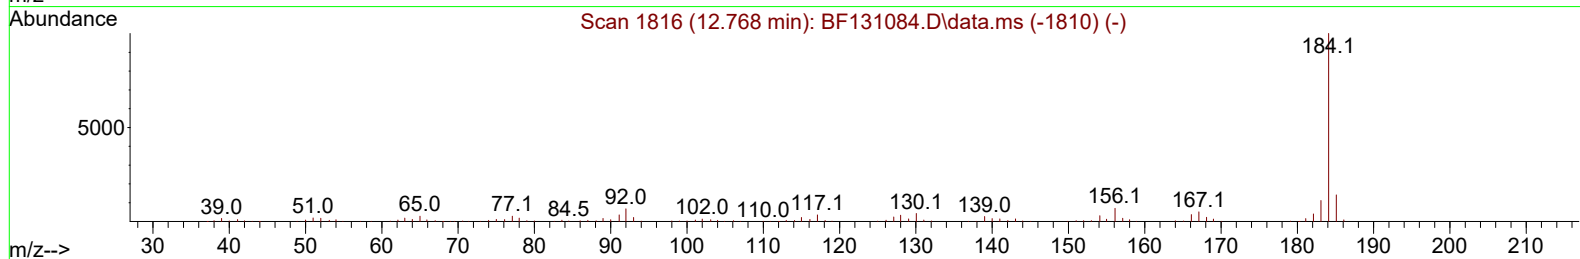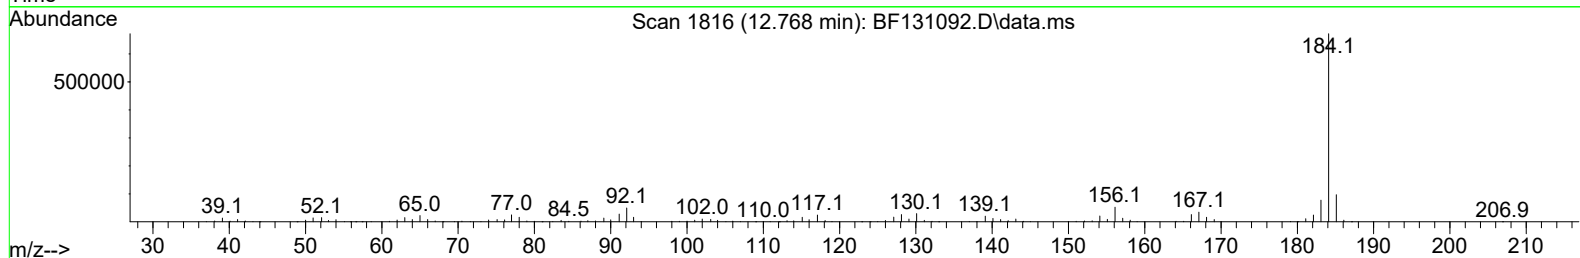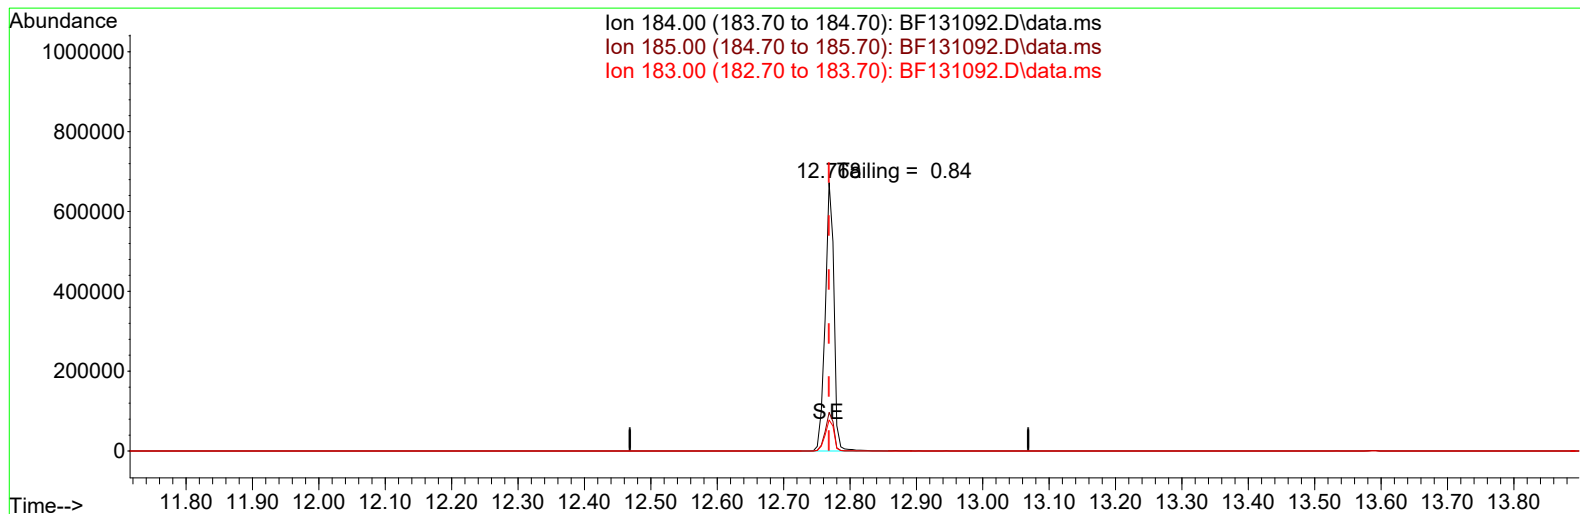

TIC: BF131092.D\data.ms

(77) Benzidine

12.768min (+ 0.000) 0.00 ng

response 614212

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.38
183.00	11.20	11.55
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/9/2022	BNA_F	<u>BF131092.D</u>
Compound Name	Response	Retention Time
DDT	312661	13.586
DDD	8952	13.286
DDE	537	12.945
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9489	322150	2.95

Instrument :
BNA_F
ClientSampleId :
DFTPP