


Data Path : Z:\HPCHEM1\BNA F\Data\BF111015\
 Data File : BF082868.D
 Acq On : 10 Nov 2015 14:07
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Nov 07 02:32:49 2015

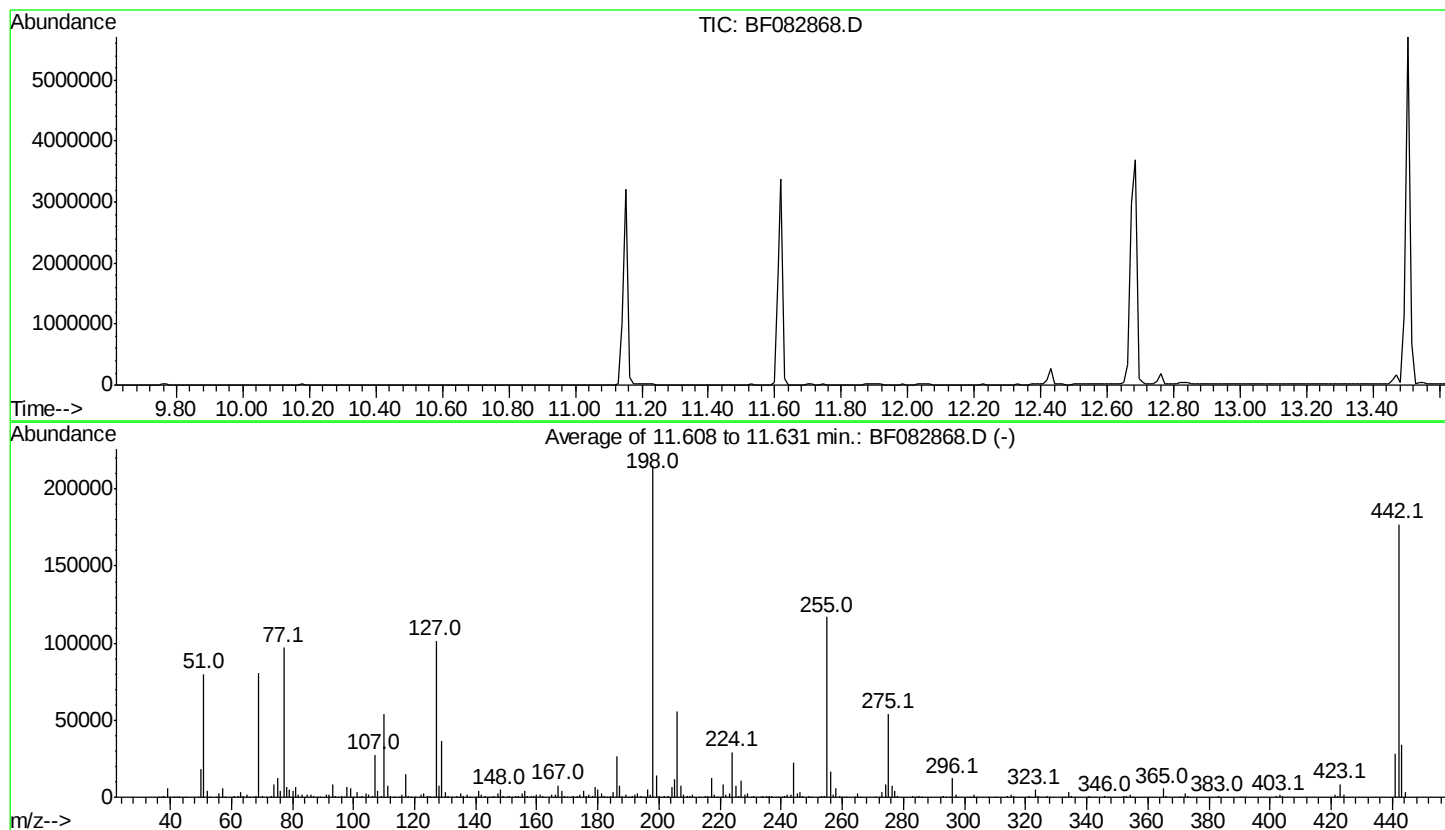

AutoFind: Scans 833, 834, 835; Background Corrected with Scan 829

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.1	79865	PASS
68	69	0.00	2	1.5	1195	PASS
69	198	0.00	100	37.3	80322	PASS
70	69	0.00	2	0.6	472	PASS
127	198	10	80	47.2	101657	PASS
197	198	0.00	2	0.6	1354	PASS
198	198	100	100	100.0	215213	PASS
199	198	5	9	6.8	14540	PASS
275	198	10	60	25.2	54179	PASS
365	198	1	100	2.7	5806	PASS
441	442	0.01	24	16.1	28567	PASS
442	198	50	100	82.3	177122	PASS
443	442	15	24	19.3	34135	PASS